

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102419\
 Data File : VU035476.D
 Acq On : 24 Oct 2019 22:15
 Operator : JC/SP
 Sample : K5509-08DL 10X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0G48DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	5	10	18	rBV3	8683	9088	1.16%	0.137%
2	1.494	41	48	63	rVB4	6606	15982	2.04%	0.241%
3	1.616	79	86	96	rVB2	74446	84743	10.84%	1.280%
4	1.790	135	140	148	rVB2	8594	11160	1.43%	0.169%
5	1.935	177	185	196	rVB	65353	83872	10.73%	1.267%
6	2.597	380	391	402	rBV	100912	165775	21.20%	2.504%
7	2.671	403	414	435	rVV	183318	318006	40.67%	4.803%
8	2.816	446	459	491	rBV	376044	765922	97.96%	11.569%
9	3.083	532	542	560	rVB	20490	41625	5.32%	0.629%
10	3.234	575	589	610	rVB	41787	96799	12.38%	1.462%
11	4.703	1026	1046	1080	rBV2	166497	485770	62.13%	7.337%
12	5.115	1159	1174	1198	rBV	121992	277264	35.46%	4.188%
13	5.771	1358	1378	1396	rBV3	217477	566024	72.39%	8.549%
14	6.292	1525	1540	1565	rBV	256419	501217	64.10%	7.570%
15	6.584	1618	1631	1643	rBV6	16137	31648	4.05%	0.478%
16	6.735	1664	1678	1700	rBV2	156249	306971	39.26%	4.637%
17	7.603	1936	1948	1966	rBV	63036	116497	14.90%	1.760%
18	7.935	2037	2051	2065	rBV	206321	367104	46.95%	5.545%
19	8.005	2067	2073	2088	rVB	9184	18116	2.32%	0.274%
20	8.214	2127	2138	2159	rBV2	37113	70456	9.01%	1.064%
21	8.684	2269	2284	2331	rBV	208424	781902	100.00%	11.810%
22	8.986	2364	2378	2389	rBV3	4949	12240	1.57%	0.185%
23	9.449	2507	2522	2544	rBV	325661	621748	79.52%	9.391%
24	10.787	2925	2938	2961	rBV	126077	227385	29.08%	3.434%
25	11.844	3253	3267	3284	rBV	180024	360516	46.11%	5.445%
26	12.224	3371	3385	3401	rBV	149949	282890	36.18%	4.273%


Sum of corrected areas: 6620720

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102419\
Data File : VU035476.D
Acq On : 24 Oct 2019 22:15
Operator : JC/SP
Sample : K5509-08DL 10X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0G48DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

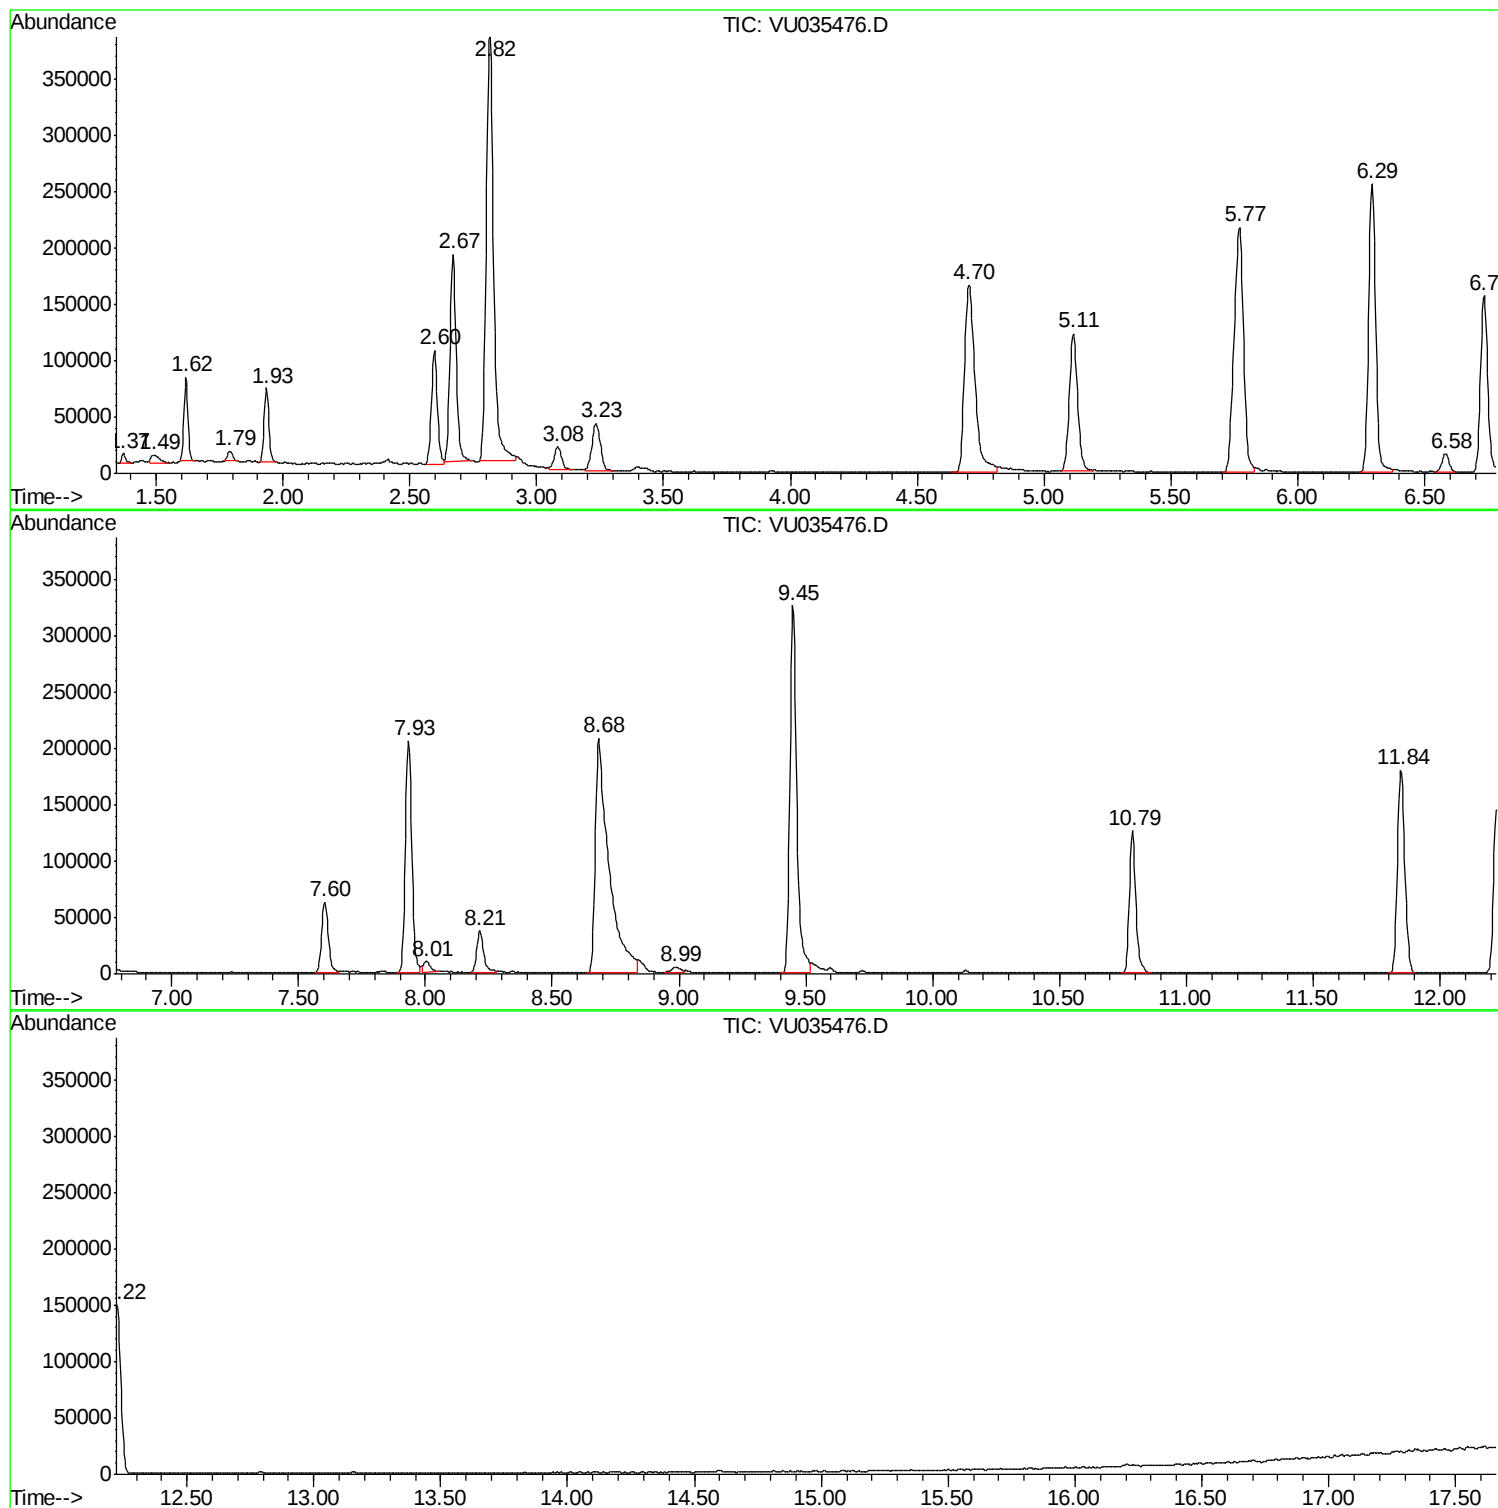

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102419\
Data File : VU035476.D
Acq On : 24 Oct 2019 22:15
Operator : JC/SP
Sample : K5509-08DL 10X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0G48DL










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.82	7.64 ug/L	765922	1,4-Difluorobenzene	6.29

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	83
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4		Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

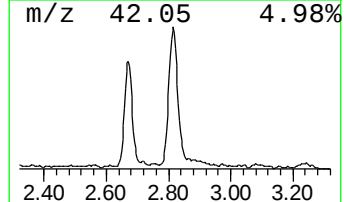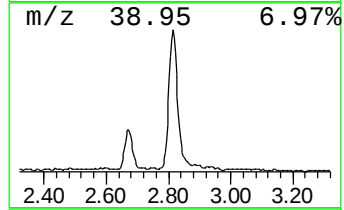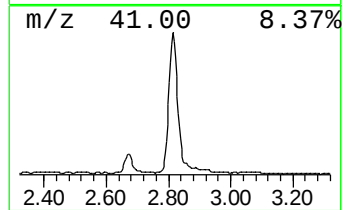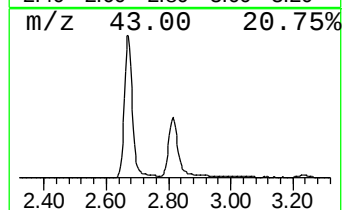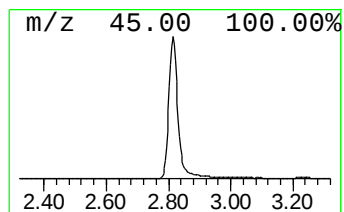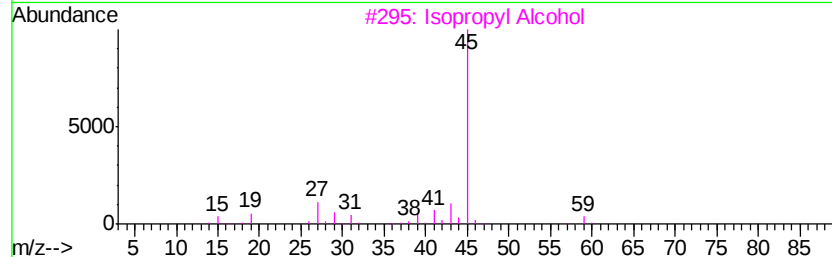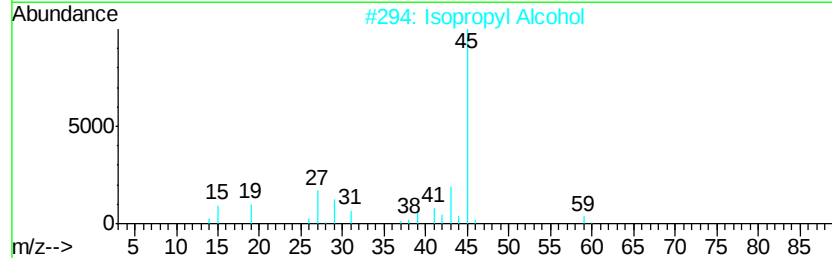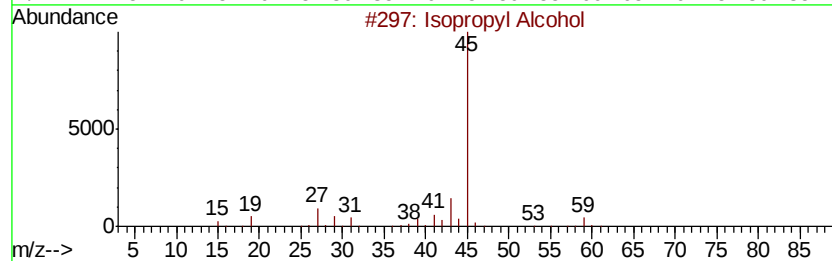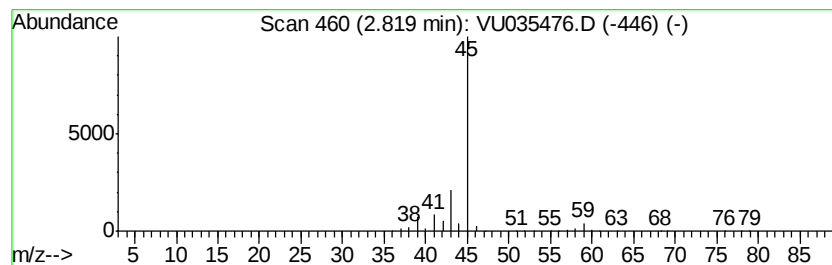

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102419\
Data File : VU035476.D
Acq On : 24 Oct 2019 22:15
Operator : JC/SP
Sample : K5509-08DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0G48DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.82	7.6	ug/L	765922	1	6.29	501217	5.0