


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102419\
Data File : VU035452.D
Acq On : 24 Oct 2019 11:22
Operator : JC/SP
Sample : BFB26
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 25 07:04:30 2019

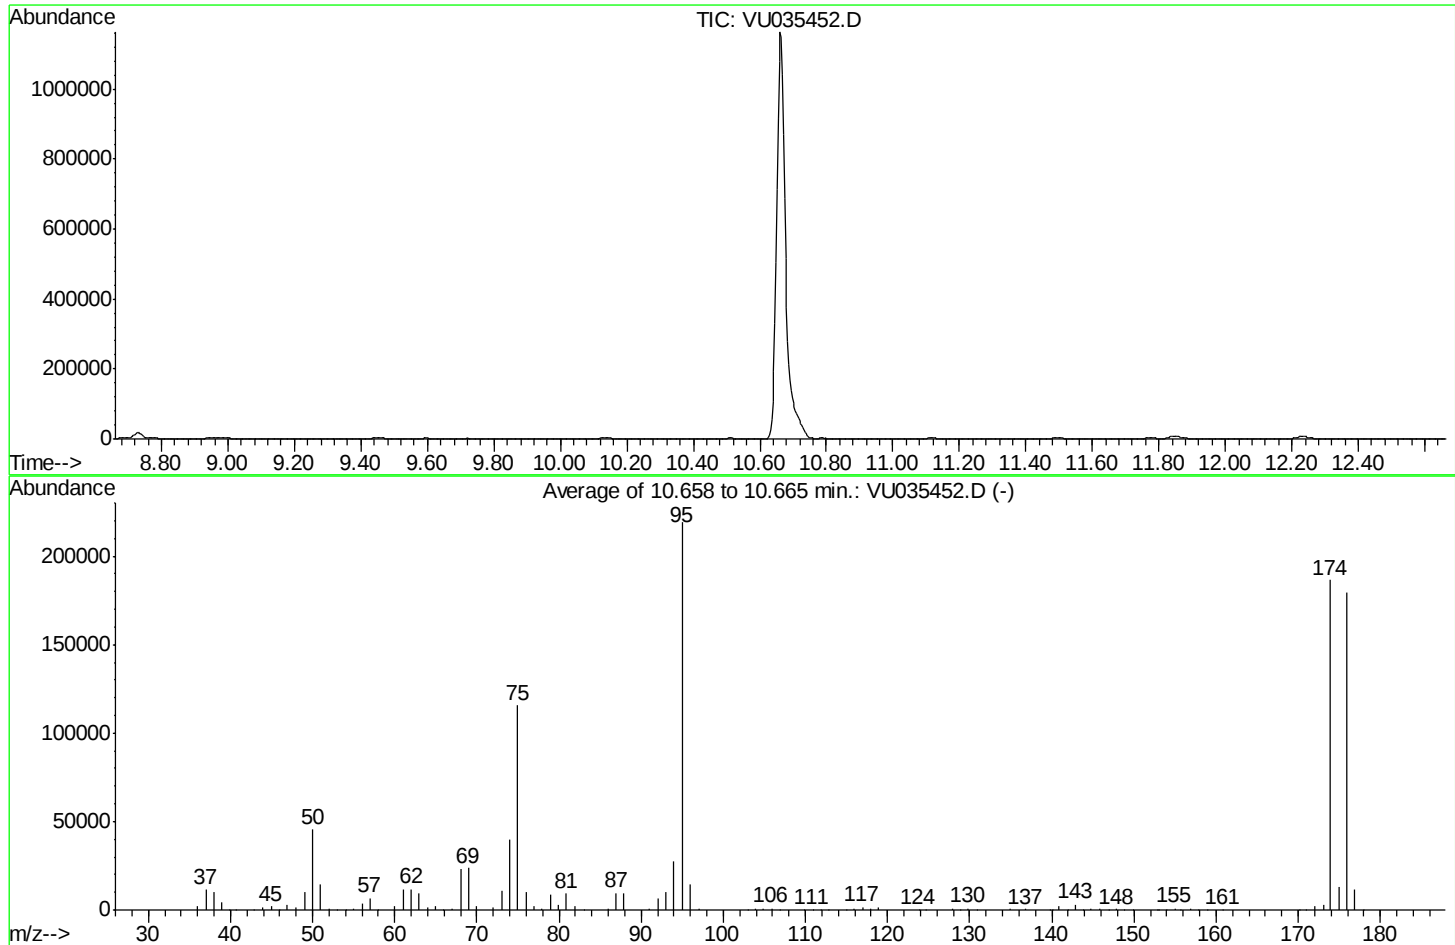

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	45416	PASS
75	95	30	80	52.8	115714	PASS
95	95	100	100	100.0	219136	PASS
96	95	5	9	6.7	14658	PASS
173	174	0.00	2	1.4	2604	PASS
174	95	50	120	85.1	186496	PASS
175	174	5	9	7.1	13234	PASS
176	174	95	101	96.2	179477	PASS
177	176	5	9	6.7	11938	PASS

m/z	Abundance
36.00	2170.0
37.00	11273.0
38.00	9397.0
39.00	4520.0
40.00	443.0
40.70	104.0
42.80	186.0
44.00	2125.0
45.00	1904.0
45.90	422.0
46.90	2775.0
48.00	1361.0
49.00	9997.0
50.00	43800.0
51.00	13980.0
51.90	555.0
53.00	281.0
55.00	700.0
56.00	3575.0
57.00	6737.0
57.90	236.0
60.00	2407.0
61.00	11464.0
62.00	11508.0
63.00	9267.0
64.00	1563.0
65.00	1951.0
66.00	164.0
67.00	530.0
68.00	22320.0
69.00	22168.0
70.00	1886.0
72.00	1521.0
73.00	11190.0
74.00	37840.0
75.00	111160.0
76.00	9601.0
77.00	1803.0
78.00	865.0
78.90	8585.0
79.90	2719.0
80.90	8839.0
82.00	2072.0
83.10	278.0
86.00	442.0
87.00	9356.0
87.90	8886.0
91.00	830.0
92.00	6774.0
93.00	9405.0
94.00	25784.0
95.00	209984.0
96.00	14594.0
97.00	389.0
102.90	103.0
103.90	864.0
104.90	377.0
105.90	978.0
106.90	221.0
109.80	135.0
110.90	242.0
111.80	140.0
112.90	165.0
114.90	300.0
115.90	973.0
116.90	1560.0
117.90	1104.0
118.90	1483.0
123.80	105.0
127.90	767.0
128.90	380.0
129.90	805.0
130.90	319.0
134.80	433.0
136.80	412.0
140.00	194.0
140.90	2302.0
141.90	335.0
142.90	2756.0
143.70	176.0
144.80	775.0
145.80	367.0
146.90	103.0
147.90	719.0
148.70	123.0
149.70	192.0
152.80	100.0
153.80	108.0
155.00	748.0
155.70	161.0
156.90	396.0
157.80	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

158.90	322.0
160.80	262.0
170.90	309.0
171.90	2505.0
173.10	2405.0
173.90	174464.0
174.90	12777.0
175.90	167232.0
176.90	11233.0
177.90	343.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	2201.0
37.00	11650.0
38.00	10150.0
39.00	4607.0
39.90	399.0
42.80	162.0
44.00	2200.0
45.00	2045.0
46.00	332.0
47.00	2705.0
48.00	1455.0
49.00	10771.0
50.00	46840.0
51.00	14525.0
52.00	534.0
53.00	307.0
55.00	778.0
56.00	3786.0
57.00	7056.0
57.90	242.0
60.00	2626.0
61.00	12180.0
62.00	12161.0
63.00	9258.0
64.00	1563.0
65.00	2068.0
66.00	147.0
67.10	658.0
68.00	23936.0
69.00	24376.0
69.90	2077.0
72.00	1520.0
73.00	11358.0
74.00	40808.0
75.00	119048.0
76.00	10178.0
77.00	1947.0
78.00	856.0
78.90	9208.0
79.90	2816.0
80.90	9463.0
81.90	2167.0
83.10	225.0
86.00	421.0
87.00	9904.0
87.90	9431.0
91.00	784.0
92.00	7022.0
93.00	10131.0
94.00	28024.0
95.00	225600.0
96.00	15127.0
97.00	428.0
102.90	102.0
103.90	928.0
104.90	451.0
105.90	974.0
106.90	239.0
109.90	138.0
110.90	256.0
111.90	188.0
112.80	214.0
114.90	327.0
115.90	1086.0
116.90	1704.0
117.90	1056.0
118.90	1479.0
123.80	156.0
127.90	856.0
128.90	376.0
129.90	844.0
130.90	281.0
134.80	449.0
136.80	506.0
140.00	183.0
140.90	2363.0
141.90	304.0
142.90	3184.0
143.80	198.0
144.80	763.0
145.80	443.0
146.90	111.0
147.90	739.0
148.80	166.0
149.80	213.0
153.00	123.0
153.80	125.0
154.90	833.0
155.70	146.0
156.90	493.0
157.80	194.0
158.90	356.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

160.80	240.0
170.10	137.0
171.00	385.0
172.00	2633.0
173.10	2687.0
173.90	192256.0
174.90	13591.0
175.90	184768.0
176.90	12306.0
177.90	379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	2152.0
37.00	11081.0
38.00	10080.0
39.00	4225.0
39.90	338.0
42.80	145.0
44.00	2181.0
45.00	1984.0
46.00	246.0
47.00	2711.0
48.00	1376.0
49.00	10597.0
50.00	45608.0
51.00	14154.0
51.90	493.0
52.90	272.0
54.00	108.0
55.00	735.0
56.00	3627.0
57.00	6713.0
58.00	270.0
60.00	2567.0
61.00	11884.0
62.00	12040.0
63.00	8773.0
63.90	1295.0
65.00	2008.0
65.90	152.0
67.10	686.0
68.00	23568.0
69.00	24312.0
69.90	1988.0
72.00	1320.0
73.00	10682.0
74.00	40408.0
75.00	116936.0
76.00	10151.0
77.00	1817.0
77.90	765.0
78.90	8980.0
79.90	2677.0
80.90	9327.0
81.90	2185.0
83.00	204.0
85.90	420.0
86.90	9707.0
87.90	9405.0
91.00	776.0
92.00	6639.0
93.00	9946.0
94.00	27856.0
95.00	221824.0
96.00	14253.0
97.10	451.0
103.90	934.0
104.90	448.0
105.90	970.0
106.80	223.0
109.90	129.0
110.90	260.0
111.90	252.0
112.80	261.0
114.90	297.0
115.90	1027.0
117.00	1610.0
117.90	963.0
118.90	1353.0
123.80	169.0
124.70	100.0
127.90	821.0
128.90	358.0
129.80	798.0
130.80	269.0
134.90	394.0
136.80	507.0
139.70	163.0
140.90	2340.0
141.90	241.0
142.90	3305.0
143.80	173.0
144.80	682.0
145.80	448.0
147.90	595.0
148.80	196.0
149.90	235.0
153.00	144.0
153.90	137.0
154.90	825.0
155.60	119.0
156.90	502.0
157.80	180.0
158.90	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

160.80	214.0
170.10	167.0
171.00	362.0
171.90	2504.0
173.10	2722.0
173.90	192768.0
175.00	13334.0
175.90	186432.0
176.90	12276.0
177.90	374.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Scan 2884 (10.613 min): VU035452.D
BFB26

m/z	Abundance
39.90	141.0
43.90	677.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26