


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102423\
Data File : VU055859.D
Acq On : 24 Oct 2023 08:46
Operator : MD/SY
Sample : BFB058
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB058

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Oct 25 05:19:13 2023

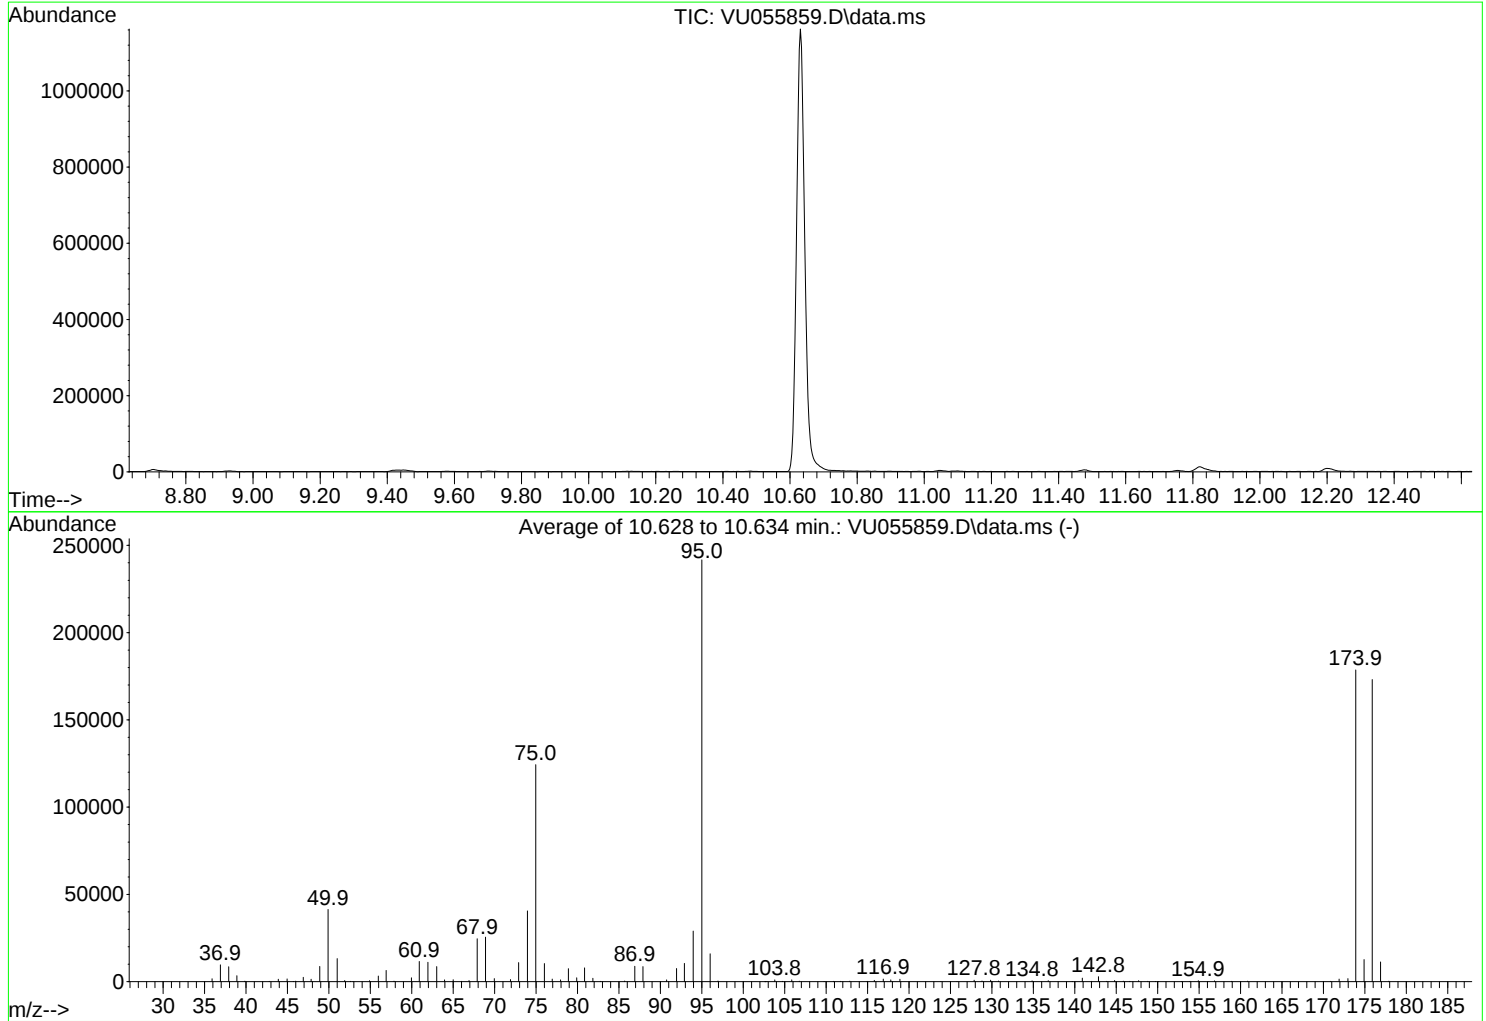

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	41387	PASS
75	95	30	80	51.4	124301	PASS
95	95	100	100	100.0	241707	PASS
96	95	5	9	6.6	15964	PASS
173	174	0.00	2	1.0	1739	PASS
174	95	50	120	73.9	178645	PASS
175	174	5	9	7.1	12685	PASS
176	174	95	101	96.9	173141	PASS
177	176	5	9	6.5	11252	PASS

m/z	Abundance
39.80	300.0
43.90	640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
35.90	1589.0
36.90	9624.0
37.90	8430.0
38.90	3406.0
39.90	505.0
42.80	182.0
43.90	1986.0
44.90	1620.0
45.70	208.0
46.10	270.0
46.90	2379.0
47.80	1457.0
48.90	8925.0
49.90	41696.0
51.00	12998.0
51.90	687.0
52.60	292.0
54.90	539.0
55.90	3124.0
56.90	6615.0
57.80	349.0
60.00	2265.0
60.90	12248.0
62.00	10316.0
63.00	8845.0
63.90	1105.0
65.00	1077.0
66.00	189.0
66.90	620.0
67.90	23888.0
68.90	25224.0
70.00	1904.0
71.90	1132.0
72.90	10796.0
74.00	40464.0
75.00	123256.0
76.00	10708.0
76.90	1394.0
77.90	1206.0
78.90	7370.0
79.90	2211.0
80.80	8172.0
81.80	1746.0
82.80	198.0
85.70	418.0
86.90	8679.0
87.90	8455.0
90.70	959.0
91.90	7564.0
92.90	10516.0
94.00	29072.0
95.00	236096.0
96.00	16321.0
96.90	337.0
102.60	107.0
103.80	1066.0
104.80	244.0
105.80	918.0
106.90	259.0
109.70	138.0
110.90	277.0
111.90	129.0
112.80	223.0
115.00	214.0
115.80	721.0
116.90	1347.0
117.80	940.0
118.90	1494.0
123.90	118.0
125.80	109.0
127.80	777.0
128.80	316.0
129.90	778.0
130.80	435.0
134.80	332.0
136.80	448.0
140.90	1916.0
142.00	168.0
142.90	2884.0
143.90	207.0
144.80	585.0
145.80	256.0
146.70	112.0
147.70	561.0
148.80	173.0
149.80	130.0
152.80	152.0
153.90	164.0
154.90	551.0
156.80	493.0
158.80	191.0
160.80	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

170.80	151.0
171.90	1237.0
173.00	1508.0
173.90	172608.0
174.90	12665.0
175.90	167232.0
176.90	11175.0
177.90	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
35.90	1723.0
36.90	10021.0
37.90	8685.0
38.90	3612.0
39.90	558.0
42.80	207.0
43.90	2038.0
45.00	1655.0
46.00	236.0
46.90	2617.0
47.80	1422.0
48.90	8916.0
49.90	42528.0
51.00	13609.0
51.90	687.0
52.60	218.0
54.90	563.0
56.00	3298.0
56.90	6669.0
57.90	284.0
59.90	2313.0
60.90	12098.0
61.90	11529.0
63.00	8696.0
64.00	1051.0
65.00	1112.0
66.00	161.0
66.90	677.0
67.90	25424.0
68.90	26456.0
70.00	1734.0
71.90	1193.0
72.90	11406.0
74.00	41720.0
75.00	128104.0
76.00	10594.0
76.90	1445.0
77.90	1100.0
78.90	7734.0
79.90	2294.0
80.80	8169.0
81.90	1937.0
82.80	243.0
85.70	473.0
86.90	8854.0
87.90	8968.0
90.80	1062.0
91.90	7803.0
92.90	10738.0
94.00	29968.0
95.00	249088.0
96.00	16512.0
96.90	318.0
102.80	149.0
103.80	1058.0
104.80	241.0
105.80	996.0
106.70	251.0
109.80	129.0
110.90	246.0
111.70	142.0
112.90	321.0
114.90	209.0
115.80	785.0
116.90	1574.0
117.80	1040.0
118.90	1416.0
125.80	118.0
127.90	887.0
128.80	365.0
129.90	842.0
130.80	433.0
134.90	436.0
136.80	560.0
139.70	108.0
140.90	2067.0
142.10	223.0
142.90	2958.0
143.80	234.0
144.80	693.0
145.80	265.0
146.60	181.0
147.70	560.0
148.80	148.0
149.70	114.0
150.10	145.0
152.90	129.0
153.90	156.0
154.90	525.0
156.10	113.0
156.80	457.0
158.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

160.80	291.0
170.90	157.0
171.90	1465.0
172.90	1806.0
173.90	183616.0
174.90	12982.0
175.90	178304.0
176.90	11408.0
177.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
35.90	1658.0
36.90	9348.0
37.90	8352.0
38.90	3262.0
39.90	560.0
42.80	147.0
43.90	1920.0
45.00	1536.0
45.90	235.0
46.90	2534.0
47.90	1194.0
48.90	8328.0
49.90	39936.0
51.00	12944.0
51.90	568.0
52.90	201.0
54.90	503.0
56.00	3228.0
56.90	5934.0
57.80	250.0
59.90	2079.0
60.90	10419.0
61.90	11453.0
63.00	8195.0
63.90	1010.0
65.00	1090.0
66.00	121.0
66.90	590.0
67.90	24408.0
68.90	24744.0
69.90	1501.0
71.90	1215.0
72.90	10599.0
73.90	39400.0
74.90	121544.0
76.00	9767.0
77.00	1541.0
78.00	877.0
78.90	7158.0
79.90	2062.0
80.90	7338.0
81.90	2007.0
82.80	251.0
85.70	348.0
86.90	8770.0
87.90	8591.0
90.80	1057.0
92.00	7236.0
92.90	10045.0
93.90	27992.0
95.00	239936.0
96.00	15059.0
97.00	365.0
102.90	179.0
103.80	1028.0
104.70	219.0
105.90	1103.0
106.60	222.0
109.80	135.0
110.90	185.0
111.70	167.0
112.90	340.0
114.90	176.0
115.80	836.0
116.90	1606.0
117.80	1044.0
118.90	1200.0
123.80	115.0
127.80	890.0
128.80	418.0
129.80	845.0
130.80	378.0
134.90	485.0
136.80	565.0
139.70	155.0
140.90	2220.0
142.10	280.0
142.80	2646.0
143.80	247.0
144.80	615.0
145.90	298.0
146.60	244.0
147.70	528.0
148.80	128.0
149.70	151.0
150.10	184.0
152.90	123.0
153.90	136.0
154.90	480.0
156.00	150.0
156.90	377.0
159.00	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

160.90	309.0
170.90	162.0
171.90	1596.0
172.90	1902.0
173.90	179712.0
174.90	12408.0
175.90	173888.0
176.90	11174.0
177.90	300.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058