


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102518\
 Data File : VU027805.D
 Acq On : 25 Oct 2018 14:18
 Operator : MD/SY
 Sample : BFB01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 30 02:27:31 2018

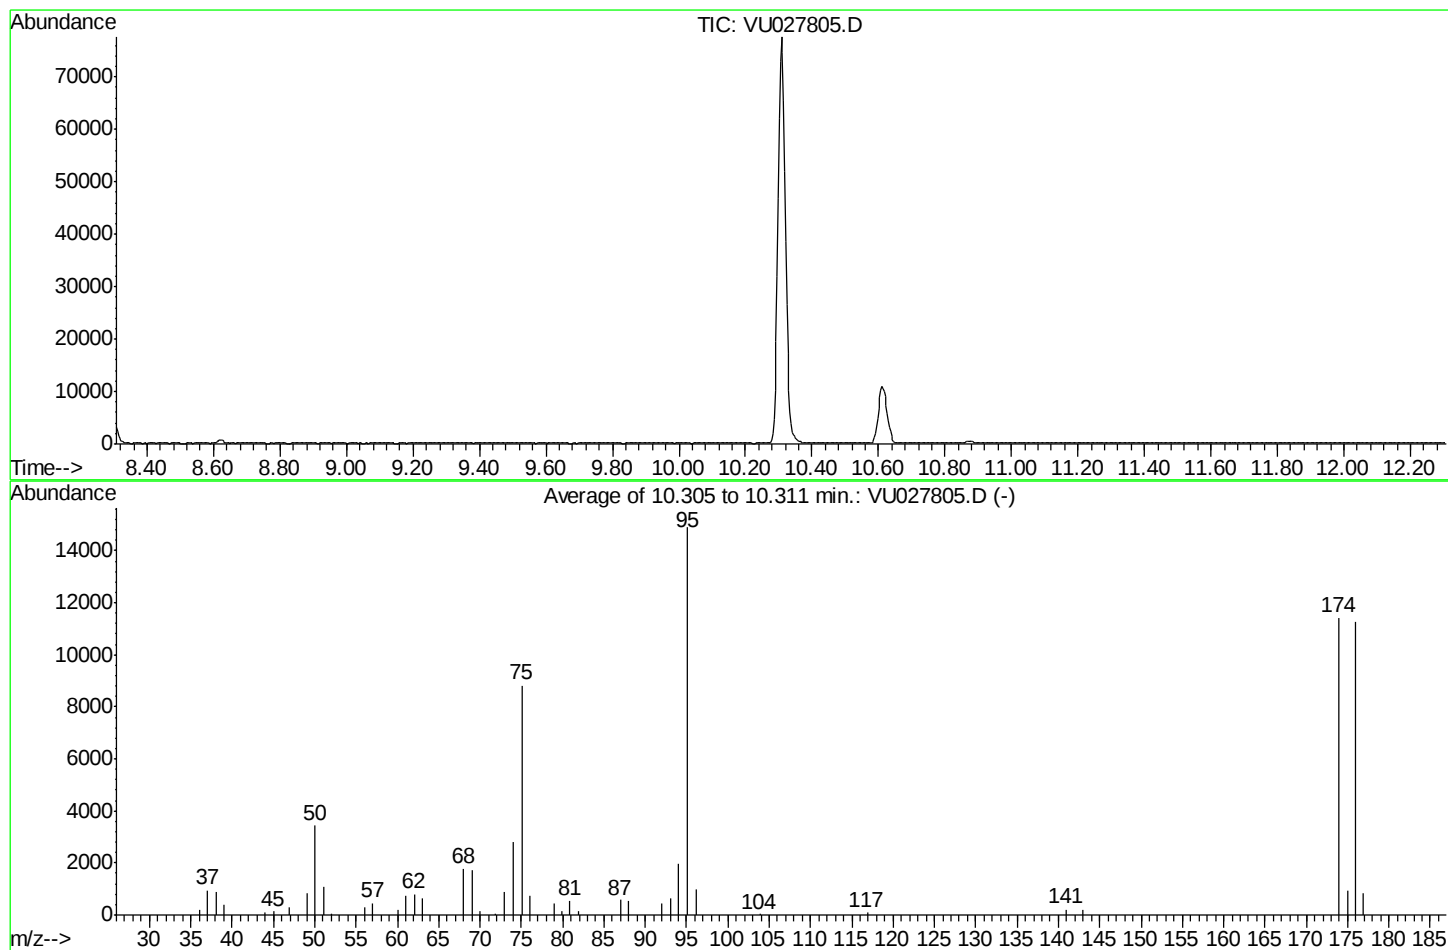

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	3439	PASS
75	95	30	80	59.2	8819	PASS
95	95	100	100	100.0	14895	PASS
96	95	5	9	6.5	968	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.7	11430	PASS
175	174	5	9	8.0	920	PASS
176	174	95	101	98.6	11274	PASS
177	176	5	9	7.4	832	PASS

m/z	Abundance
44.10	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	166.0
37.00	930.0
38.10	877.0
39.00	372.0
44.00	268.0
45.00	136.0
46.90	268.0
49.00	749.0
50.00	3354.0
51.00	1022.0
52.10	106.0
56.00	282.0
57.00	454.0
60.00	175.0
61.00	744.0
62.10	812.0
63.00	612.0
68.00	1714.0
69.00	1703.0
70.00	146.0
73.00	840.0
74.10	2749.0
75.10	8643.0
76.00	772.0
79.00	497.0
79.80	139.0
80.90	552.0
81.90	131.0
87.00	636.0
88.00	505.0
92.00	455.0
93.00	668.0
94.10	1924.0
95.10	14586.0
96.10	1053.0
140.90	202.0
142.90	194.0
174.00	10980.0
175.00	930.0
176.00	10856.0
177.00	802.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	197.0
37.00	919.0
38.00	838.0
39.00	350.0
44.00	246.0
45.00	139.0
46.90	290.0
49.00	889.0
50.10	3405.0
51.10	1107.0
56.00	268.0
57.00	446.0
60.10	180.0
61.00	761.0
62.00	768.0
63.00	678.0
68.00	1804.0
69.00	1707.0
70.10	139.0
71.90	111.0
73.00	923.0
74.00	2788.0
75.10	8653.0
76.00	740.0
78.90	414.0
79.90	189.0
80.90	532.0
81.90	142.0
87.00	510.0
88.00	555.0
92.00	460.0
93.00	647.0
94.00	1982.0
95.10	14722.0
96.10	854.0
116.90	142.0
141.00	247.0
143.00	217.0
174.00	11543.0
175.00	920.0
176.00	11368.0
176.90	855.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	197.0
37.00	919.0
38.00	838.0
39.00	350.0
44.00	246.0
45.00	139.0
46.90	290.0
49.00	889.0
50.10	3405.0
51.10	1107.0
56.00	268.0
57.00	446.0
60.10	180.0
61.00	761.0
62.00	768.0
63.00	678.0
68.00	1804.0
69.00	1707.0
70.10	139.0
71.90	111.0
73.00	923.0
74.00	2788.0
75.10	8653.0
76.00	740.0
78.90	414.0
79.90	189.0
80.90	532.0
81.90	142.0
87.00	510.0
88.00	555.0
92.00	460.0
93.00	647.0
94.00	1982.0
95.10	14722.0
96.10	854.0
116.90	142.0
141.00	247.0
143.00	217.0
174.00	11543.0
175.00	920.0
176.00	11368.0
176.90	855.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01