


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102519\
 Data File : VU035478.D
 Acq On : 25 Oct 2019 10:01
 Operator : JC/SP
 Sample : BFB27
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102519WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Oct 26 04:07:11 2019

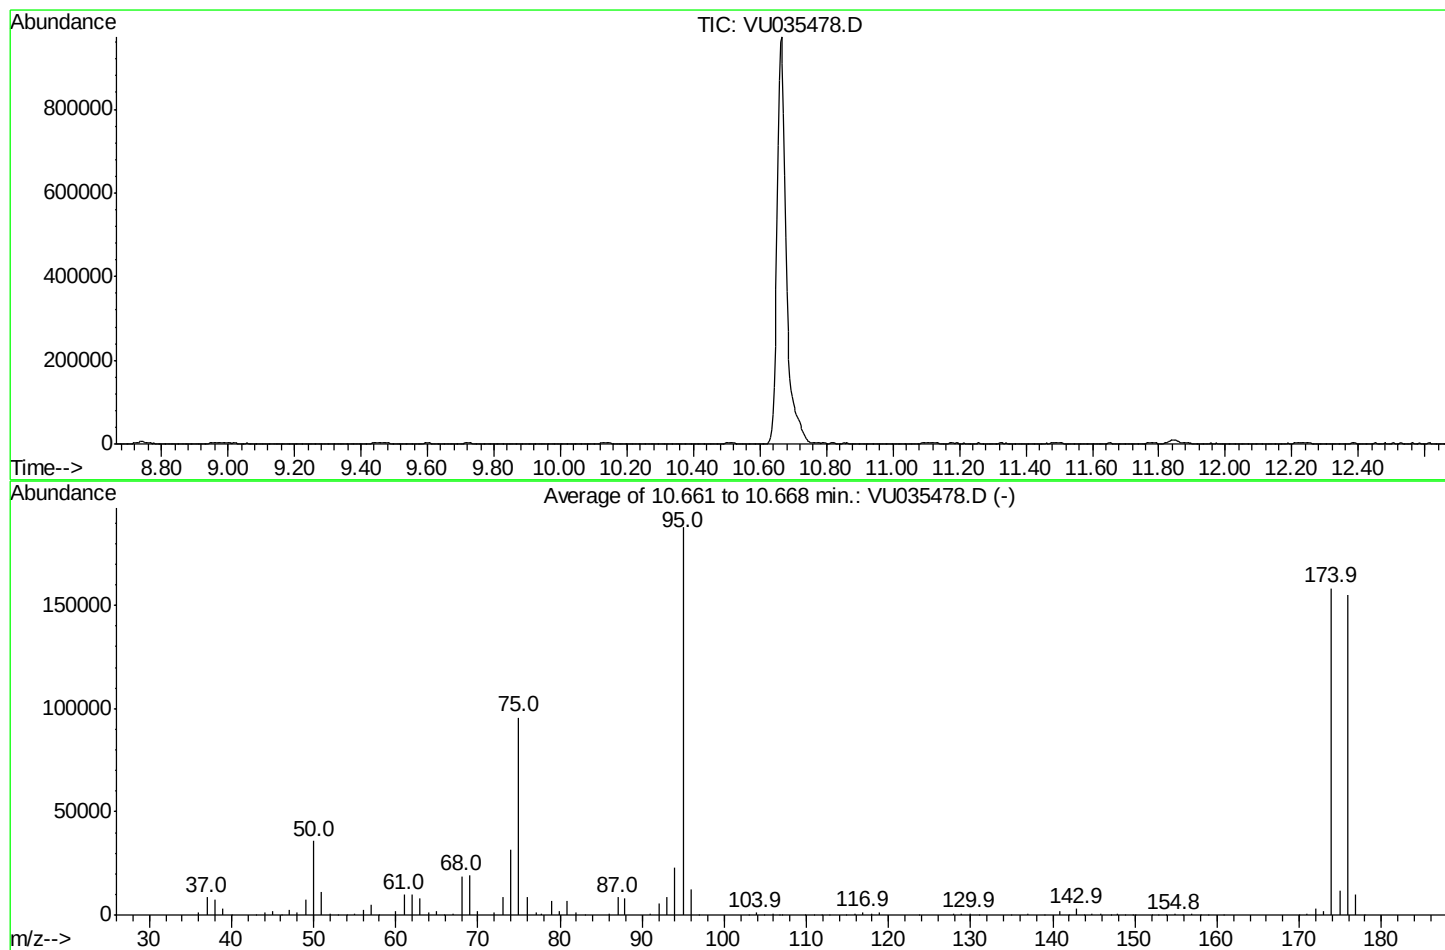

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	35728	PASS
75	95	30	80	51.0	95800	PASS
95	95	100	100	100.0	187904	PASS
96	95	5	9	6.7	12670	PASS
173	174	0.00	2	1.4	2178	PASS
174	95	50	120	84.3	158378	PASS
175	174	5	9	7.7	12118	PASS
176	174	95	101	98.0	155200	PASS
177	176	5	9	6.4	9981	PASS

Scan 2884 (10.613 min): VU035478.D
BFB27

m/z	Abundance
39.90	279.0
44.00	647.0
68.90	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	1617.0
37.00	8744.0
38.00	7758.0
39.00	3669.0
40.00	323.0
43.00	142.0
44.00	1932.0
45.00	1541.0
46.00	255.0
47.00	2548.0
48.00	1010.0
49.00	7765.0
50.00	36816.0
51.00	11321.0
52.10	391.0
52.90	306.0
54.00	138.0
55.00	547.0
56.00	2783.0
57.00	5282.0
57.90	223.0
60.00	2036.0
61.00	9668.0
62.00	9796.0
63.00	7987.0
64.00	1290.0
65.00	1776.0
66.00	178.0
66.90	446.0
68.00	19496.0
69.00	20056.0
70.00	1805.0
71.90	1065.0
73.00	8857.0
74.00	32264.0
75.00	97648.0
76.00	8987.0
77.10	1375.0
77.80	624.0
78.90	7123.0
79.90	1927.0
80.90	7191.0
81.90	1453.0
83.00	209.0
86.00	379.0
87.00	9120.0
87.90	8250.0
91.00	706.0
92.00	5644.0
93.00	8651.0
94.00	23824.0
95.00	191872.0
96.00	12964.0
97.00	372.0
103.90	1068.0
104.80	211.0
105.90	935.0
106.70	172.0
109.90	166.0
110.90	203.0
111.90	221.0
112.80	147.0
114.80	295.0
115.90	756.0
116.90	1430.0
117.90	684.0
118.90	1295.0
127.90	618.0
128.90	411.0
129.90	631.0
131.00	318.0
134.90	313.0
136.90	406.0
140.90	1899.0
141.90	156.0
142.90	2874.0
143.90	249.0
144.80	810.0
145.90	372.0
147.00	142.0
147.90	453.0
148.80	105.0
150.00	164.0
152.80	185.0
153.80	121.0
154.90	536.0
155.80	129.0
156.90	351.0
157.90	138.0
158.80	259.0
160.80	294.0
169.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

170.90	467.0
171.90	2970.0
173.00	2323.0
173.90	158912.0
174.90	12160.0
175.90	153792.0
176.90	10044.0
177.90	322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	1597.0
37.00	8809.0
38.00	7656.0
39.00	3471.0
40.00	295.0
42.90	125.0
44.00	1870.0
45.00	1650.0
46.00	250.0
47.00	2581.0
48.00	1016.0
49.00	7555.0
50.00	36712.0
51.00	11386.0
52.10	372.0
52.90	328.0
54.00	128.0
55.00	507.0
56.00	2828.0
57.00	5440.0
57.90	193.0
60.00	2047.0
61.00	9890.0
62.00	10200.0
63.00	8090.0
64.00	1272.0
65.00	1820.0
66.00	128.0
66.90	468.0
68.00	19112.0
69.00	20248.0
70.00	1686.0
71.90	1141.0
73.00	9065.0
74.00	32352.0
75.00	98384.0
76.00	8903.0
77.10	1364.0
77.80	644.0
78.90	6968.0
79.90	1871.0
80.90	7257.0
81.90	1455.0
83.00	258.0
85.90	342.0
87.00	8846.0
87.90	8535.0
90.90	724.0
92.00	5791.0
93.00	8603.0
94.00	23872.0
95.00	192448.0
96.00	13044.0
96.90	305.0
102.90	106.0
103.90	1042.0
104.90	221.0
105.90	915.0
106.90	167.0
109.90	160.0
110.90	227.0
111.90	201.0
112.80	203.0
114.80	290.0
115.90	799.0
116.90	1484.0
117.90	676.0
118.80	1429.0
123.70	119.0
127.90	635.0
128.90	424.0
129.90	747.0
130.90	310.0
134.80	280.0
136.90	398.0
140.90	1871.0
141.90	160.0
142.90	3032.0
143.80	226.0
144.80	822.0
145.90	446.0
147.00	125.0
147.90	511.0
149.70	164.0
152.10	104.0
152.80	211.0
153.80	104.0
154.90	482.0
155.80	138.0
156.90	384.0
157.90	106.0
158.80	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

160.80	258.0
169.90	105.0
170.90	455.0
172.00	2976.0
173.00	2244.0
173.90	162176.0
174.90	12464.0
175.90	159552.0
176.90	10251.0
177.90	327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	1407.0
37.00	8201.0
38.00	6977.0
39.00	3045.0
40.00	311.0
43.00	104.0
44.00	1733.0
45.00	1593.0
46.10	204.0
47.00	2449.0
48.00	938.0
49.00	6937.0
50.00	33656.0
51.00	10451.0
52.00	364.0
52.90	299.0
55.00	462.0
56.00	2524.0
57.00	4981.0
57.90	176.0
60.00	1910.0
61.00	9402.0
62.00	9262.0
63.00	7400.0
64.00	1230.0
65.00	1763.0
65.90	144.0
66.90	421.0
68.00	17544.0
69.00	18584.0
70.00	1377.0
72.00	1030.0
73.00	8537.0
74.00	30328.0
75.00	91368.0
76.00	8076.0
77.10	1148.0
77.80	685.0
78.90	6532.0
79.80	1686.0
80.90	6779.0
81.90	1394.0
83.00	250.0
85.90	287.0
87.00	8029.0
87.90	7863.0
90.90	711.0
92.00	5308.0
93.00	8011.0
94.00	21864.0
95.00	179392.0
96.00	12004.0
96.90	239.0
103.90	863.0
104.90	258.0
105.90	832.0
107.00	182.0
109.90	126.0
110.90	204.0
111.90	156.0
112.80	223.0
114.70	290.0
115.90	736.0
116.90	1432.0
117.90	622.0
118.80	1384.0
123.70	134.0
127.90	593.0
128.90	370.0
129.90	781.0
130.90	307.0
134.80	229.0
137.00	359.0
138.90	101.0
140.90	1765.0
142.00	161.0
142.90	2836.0
143.90	183.0
144.80	742.0
145.90	435.0
147.90	466.0
149.70	161.0
152.90	186.0
154.80	408.0
155.90	140.0
156.90	347.0
158.90	200.0
160.80	188.0
170.90	359.0
172.00	2623.0
173.00	1967.0
173.90	154048.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

174.90	11731.0
175.90	152256.0
176.90	9650.0
177.90	335.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27