


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102521\
Data File : VU045373.D
Acq On : 25 Oct 2021 09:59
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
Title : SW846 8260
Last Update : Tue Sep 28 12:32:13 2021

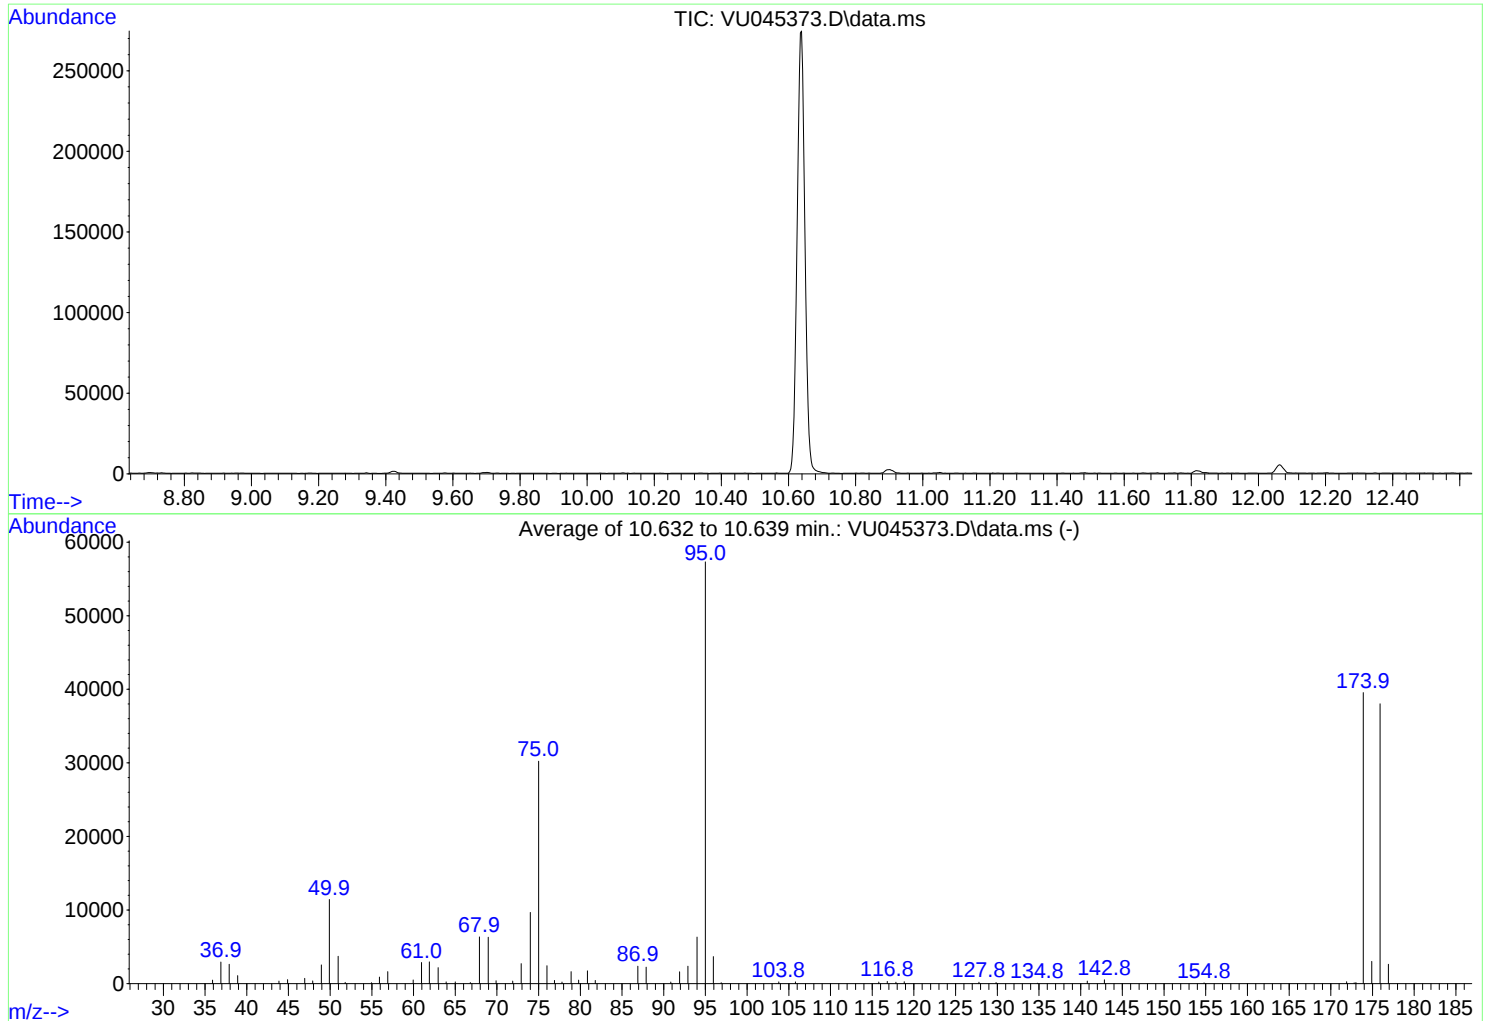

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11448	PASS
75	95	30	60	52.7	30221	PASS
95	95	100	100	100.0	57323	PASS
96	95	5	9	6.4	3687	PASS
173	174	0.00	2	0.4	158	PASS
174	95	50	100	69.0	39563	PASS
175	174	5	9	7.7	3027	PASS
176	174	95	101	96.1	38035	PASS
177	176	5	9	6.9	2634	PASS