

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055870.D
 Acq On : 25 Oct 2023 11:31
 Operator : MD/SY
 Sample : 04952-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	109	rVB	233743	273752	11.92%	1.532%
2	1.894	181	188	217	rVB	179838	286079	12.45%	1.601%
3	2.560	383	395	412	rBV	415077	683385	29.75%	3.824%
4	2.788	459	466	472	rBV3	1795	2881	0.13%	0.016%
5	2.862	485	489	494	rBV5	535	634	0.03%	0.004%
6	3.039	534	544	557	rBV8	4281	8333	0.36%	0.047%
7	3.181	570	588	608	rBV2	12684	34396	1.50%	0.192%
8	3.283	618	620	624	rBV2	424	302	0.01%	0.002%
9	3.338	633	637	639	rBV	723	548	0.02%	0.003%
10	3.377	645	649	652	rBV2	382	329	0.01%	0.002%
11	3.537	693	699	704	rBV2	576	744	0.03%	0.004%
12	3.853	791	797	802	rVB2	311	353	0.02%	0.002%
13	3.898	805	811	813	rBV2	422	349	0.02%	0.002%
14	4.161	887	893	895	rBV	338	315	0.01%	0.002%
15	4.280	926	930	936	rVB2	260	301	0.01%	0.002%
16	4.322	940	943	949	rVB2	304	357	0.02%	0.002%
17	4.354	949	953	957	rBV	350	312	0.01%	0.002%
18	4.615	1022	1034	1078	rBV	192934	509926	22.20%	2.853%
19	5.058	1151	1172	1197	rBV	416318	937681	40.82%	5.246%
20	5.328	1245	1256	1270	rVB6	3390	8197	0.36%	0.046%
21	5.492	1302	1307	1313	rBV3	575	554	0.02%	0.003%
22	5.721	1356	1378	1408	rBV2	827445	2297024	100.00%	12.852%
23	6.033	1470	1475	1478	rBV3	516	601	0.03%	0.003%
24	6.106	1491	1498	1500	rBV2	600	771	0.03%	0.004%
25	6.158	1512	1514	1520	rVB2	476	336	0.01%	0.002%
26	6.245	1527	1541	1570	rBV	627459	1224644	53.31%	6.852%
27	6.524	1619	1628	1641	rVB9	3384	7120	0.31%	0.040%
28	6.595	1641	1650	1654	rBV5	1527	2026	0.09%	0.011%
29	6.685	1664	1678	1707	rBV	527223	1047944	45.62%	5.863%
30	6.885	1737	1740	1746	rVB6	573	522	0.02%	0.003%
31	6.917	1746	1750	1752	rBV3	430	316	0.01%	0.002%
32	6.933	1752	1755	1758	rVB2	598	354	0.02%	0.002%
33	7.187	1815	1834	1844	rBV7	7303	17135	0.75%	0.096%
34	7.270	1858	1860	1865	rVB2	628	415	0.02%	0.002%
35	7.499	1928	1931	1936	rBV3	514	538	0.02%	0.003%
36	7.563	1938	1951	1977	rBV	291988	519662	22.62%	2.908%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055870.D
 Acq On : 25 Oct 2023 11:31
 Operator : MD/SY
 Sample : 04952-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.698	1985	1993	1998	rBV5	3255	4732	0.21%	0.026%
38	7.756	2008	2011	2017	rVB4	652	511	0.02%	0.003%
39	7.798	2019	2024	2028	rBV2	674	689	0.03%	0.004%
40	7.894	2040	2054	2090	rBV	993800	1792285	78.03%	10.028%
41	8.177	2129	2142	2174	rBV	200977	355677	15.48%	1.990%
42	8.286	2174	2176	2179	rVV5	701	496	0.02%	0.003%
43	8.467	2221	2232	2246	rBV3	15216	27716	1.21%	0.155%
44	8.630	2271	2283	2321	rBV	693823	1339911	58.33%	7.497%
45	8.891	2361	2364	2365	rBV	616	303	0.01%	0.002%
46	8.936	2376	2378	2381	rBV4	455	306	0.01%	0.002%
47	9.003	2393	2399	2401	rBV4	444	449	0.02%	0.003%
48	9.055	2412	2415	2420	rVB4	568	536	0.02%	0.003%
49	9.090	2422	2426	2432	rBV3	766	753	0.03%	0.004%
50	9.209	2459	2463	2464	rBV3	398	294	0.01%	0.002%
51	9.238	2469	2472	2475	rVB3	553	360	0.02%	0.002%
52	9.293	2487	2489	2493	rVB2	542	339	0.01%	0.002%
53	9.315	2493	2496	2499	rBV2	624	497	0.02%	0.003%
54	9.335	2499	2502	2506	rBV3	393	320	0.01%	0.002%
55	9.415	2514	2527	2559	rBV	941741	1586601	69.07%	8.877%
56	9.692	2608	2613	2619	rVV5	1478	2206	0.10%	0.012%
57	9.737	2623	2627	2630	rVV	377	319	0.01%	0.002%
58	9.962	2692	2697	2699	rBV2	360	306	0.01%	0.002%
59	9.984	2701	2704	2707	rVB	562	329	0.01%	0.002%
60	10.013	2710	2713	2717	rVB2	682	387	0.02%	0.002%
61	10.138	2746	2752	2755	rVB4	617	626	0.03%	0.004%
62	10.380	2822	2827	2829	rBV2	554	391	0.02%	0.002%
63	10.454	2847	2850	2853	rBV3	531	376	0.02%	0.002%
64	10.518	2867	2870	2875	rVB2	660	540	0.02%	0.003%
65	10.566	2882	2885	2889	rBV2	603	425	0.02%	0.002%
66	10.704	2920	2928	2930	rBV2	437	467	0.02%	0.003%
67	10.753	2930	2943	2966	rBV	847149	1385168	60.30%	7.750%
68	10.891	2974	2986	2995	rBV3	13719	21743	0.95%	0.122%
69	11.039	3028	3032	3034	rBV3	415	316	0.01%	0.002%
70	11.074	3039	3043	3046	rBV2	383	303	0.01%	0.002%
71	11.103	3050	3052	3056	rVB3	482	303	0.01%	0.002%
72	11.209	3082	3085	3090	rVB2	616	511	0.02%	0.003%
73	11.309	3112	3116	3120	rVB3	432	379	0.02%	0.002%
74	11.373	3132	3136	3141	rBV2	400	396	0.02%	0.002%
75	11.409	3144	3147	3151	rBV2	876	574	0.02%	0.003%
76	11.473	3162	3167	3169	rBV2	659	520	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055870.D
 Acq On : 25 Oct 2023 11:31
 Operator : MD/SY
 Sample : 04952-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.486	3169	3171	3179	rVB3	590	690	0.03%	0.004%
78	11.634	3214	3217	3222	rVB3	557	441	0.02%	0.002%
79	11.717	3238	3243	3247	rBV3	550	518	0.02%	0.003%
80	11.743	3247	3251	3253	rBV3	1173	948	0.04%	0.005%
81	11.810	3259	3272	3300	rBV	1003571	1631834	71.04%	9.130%
82	11.971	3319	3322	3326	rVB5	1035	809	0.04%	0.005%
83	12.119	3365	3368	3369	rBV2	792	440	0.02%	0.002%
84	12.190	3377	3390	3415	rVV	1090212	1827776	79.57%	10.227%
85	12.444	3467	3469	3473	rBV4	597	503	0.02%	0.003%
86	12.708	3549	3551	3554	rVB2	566	303	0.01%	0.002%
87	12.740	3557	3561	3563	rBV3	540	381	0.02%	0.002%
88	12.765	3564	3569	3570	rBV3	1558	1242	0.05%	0.007%
89	12.878	3601	3604	3606	rBV2	384	304	0.01%	0.002%
90	13.000	3639	3642	3644	rVV2	440	335	0.01%	0.002%
91	13.264	3722	3724	3728	rVB3	731	484	0.02%	0.003%
92	13.289	3728	3732	3733	rBV	640	376	0.02%	0.002%
93	13.479	3788	3791	3795	rBV2	873	724	0.03%	0.004%
94	13.556	3812	3815	3821	rBV2	566	640	0.03%	0.004%
95	13.820	3895	3897	3899	rBV2	635	383	0.02%	0.002%
96	13.846	3900	3905	3906	rBV3	1829	1419	0.06%	0.008%
97	14.334	4053	4057	4063	rBV7	1613	1906	0.08%	0.011%
98	14.563	4126	4128	4131	rBV2	870	422	0.02%	0.002%
99	14.765	4188	4191	4196	rBV3	900	830	0.04%	0.005%
100	15.277	4348	4350	4357	rVB4	1153	683	0.03%	0.004%




Sum of corrected areas: 17872887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055870.D
Acq On : 25 Oct 2023 11:31
Operator : MD/SY
Sample : 04952-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

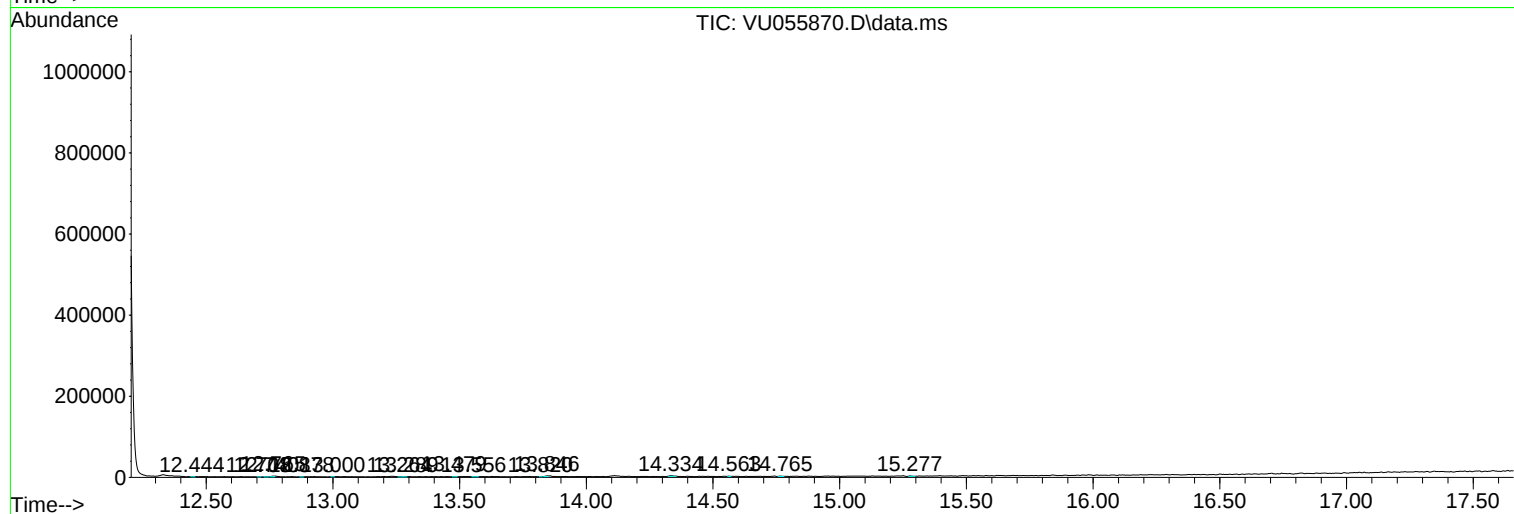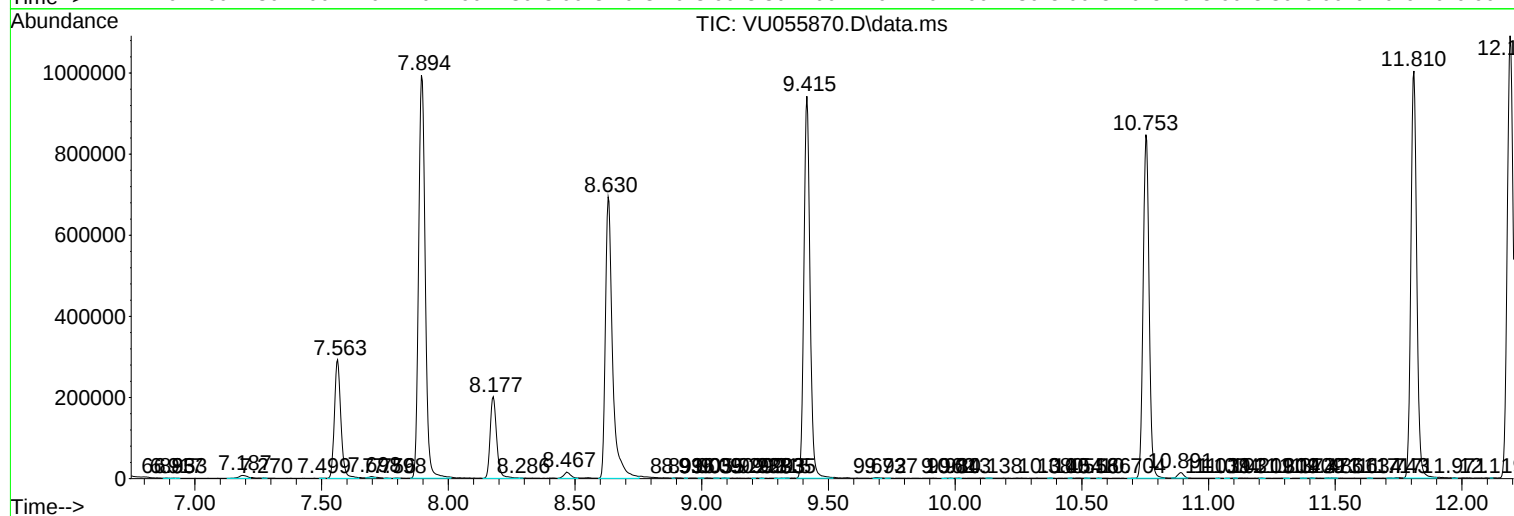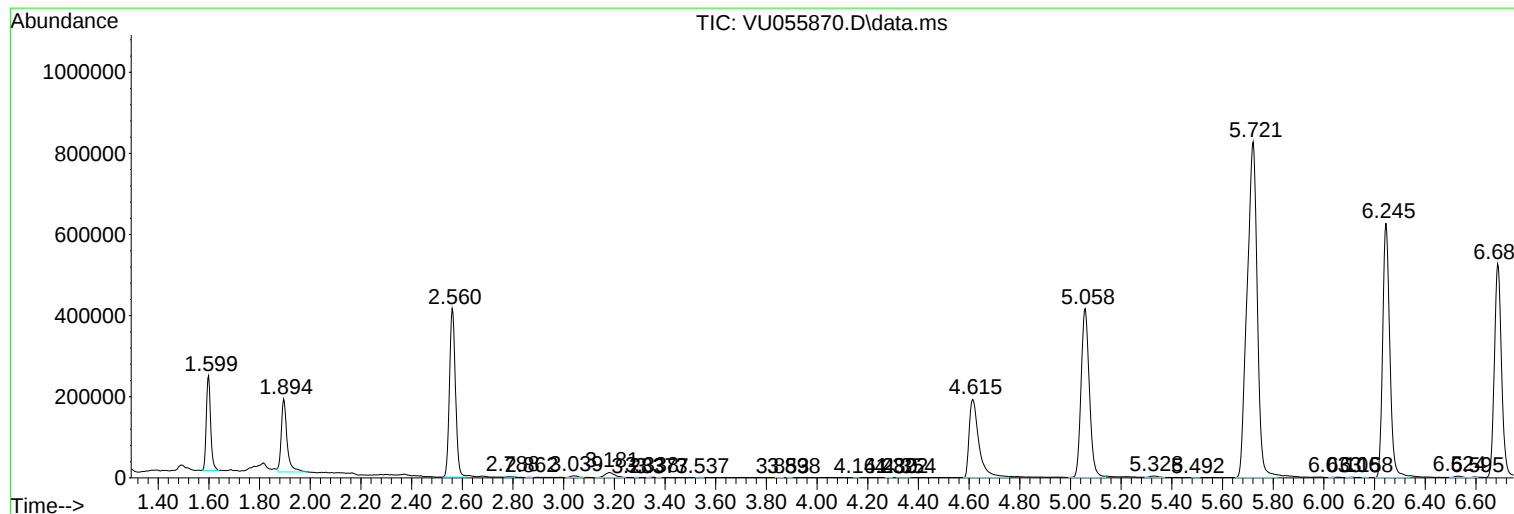

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055870.D
Acq On : 25 Oct 2023 11:31
Operator : MD/SY
Sample : 04952-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055870.D
Acq On : 25 Oct 2023 11:31
Operator : MD/SY
Sample : 04952-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc