

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055871.D
 Acq On : 25 Oct 2023 11:56
 Operator : MD/SY
 Sample : 04952-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	89	95	108	rVB	205019	250246	11.52%	1.456%
2	1.885	178	185	209	rVB	160945	261434	12.03%	1.521%
3	2.557	382	394	409	rBV	392451	639612	29.44%	3.722%
4	2.737	448	450	454	rBV3	469	352	0.02%	0.002%
5	2.859	482	488	489	rBV2	619	615	0.03%	0.004%
6	2.933	505	511	514	rBV5	813	802	0.04%	0.005%
7	2.952	514	517	521	rVV4	771	774	0.04%	0.005%
8	2.985	525	527	532	rVV2	627	498	0.02%	0.003%
9	3.036	535	543	556	rBV3	4928	9300	0.43%	0.054%
10	3.178	577	587	599	rVV2	9542	20453	0.94%	0.119%
11	3.351	636	641	644	rBV2	927	1075	0.05%	0.006%
12	3.387	649	652	660	rVB2	553	651	0.03%	0.004%
13	3.573	705	710	714	rBV3	342	316	0.01%	0.002%
14	3.660	732	737	738	rBV2	774	365	0.02%	0.002%
15	3.766	766	770	774	rVB2	533	458	0.02%	0.003%
16	3.843	787	794	796	rBV2	423	410	0.02%	0.002%
17	3.923	814	819	822	rVV	350	335	0.02%	0.002%
18	4.100	871	874	879	rVB	465	388	0.02%	0.002%
19	4.232	912	915	922	rVB2	347	346	0.02%	0.002%
20	4.370	953	958	963	rVB	389	401	0.02%	0.002%
21	4.457	979	985	990	rBV2	431	445	0.02%	0.003%
22	4.557	1011	1016	1020	rVB2	344	346	0.02%	0.002%
23	4.612	1021	1033	1062	rBV	190121	498500	22.94%	2.901%
24	4.904	1122	1124	1128	rVB2	777	524	0.02%	0.003%
25	4.933	1128	1133	1135	rVB2	656	495	0.02%	0.003%
26	4.965	1138	1143	1147	rBV3	385	423	0.02%	0.002%
27	5.055	1154	1171	1197	rBV	393152	886522	40.80%	5.159%
28	5.258	1231	1234	1238	rBV3	492	546	0.03%	0.003%
29	5.322	1247	1254	1256	rBV3	2776	3006	0.14%	0.017%
30	5.563	1323	1329	1332	rBV2	374	412	0.02%	0.002%
31	5.718	1356	1377	1400	rBV2	784040	2172822	100.00%	12.645%
32	5.962	1447	1453	1455	rBV4	1319	1219	0.06%	0.007%
33	6.046	1471	1479	1482	rBV6	629	881	0.04%	0.005%
34	6.242	1527	1540	1566	rBV	632373	1238204	56.99%	7.206%
35	6.399	1586	1589	1591	rBV3	1037	519	0.02%	0.003%
36	6.525	1620	1628	1639	rVB9	2910	5886	0.27%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055871.D
 Acq On : 25 Oct 2023 11:56
 Operator : MD/SY
 Sample : 04952-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.583	1642	1646	1647	rBV2	732	474	0.02%	0.003%
38	6.685	1663	1678	1702	rBV	499700	994628	45.78%	5.788%
39	7.023	1779	1783	1786	rVB2	476	326	0.02%	0.002%
40	7.184	1820	1833	1846	rBV5	7655	19070	0.88%	0.111%
41	7.351	1880	1885	1888	rBV2	451	414	0.02%	0.002%
42	7.560	1936	1950	1974	rBV	271052	488372	22.48%	2.842%
43	7.695	1987	1992	2000	rVB5	2609	3539	0.16%	0.021%
44	7.795	2019	2023	2026	rBV3	819	659	0.03%	0.004%
45	7.894	2041	2054	2079	rBV	945098	1661066	76.45%	9.667%
46	8.174	2129	2141	2158	rBV	187708	329565	15.17%	1.918%
47	8.412	2209	2215	2217	rBV4	557	478	0.02%	0.003%
48	8.470	2222	2233	2246	rVV	18521	31957	1.47%	0.186%
49	8.553	2256	2259	2264	rVB5	1770	1484	0.07%	0.009%
50	8.634	2269	2284	2319	rBV	685570	1353056	62.27%	7.874%
51	8.859	2351	2354	2356	rBV4	536	315	0.01%	0.002%
52	8.914	2368	2371	2375	rVB5	651	482	0.02%	0.003%
53	9.000	2395	2398	2403	rBV3	721	814	0.04%	0.005%
54	9.052	2411	2414	2417	rBV3	453	365	0.02%	0.002%
55	9.158	2443	2447	2451	rVB4	602	520	0.02%	0.003%
56	9.277	2480	2484	2490	rVB3	748	782	0.04%	0.005%
57	9.306	2490	2493	2495	rBV2	628	413	0.02%	0.002%
58	9.332	2499	2501	2506	rVB3	689	460	0.02%	0.003%
59	9.415	2510	2527	2550	rBV	927399	1565953	72.07%	9.113%
60	9.618	2586	2590	2594	rVB6	1264	1167	0.05%	0.007%
61	9.644	2594	2598	2600	rBV2	436	350	0.02%	0.002%
62	9.685	2608	2611	2613	rBV2	614	430	0.02%	0.003%
63	9.721	2620	2622	2626	rVB2	673	363	0.02%	0.002%
64	9.875	2665	2670	2671	rBV	607	498	0.02%	0.003%
65	9.968	2694	2699	2703	rBV3	583	705	0.03%	0.004%
66	10.110	2741	2743	2746	rVV3	551	359	0.02%	0.002%
67	10.139	2749	2752	2758	rVB2	828	549	0.03%	0.003%
68	10.248	2784	2786	2787	rBV	785	306	0.01%	0.002%
69	10.283	2794	2797	2804	rBV2	431	377	0.02%	0.002%
70	10.409	2832	2836	2842	rBV2	491	473	0.02%	0.003%
71	10.496	2861	2863	2872	rVB3	745	522	0.02%	0.003%
72	10.537	2872	2876	2881	rVB2	366	422	0.02%	0.002%
73	10.656	2910	2913	2917	rBV2	731	684	0.03%	0.004%
74	10.753	2930	2943	2967	rBV	826407	1354694	62.35%	7.884%
75	10.891	2976	2986	2996	rVB2	18630	29897	1.38%	0.174%
76	11.013	3020	3024	3029	rBV3	498	457	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055871.D
 Acq On : 25 Oct 2023 11:56
 Operator : MD/SY
 Sample : 04952-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.039	3029	3032	3036	rBV2	387	357	0.02%	0.002%
78	11.094	3045	3049	3053	rBV3	656	612	0.03%	0.004%
79	11.177	3068	3075	3080	rBV3	622	831	0.04%	0.005%
80	11.357	3127	3131	3134	rBV2	438	427	0.02%	0.002%
81	11.473	3164	3167	3170	rBV2	630	403	0.02%	0.002%
82	11.569	3194	3197	3200	rBV2	506	405	0.02%	0.002%
83	11.605	3205	3208	3210	rVV	605	455	0.02%	0.003%
84	11.743	3248	3251	3259	rVB4	1292	1417	0.07%	0.008%
85	11.807	3259	3271	3288	rBV	999661	1598665	73.58%	9.304%
86	12.058	3347	3349	3352	rBV2	430	368	0.02%	0.002%
87	12.094	3358	3360	3364	rBV3	740	362	0.02%	0.002%
88	12.190	3377	3390	3411	rBV	1051021	1715741	78.96%	9.985%
89	12.450	3468	3471	3478	rVB4	955	996	0.05%	0.006%
90	12.505	3484	3488	3489	rBV3	874	535	0.02%	0.003%
91	12.769	3561	3570	3580	rBV2	3771	6190	0.28%	0.036%
92	12.811	3581	3583	3589	rVB4	586	431	0.02%	0.003%
93	12.852	3594	3596	3602	rBV3	559	676	0.03%	0.004%
94	13.106	3671	3675	3682	rVB3	681	726	0.03%	0.004%
95	13.232	3708	3714	3720	rBV3	1085	1265	0.06%	0.007%
96	13.396	3763	3765	3769	rBV3	558	379	0.02%	0.002%
97	13.508	3797	3800	3801	rBV	736	418	0.02%	0.002%
98	13.849	3902	3906	3910	rBV4	1709	1755	0.08%	0.010%
99	14.412	4077	4081	4084	rBV3	747	782	0.04%	0.005%
100	15.254	4338	4343	4347	rBV4	1464	1788	0.08%	0.010%


Sum of corrected areas: 17183010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055871.D
Acq On : 25 Oct 2023 11:56
Operator : MD/SY
Sample : 04952-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

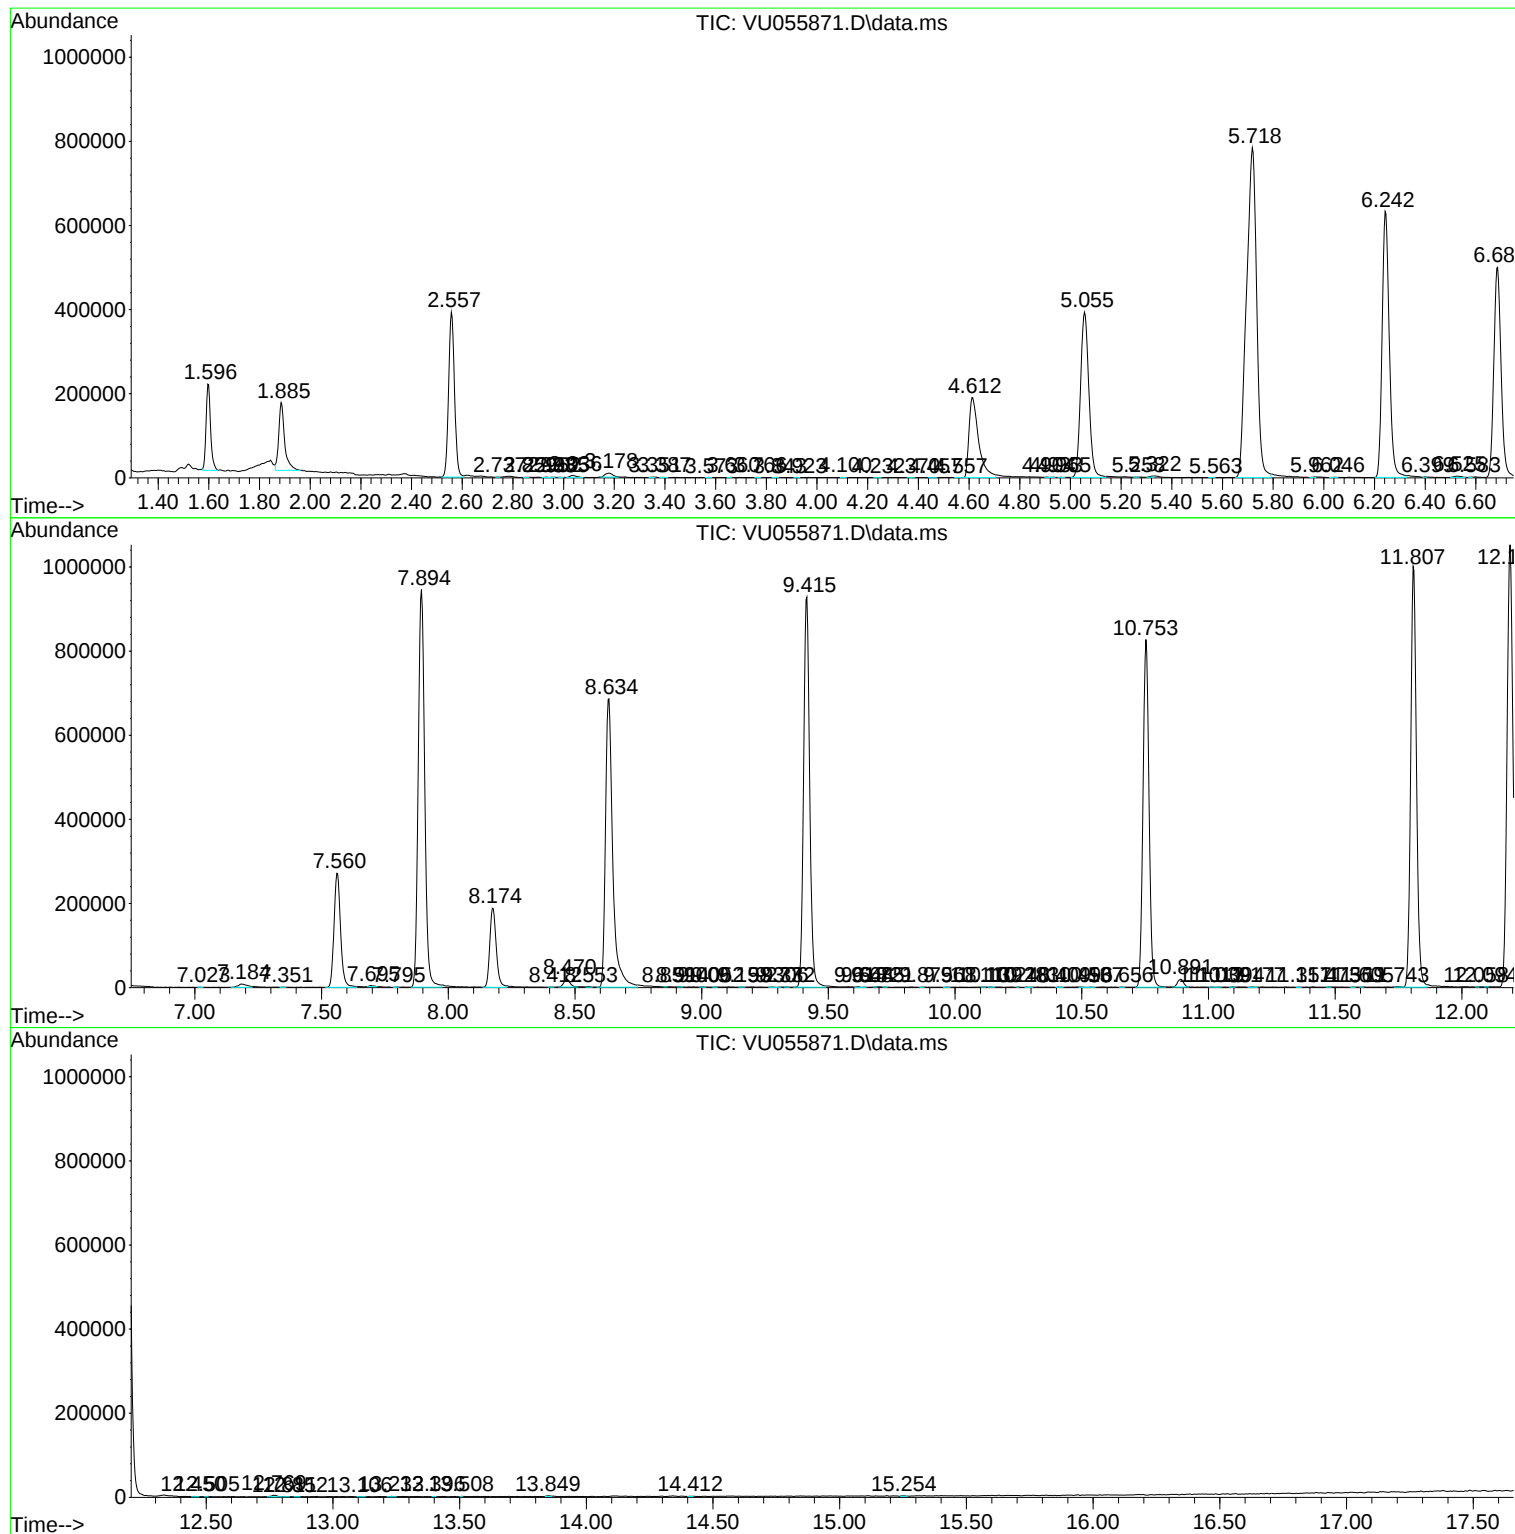

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055871.D
Acq On : 25 Oct 2023 11:56
Operator : MD/SY
Sample : 04952-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055871.D
Acq On : 25 Oct 2023 11:56
Operator : MD/SY
Sample : 04952-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc