

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055873.D
 Acq On : 25 Oct 2023 12:44
 Operator : MD/SY
 Sample : 04952-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	116	rVB	210666	264895	11.84%	1.510%
2	1.885	178	185	204	rVB	164310	250885	11.22%	1.430%
3	2.557	381	394	412	rBV	391113	643919	28.79%	3.671%
4	2.785	458	465	472	rBV3	2082	3151	0.14%	0.018%
5	2.930	506	510	511	rBV2	560	330	0.01%	0.002%
6	3.036	533	543	560	rVB8	3891	8324	0.37%	0.047%
7	3.123	566	570	574	rBV3	447	322	0.01%	0.002%
8	3.174	574	586	599	rBV3	4439	10243	0.46%	0.058%
9	3.316	627	630	635	rVB2	519	444	0.02%	0.003%
10	3.345	635	639	645	rBV	520	626	0.03%	0.004%
11	3.383	648	651	653	rBV	489	298	0.01%	0.002%
12	3.550	698	703	707	rVB2	302	302	0.01%	0.002%
13	3.595	711	717	722	rBV3	382	452	0.02%	0.003%
14	3.666	735	739	742	rBV	488	407	0.02%	0.002%
15	3.833	788	791	795	rVB3	592	434	0.02%	0.002%
16	4.007	839	845	848	rBV	401	354	0.02%	0.002%
17	4.075	861	866	870	rBV	337	318	0.01%	0.002%
18	4.161	887	893	897	rBV2	295	374	0.02%	0.002%
19	4.216	907	910	912	rVV2	503	294	0.01%	0.002%
20	4.245	916	919	926	rVB2	314	288	0.01%	0.002%
21	4.438	973	979	982	rBV2	310	343	0.02%	0.002%
22	4.509	996	1001	1003	rBV2	358	308	0.01%	0.002%
23	4.615	1022	1034	1066	rBV	199637	527016	23.56%	3.004%
24	5.055	1155	1171	1194	rBV	404172	903299	40.39%	5.149%
25	5.290	1240	1244	1246	rBV4	397	336	0.02%	0.002%
26	5.329	1246	1256	1267	rVB2	4395	9941	0.44%	0.057%
27	5.589	1333	1337	1339	rBV	327	275	0.01%	0.002%
28	5.718	1354	1377	1405	rBV2	806791	2236586	100.00%	12.750%
29	6.026	1469	1473	1475	rBV4	572	380	0.02%	0.002%
30	6.155	1510	1513	1518	rVB3	470	420	0.02%	0.002%
31	6.187	1521	1523	1527	rBV2	424	303	0.01%	0.002%
32	6.245	1527	1541	1568	rBV	636326	1237613	55.33%	7.055%
33	6.486	1612	1616	1618	rBV3	366	304	0.01%	0.002%
34	6.525	1621	1628	1639	rVB8	3800	5873	0.26%	0.033%
35	6.595	1645	1650	1659	rVB7	1465	2656	0.12%	0.015%
36	6.685	1664	1678	1702	rBV	514115	1025627	45.86%	5.847%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055873.D
 Acq On : 25 Oct 2023 12:44
 Operator : MD/SY
 Sample : 04952-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.972	1763	1767	1770	rBV2	475	431	0.02%	0.002%
38	7.078	1797	1800	1806	rVB4	494	485	0.02%	0.003%
39	7.123	1811	1814	1818	rBV	379	285	0.01%	0.002%
40	7.197	1820	1837	1847	rBV5	7748	20540	0.92%	0.117%
41	7.338	1878	1881	1886	rVB3	514	341	0.02%	0.002%
42	7.380	1886	1894	1896	rBV4	463	491	0.02%	0.003%
43	7.563	1931	1951	1974	rBV	276339	496688	22.21%	2.831%
44	7.695	1986	1992	2006	rVB4	4455	7576	0.34%	0.043%
45	7.782	2017	2019	2023	rBV2	327	277	0.01%	0.002%
46	7.801	2023	2025	2027	rBV2	613	286	0.01%	0.002%
47	7.894	2040	2054	2085	rBV	964625	1702277	76.11%	9.704%
48	8.174	2128	2141	2166	rBV	189678	339391	15.17%	1.935%
49	8.325	2184	2188	2190	rBV3	510	386	0.02%	0.002%
50	8.341	2190	2193	2194	rVV3	618	359	0.02%	0.002%
51	8.351	2194	2196	2201	rVV3	983	636	0.03%	0.004%
52	8.470	2222	2233	2242	rVV3	12226	21956	0.98%	0.125%
53	8.553	2257	2259	2263	rVB2	1444	746	0.03%	0.004%
54	8.634	2272	2284	2319	rBV	721889	1413918	63.22%	8.060%
55	8.878	2357	2360	2365	rVB3	537	372	0.02%	0.002%
56	8.901	2365	2367	2371	rBV3	495	327	0.01%	0.002%
57	8.949	2379	2382	2384	rVB	739	375	0.02%	0.002%
58	8.997	2395	2397	2400	rVV	778	560	0.03%	0.003%
59	9.013	2400	2402	2405	rVB3	841	486	0.02%	0.003%
60	9.113	2429	2433	2437	rVB3	894	744	0.03%	0.004%
61	9.161	2444	2448	2449	rBV2	545	362	0.02%	0.002%
62	9.290	2486	2488	2492	rBV2	547	334	0.01%	0.002%
63	9.415	2513	2527	2556	rBV	931348	1569050	70.15%	8.945%
64	9.576	2575	2577	2582	rVB4	993	687	0.03%	0.004%
65	9.688	2607	2612	2614	rBV4	778	636	0.03%	0.004%
66	9.750	2626	2631	2632	rBV3	474	379	0.02%	0.002%
67	9.824	2651	2654	2658	rBV2	396	302	0.01%	0.002%
68	9.962	2695	2697	2703	rVB2	301	273	0.01%	0.002%
69	10.123	2744	2747	2749	rVB3	561	300	0.01%	0.002%
70	10.151	2749	2756	2757	rBV3	537	454	0.02%	0.003%
71	10.242	2782	2784	2789	rBV2	355	271	0.01%	0.002%
72	10.338	2812	2814	2817	rBV2	394	321	0.01%	0.002%
73	10.473	2853	2856	2858	rBV	562	327	0.01%	0.002%
74	10.753	2927	2943	2968	rBV	848014	1392393	62.26%	7.938%
75	10.891	2976	2986	2998	rVB2	13076	21947	0.98%	0.125%
76	10.946	3000	3003	3007	rVB4	565	367	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055873.D
 Acq On : 25 Oct 2023 12:44
 Operator : MD/SY
 Sample : 04952-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.007	3019	3022	3026	rBV3	735	545	0.02%	0.003%
78	11.026	3026	3028	3033	rVB2	785	620	0.03%	0.004%
79	11.068	3039	3041	3045	rVB	569	348	0.02%	0.002%
80	11.119	3054	3057	3059	rBV	438	322	0.01%	0.002%
81	11.274	3099	3105	3108	rBV2	573	521	0.02%	0.003%
82	11.296	3108	3112	3117	rBV2	691	860	0.04%	0.005%
83	11.412	3145	3148	3153	rVB3	858	685	0.03%	0.004%
84	11.505	3174	3177	3184	rBV5	494	513	0.02%	0.003%
85	11.563	3192	3195	3198	rBV2	719	552	0.02%	0.003%
86	11.676	3226	3230	3232	rBV	364	332	0.01%	0.002%
87	11.811	3258	3272	3291	rBV	990906	1609672	71.97%	9.176%
88	12.077	3354	3355	3361	rBV5	576	460	0.02%	0.003%
89	12.190	3376	3390	3412	rBV	1093181	1781726	79.66%	10.157%
90	12.505	3483	3488	3491	rBV2	731	736	0.03%	0.004%
91	12.762	3563	3568	3569	rBV2	2135	1755	0.08%	0.010%
92	12.807	3580	3582	3586	rVB3	636	348	0.02%	0.002%
93	13.007	3641	3644	3648	rBV3	720	624	0.03%	0.004%
94	13.055	3657	3659	3664	rVB2	489	297	0.01%	0.002%
95	13.235	3713	3715	3719	rBV2	739	393	0.02%	0.002%
96	13.412	3766	3770	3774	rBV2	589	568	0.03%	0.003%
97	13.454	3777	3783	3785	rBV4	849	702	0.03%	0.004%
98	13.743	3871	3873	3879	rVB2	593	350	0.02%	0.002%
99	13.856	3901	3908	3910	rBV4	1889	1739	0.08%	0.010%
100	15.116	4297	4300	4303	rBV5	1307	978	0.04%	0.006%




Sum of corrected areas: 17541922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055873.D
Acq On : 25 Oct 2023 12:44
Operator : MD/SY
Sample : 04952-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

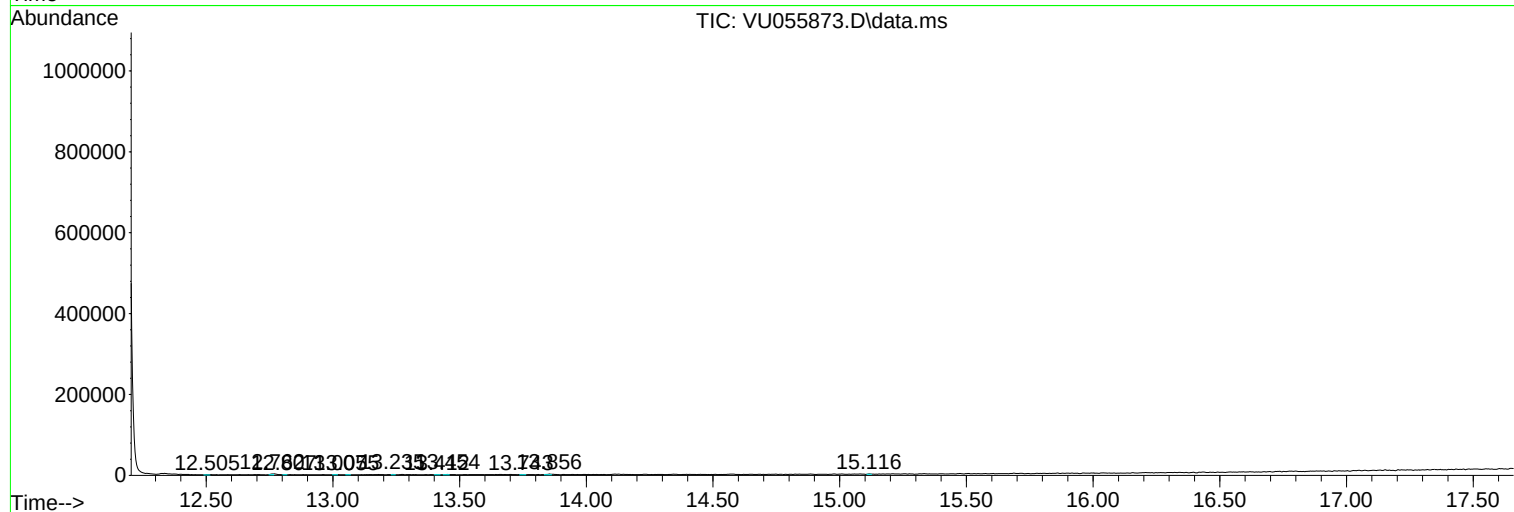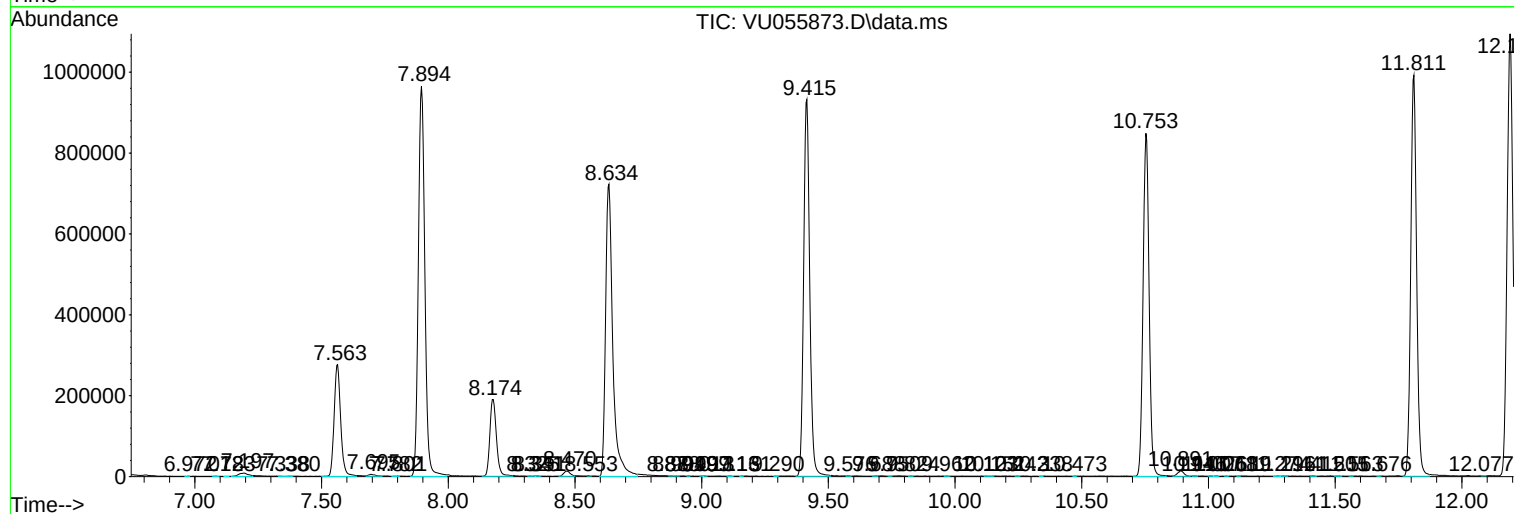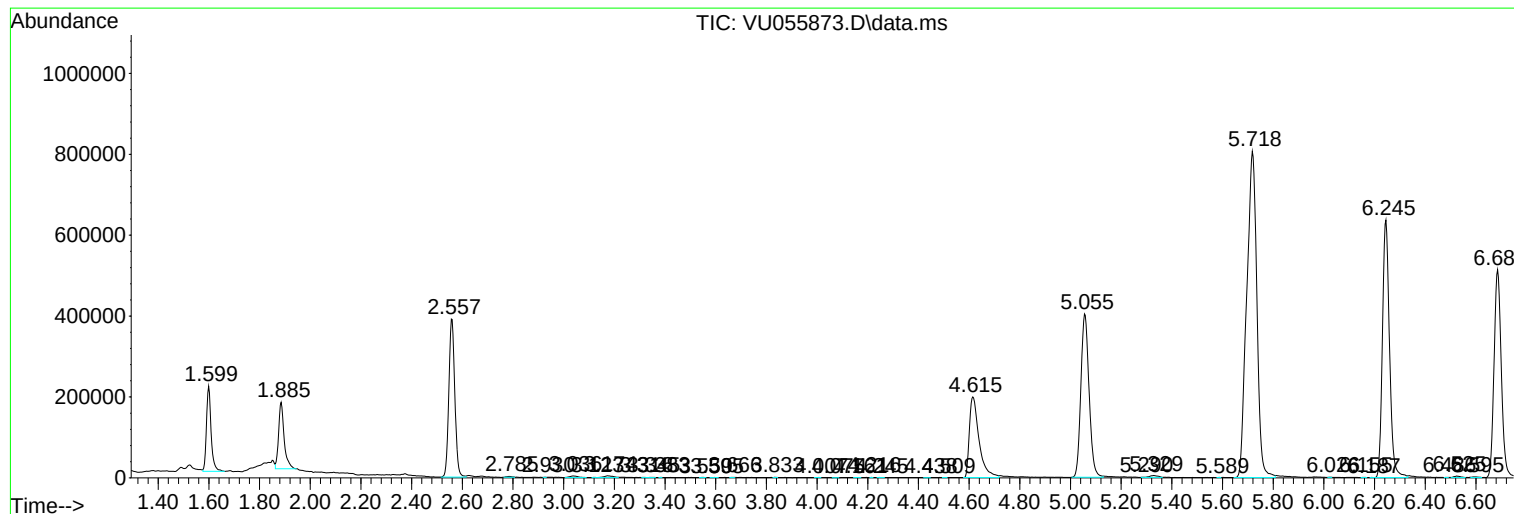

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055873.D
Acq On : 25 Oct 2023 12:44
Operator : MD/SY
Sample : 04952-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055873.D
Acq On : 25 Oct 2023 12:44
Operator : MD/SY
Sample : 04952-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------