

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055874.D
 Acq On : 25 Oct 2023 13:08
 Operator : MD/SY
 Sample : 04952-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	109	rVB	206702	241728	10.85%	1.367%
2	1.888	178	186	209	rVB	163788	263518	11.83%	1.490%
3	2.560	382	395	410	rBV	387723	636225	28.55%	3.597%
4	2.676	424	431	441	rVB8	3201	5575	0.25%	0.032%
5	2.785	452	465	482	rVB3	3386	7483	0.34%	0.042%
6	2.856	482	487	489	rVB2	519	425	0.02%	0.002%
7	2.885	493	496	498	rBV2	509	356	0.02%	0.002%
8	2.904	499	502	506	rVB3	863	592	0.03%	0.003%
9	2.930	506	510	512	rBV3	507	421	0.02%	0.002%
10	3.043	534	545	557	rVB5	4585	9099	0.41%	0.051%
11	3.171	575	585	586	rBV2	3487	3778	0.17%	0.021%
12	3.573	707	710	714	rVB2	434	281	0.01%	0.002%
13	3.592	714	716	724	rBV2	429	573	0.03%	0.003%
14	3.637	728	730	736	rVB2	422	326	0.01%	0.002%
15	3.682	740	744	747	rBV	573	505	0.02%	0.003%
16	3.837	787	792	794	rBV	406	346	0.02%	0.002%
17	4.046	853	857	863	rVB	492	500	0.02%	0.003%
18	4.088	863	870	871	rBV	452	461	0.02%	0.003%
19	4.113	875	878	886	rVB2	367	385	0.02%	0.002%
20	4.306	934	938	942	rVV	421	457	0.02%	0.003%
21	4.335	943	947	952	rVV3	633	504	0.02%	0.003%
22	4.615	1018	1034	1062	rBV	204690	536394	24.07%	3.033%
23	4.901	1120	1123	1124	rBV	478	273	0.01%	0.002%
24	5.055	1155	1171	1198	rBV	401530	907887	40.75%	5.133%
25	5.332	1243	1257	1275	rVB3	5233	14494	0.65%	0.082%
26	5.406	1275	1280	1284	rVV3	369	414	0.02%	0.002%
27	5.531	1315	1319	1324	rVB2	432	339	0.02%	0.002%
28	5.718	1356	1377	1408	rBV2	798236	2228120	100.00%	12.598%
29	6.042	1474	1478	1484	rVB3	829	911	0.04%	0.005%
30	6.123	1500	1503	1507	rVB2	975	705	0.03%	0.004%
31	6.184	1517	1522	1526	rVB2	572	440	0.02%	0.002%
32	6.245	1526	1541	1567	rBV	644401	1262056	56.64%	7.136%
33	6.522	1619	1627	1640	rVB9	2911	5992	0.27%	0.034%
34	6.592	1640	1649	1657	rBV6	1796	3169	0.14%	0.018%
35	6.686	1663	1678	1699	rBV	515987	1021424	45.84%	5.775%
36	6.898	1741	1744	1747	rVB2	798	438	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055874.D
 Acq On : 25 Oct 2023 13:08
 Operator : MD/SY
 Sample : 04952-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.962	1762	1764	1768	rVB3	668	381	0.02%	0.002%
38	7.062	1791	1795	1798	rBV	337	339	0.02%	0.002%
39	7.120	1809	1813	1817	rBV2	281	273	0.01%	0.002%
40	7.184	1817	1833	1850	rBV6	8290	21981	0.99%	0.124%
41	7.293	1865	1867	1871	rVB2	674	424	0.02%	0.002%
42	7.312	1871	1873	1876	rBV2	416	341	0.02%	0.002%
43	7.563	1938	1951	1976	rBV	271812	494603	22.20%	2.796%
44	7.698	1987	1993	2005	rVB5	3171	5459	0.25%	0.031%
45	7.788	2019	2021	2023	rVV2	478	278	0.01%	0.002%
46	7.808	2024	2027	2033	rVB3	892	702	0.03%	0.004%
47	7.843	2036	2038	2041	rBV	466	386	0.02%	0.002%
48	7.894	2041	2054	2091	rBV	977657	1710515	76.77%	9.671%
49	8.177	2129	2142	2158	rBV	199982	340448	15.28%	1.925%
50	8.296	2177	2179	2182	rVB2	673	324	0.01%	0.002%
51	8.351	2193	2196	2203	rVB3	984	807	0.04%	0.005%
52	8.383	2203	2206	2210	rVB3	490	381	0.02%	0.002%
53	8.422	2214	2218	2221	rBV4	749	676	0.03%	0.004%
54	8.470	2221	2233	2240	rBV	10595	19179	0.86%	0.108%
55	8.557	2253	2260	2266	rVB7	1903	2314	0.10%	0.013%
56	8.631	2270	2283	2320	rBV	727449	1444495	64.83%	8.167%
57	8.930	2372	2376	2383	rBV4	958	1035	0.05%	0.006%
58	8.968	2384	2388	2390	rVV5	508	345	0.02%	0.002%
59	9.033	2405	2408	2411	rBV5	527	393	0.02%	0.002%
60	9.065	2413	2418	2421	rBV3	404	335	0.02%	0.002%
61	9.203	2457	2461	2464	rBV2	581	496	0.02%	0.003%
62	9.303	2490	2492	2495	rBV2	505	308	0.01%	0.002%
63	9.335	2498	2502	2503	rBV2	408	278	0.01%	0.002%
64	9.415	2513	2527	2554	rBV	979576	1623053	72.84%	9.177%
65	9.711	2617	2619	2622	rVB2	1108	606	0.03%	0.003%
66	9.727	2622	2624	2627	rVB	706	290	0.01%	0.002%
67	9.856	2662	2664	2668	rVB4	614	340	0.02%	0.002%
68	10.110	2741	2743	2747	rVB3	762	365	0.02%	0.002%
69	10.129	2747	2749	2753	rBV2	672	510	0.02%	0.003%
70	10.174	2760	2763	2766	rBV2	493	353	0.02%	0.002%
71	10.660	2910	2914	2917	rBV	512	384	0.02%	0.002%
72	10.753	2929	2943	2966	rBV	866429	1420699	63.76%	8.033%
73	10.891	2978	2986	2995	rVB3	9469	14773	0.66%	0.084%
74	10.959	3004	3007	3010	rBV	371	302	0.01%	0.002%
75	11.065	3035	3040	3042	rVB2	408	374	0.02%	0.002%
76	11.081	3042	3045	3047	rBV2	526	340	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055874.D
 Acq On : 25 Oct 2023 13:08
 Operator : MD/SY
 Sample : 04952-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.200	3079	3082	3084	rBV	495	325	0.01%	0.002%
78	11.383	3135	3139	3143	rBV2	522	402	0.02%	0.002%
79	11.409	3143	3147	3150	rBV3	1195	888	0.04%	0.005%
80	11.467	3162	3165	3166	rBV	559	345	0.02%	0.002%
81	11.489	3170	3172	3177	rVB	637	491	0.02%	0.003%
82	11.570	3194	3197	3202	rBV2	526	600	0.03%	0.003%
83	11.811	3259	3272	3292	rBV	1010573	1634124	73.34%	9.239%
84	12.061	3348	3350	3351	rBV	641	295	0.01%	0.002%
85	12.190	3373	3390	3419	rBV	1097828	1774430	79.64%	10.033%
86	12.766	3565	3569	3570	rBV	1606	1183	0.05%	0.007%
87	12.833	3586	3590	3595	rBV3	511	637	0.03%	0.004%
88	12.856	3595	3597	3598	rBV	627	277	0.01%	0.002%
89	12.894	3606	3609	3610	rBV2	701	365	0.02%	0.002%
90	12.971	3630	3633	3637	rBV3	580	462	0.02%	0.003%
91	13.036	3651	3653	3656	rVB3	770	284	0.01%	0.002%
92	13.113	3674	3677	3679	rBV	565	353	0.02%	0.002%
93	13.187	3698	3700	3703	rVB2	797	384	0.02%	0.002%
94	13.502	3794	3798	3800	rBV2	518	410	0.02%	0.002%
95	13.807	3889	3893	3896	rBV4	812	538	0.02%	0.003%
96	14.238	4025	4027	4032	rVB4	677	375	0.02%	0.002%
97	14.335	4055	4057	4059	rBV2	742	423	0.02%	0.002%
98	14.457	4092	4095	4097	rBV2	772	393	0.02%	0.002%
99	14.537	4117	4120	4122	rBV3	1000	616	0.03%	0.003%
100	15.476	4409	4412	4417	rBV4	1473	1659	0.07%	0.009%




Sum of corrected areas: 17686738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055874.D
Acq On : 25 Oct 2023 13:08
Operator : MD/SY
Sample : 04952-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

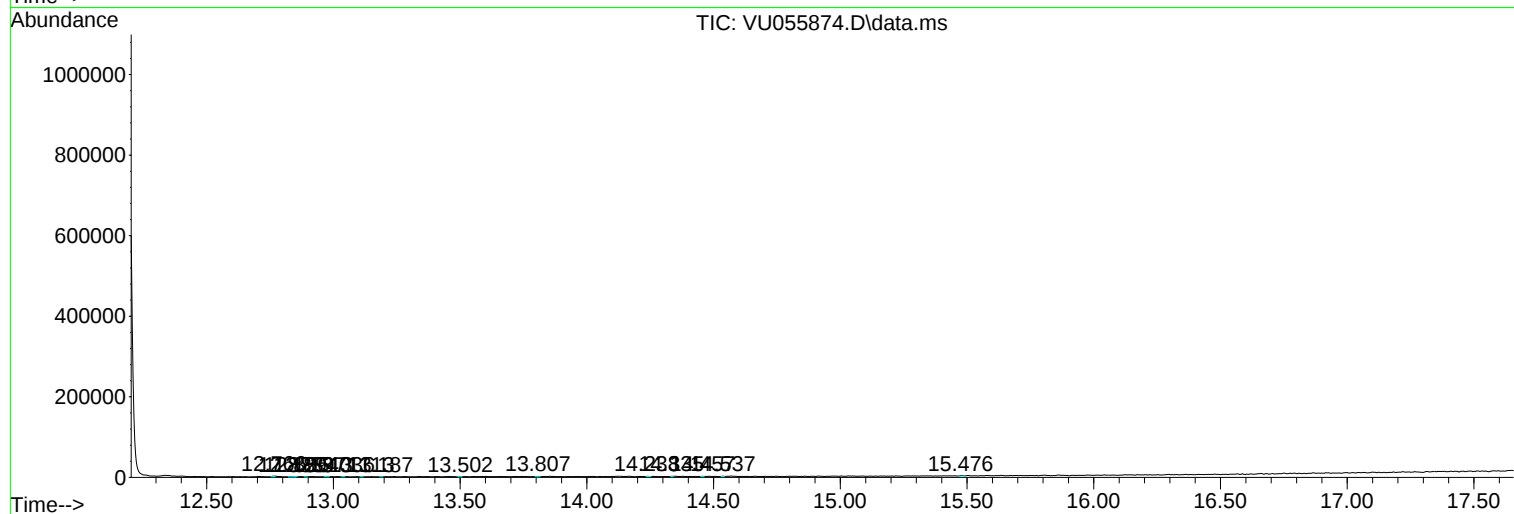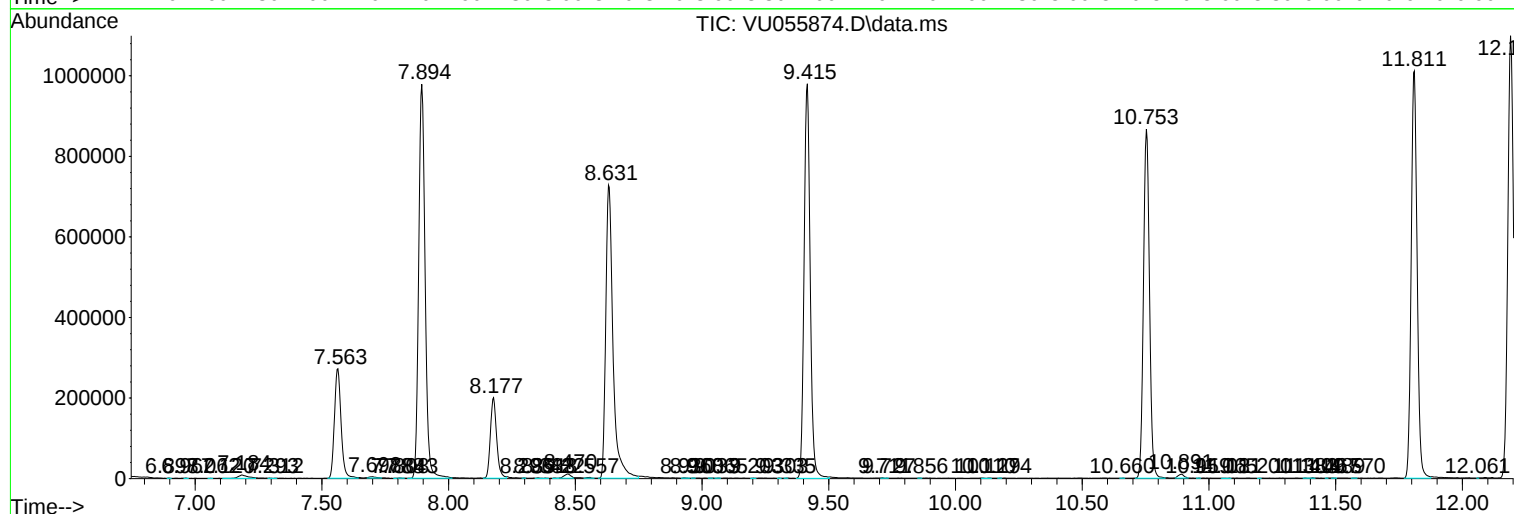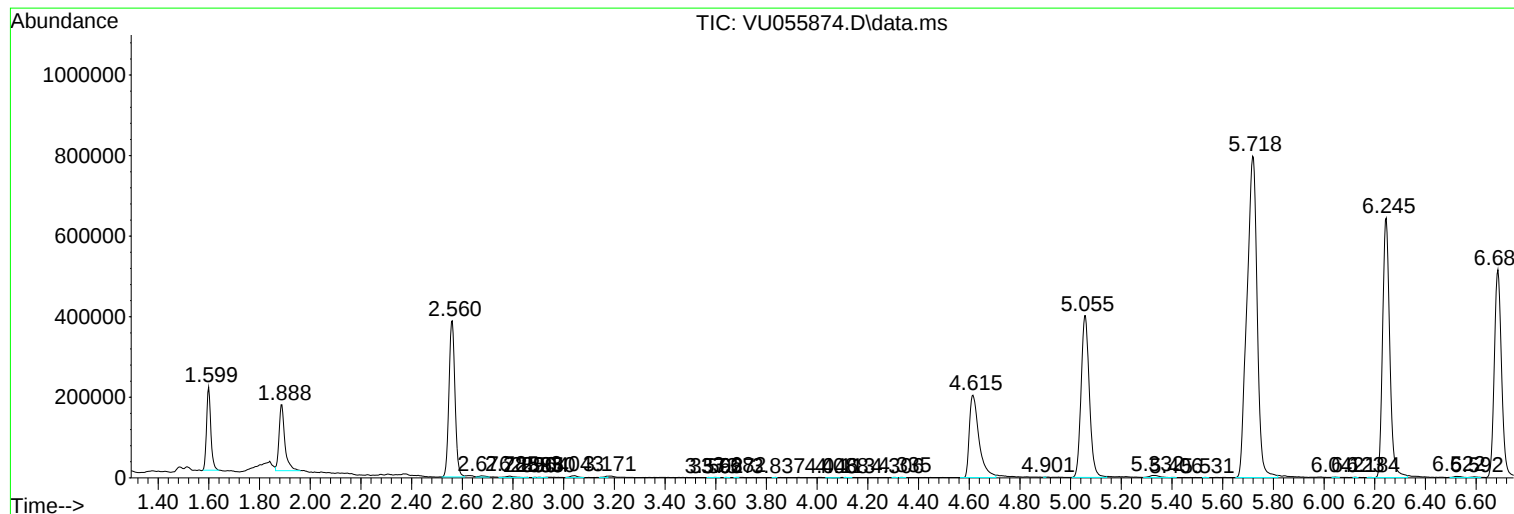

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055874.D
Acq On : 25 Oct 2023 13:08
Operator : MD/SY
Sample : 04952-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055874.D
Acq On : 25 Oct 2023 13:08
Operator : MD/SY
Sample : 04952-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------