

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055875.D
 Acq On : 25 Oct 2023 13:32
 Operator : MD/SY
 Sample : 04952-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	111	rVB	207634	247792	11.16%	1.418%
2	1.885	178	185	202	rVB	159461	240506	10.84%	1.376%
3	2.557	382	394	411	rBV	385866	637311	28.71%	3.647%
4	2.785	460	465	478	rVB2	2730	4587	0.21%	0.026%
5	2.907	501	503	507	rBV2	583	503	0.02%	0.003%
6	2.943	510	514	517	rBV4	449	429	0.02%	0.002%
7	3.039	534	544	558	rVB5	4190	8714	0.39%	0.050%
8	3.177	576	587	600	rBV4	3060	7856	0.35%	0.045%
9	3.319	629	631	634	rVV	473	369	0.02%	0.002%
10	3.428	660	665	670	rVB2	625	527	0.02%	0.003%
11	3.595	709	717	723	rBV3	560	859	0.04%	0.005%
12	3.663	732	738	739	rBV	704	476	0.02%	0.003%
13	3.692	745	747	754	rVB3	843	786	0.04%	0.004%
14	3.756	759	767	771	rBV	563	689	0.03%	0.004%
15	3.866	795	801	803	rBV2	437	427	0.02%	0.002%
16	4.267	924	926	930	rBV	519	376	0.02%	0.002%
17	4.502	994	999	1007	rVB2	482	487	0.02%	0.003%
18	4.615	1023	1034	1069	rBV	200197	521461	23.49%	2.984%
19	5.055	1155	1171	1204	rBV	400388	900067	40.55%	5.151%
20	5.329	1247	1256	1273	rVB4	5308	13825	0.62%	0.079%
21	5.505	1308	1311	1316	rBV2	609	592	0.03%	0.003%
22	5.554	1323	1326	1330	rVB3	680	468	0.02%	0.003%
23	5.576	1330	1333	1336	rBV	526	374	0.02%	0.002%
24	5.718	1355	1377	1410	rBV2	797875	2219477	100.00%	12.701%
25	5.962	1449	1453	1455	rBV4	1019	736	0.03%	0.004%
26	6.029	1471	1474	1475	rBV	578	343	0.02%	0.002%
27	6.123	1498	1503	1506	rBV2	636	471	0.02%	0.003%
28	6.177	1517	1520	1524	rVB3	595	456	0.02%	0.003%
29	6.245	1524	1541	1566	rBV	641877	1241215	55.92%	7.103%
30	6.525	1619	1628	1631	rBV7	2983	3825	0.17%	0.022%
31	6.586	1637	1647	1649	rBV4	1404	1775	0.08%	0.010%
32	6.685	1663	1678	1704	rBV	510279	1013564	45.67%	5.800%
33	6.872	1734	1736	1742	rVB4	743	511	0.02%	0.003%
34	6.949	1757	1760	1765	rBV2	442	357	0.02%	0.002%
35	6.991	1770	1773	1780	rVB3	466	415	0.02%	0.002%
36	7.100	1801	1807	1812	rVB2	620	603	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055875.D
 Acq On : 25 Oct 2023 13:32
 Operator : MD/SY
 Sample : 04952-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.187	1820	1834	1859	rBV6	7624	21326	0.96%	0.122%
38	7.283	1862	1864	1869	rVB3	886	780	0.04%	0.004%
39	7.335	1877	1880	1883	rBV2	396	322	0.01%	0.002%
40	7.454	1912	1917	1921	rVB3	411	419	0.02%	0.002%
41	7.560	1938	1950	1967	rBV	273432	489487	22.05%	2.801%
42	7.701	1986	1994	2004	rVB4	2760	5635	0.25%	0.032%
43	7.788	2015	2021	2023	rBV3	900	1001	0.05%	0.006%
44	7.798	2023	2024	2028	rVB4	502	337	0.02%	0.002%
45	7.894	2040	2054	2091	rBV	954542	1675155	75.48%	9.586%
46	8.174	2130	2141	2171	rBV	191961	336787	15.17%	1.927%
47	8.312	2181	2184	2187	rBV2	486	414	0.02%	0.002%
48	8.380	2202	2205	2209	rBV2	579	431	0.02%	0.002%
49	8.470	2223	2233	2242	rBV3	7838	14896	0.67%	0.085%
50	8.544	2253	2256	2259	rBV4	998	709	0.03%	0.004%
51	8.634	2271	2284	2326	rBV	730201	1425888	64.24%	8.160%
52	8.971	2386	2389	2390	rBV2	826	480	0.02%	0.003%
53	9.123	2432	2436	2439	rBV3	469	433	0.02%	0.002%
54	9.145	2440	2443	2444	rVV3	626	344	0.02%	0.002%
55	9.161	2444	2448	2454	rVB4	497	604	0.03%	0.003%
56	9.225	2466	2468	2472	rVB2	645	371	0.02%	0.002%
57	9.341	2502	2504	2509	rVB2	646	444	0.02%	0.003%
58	9.412	2512	2526	2552	rBV	943889	1588101	71.55%	9.088%
59	9.701	2614	2616	2620	rVB2	861	546	0.02%	0.003%
60	9.827	2653	2655	2661	rVB3	648	495	0.02%	0.003%
61	9.875	2668	2670	2675	rVB3	555	383	0.02%	0.002%
62	10.068	2727	2730	2733	rVV	684	514	0.02%	0.003%
63	10.161	2756	2759	2763	rBV	721	555	0.03%	0.003%
64	10.187	2763	2767	2769	rBV3	645	511	0.02%	0.003%
65	10.753	2930	2943	2972	rBV	850098	1403221	63.22%	8.030%
66	10.888	2976	2985	2998	rVB3	7990	13575	0.61%	0.078%
67	10.981	3009	3014	3019	rBV3	592	677	0.03%	0.004%
68	11.058	3035	3038	3043	rBV	419	440	0.02%	0.003%
69	11.084	3043	3046	3050	rVB	581	411	0.02%	0.002%
70	11.122	3053	3058	3059	rBV	532	438	0.02%	0.003%
71	11.251	3096	3098	3104	rVB2	501	445	0.02%	0.003%
72	11.412	3146	3148	3152	rVB2	617	351	0.02%	0.002%
73	11.540	3183	3188	3192	rBV2	454	432	0.02%	0.002%
74	11.563	3192	3195	3199	rBV3	402	353	0.02%	0.002%
75	11.663	3223	3226	3232	rBV2	426	425	0.02%	0.002%
76	11.730	3242	3247	3250	rBV2	894	882	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055875.D
 Acq On : 25 Oct 2023 13:32
 Operator : MD/SY
 Sample : 04952-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.811	3259	3272	3294	rBV	1010857	1633753	73.61%	9.349%
78	12.032	3339	3341	3348	rVB5	669	569	0.03%	0.003%
79	12.065	3348	3351	3353	rVB3	684	394	0.02%	0.002%
80	12.094	3354	3360	3362	rBV5	1150	1101	0.05%	0.006%
81	12.106	3362	3364	3370	rVB5	929	620	0.03%	0.004%
82	12.190	3376	3390	3413	rBV	1062875	1766073	79.57%	10.106%
83	12.470	3475	3477	3480	rBV2	831	560	0.03%	0.003%
84	12.753	3561	3565	3566	rBV2	949	645	0.03%	0.004%
85	13.039	3652	3654	3660	rVB4	931	743	0.03%	0.004%
86	13.065	3660	3662	3665	rBV2	735	382	0.02%	0.002%
87	13.145	3684	3687	3688	rBV	609	370	0.02%	0.002%
88	13.306	3733	3737	3741	rBV3	703	772	0.03%	0.004%
89	13.711	3860	3863	3869	rBV3	603	536	0.02%	0.003%
90	13.740	3870	3872	3874	rVB2	775	322	0.01%	0.002%
91	13.759	3874	3878	3879	rBV	504	407	0.02%	0.002%
92	13.849	3902	3906	3907	rBV4	832	606	0.03%	0.003%
93	13.955	3937	3939	3942	rBV	591	329	0.01%	0.002%
94	14.161	4001	4003	4005	rBV3	644	353	0.02%	0.002%
95	14.447	4089	4092	4096	rVB4	1165	891	0.04%	0.005%
96	14.466	4096	4098	4099	rBV	1506	410	0.02%	0.002%
97	14.708	4171	4173	4175	rBV3	885	431	0.02%	0.002%
98	14.753	4185	4187	4191	rBV4	746	625	0.03%	0.004%
99	14.810	4202	4205	4211	rBV4	1246	1428	0.06%	0.008%
100	15.090	4290	4292	4296	rBV2	809	616	0.03%	0.004%




Sum of corrected areas: 17475183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055875.D
Acq On : 25 Oct 2023 13:32
Operator : MD/SY
Sample : 04952-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

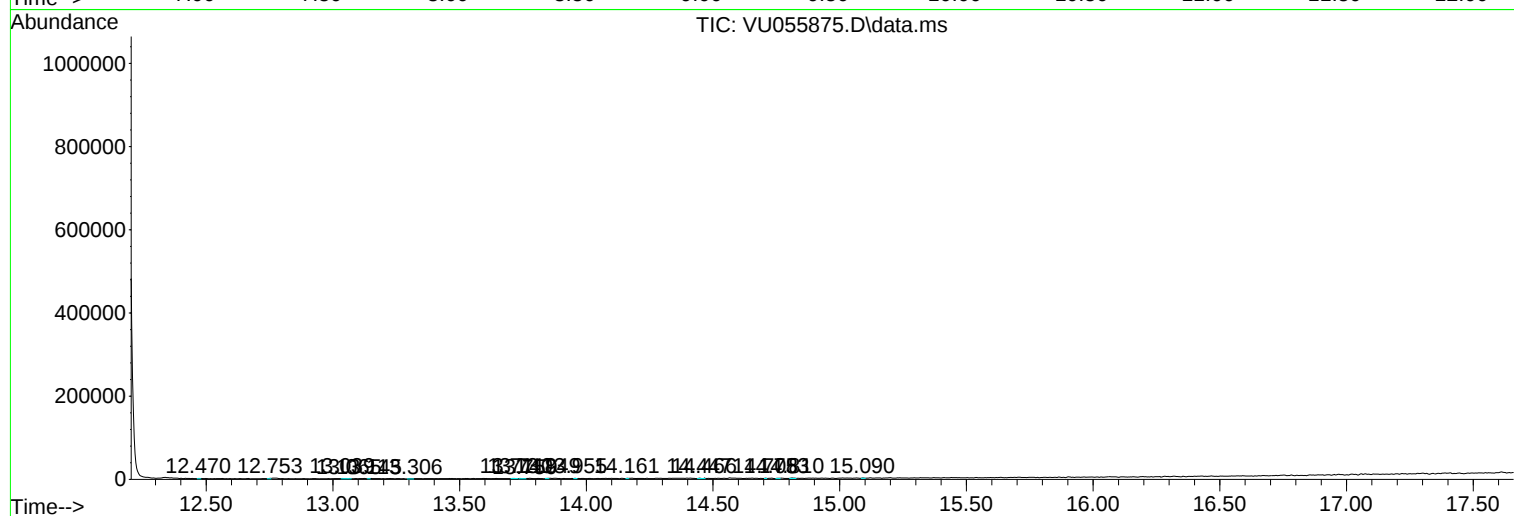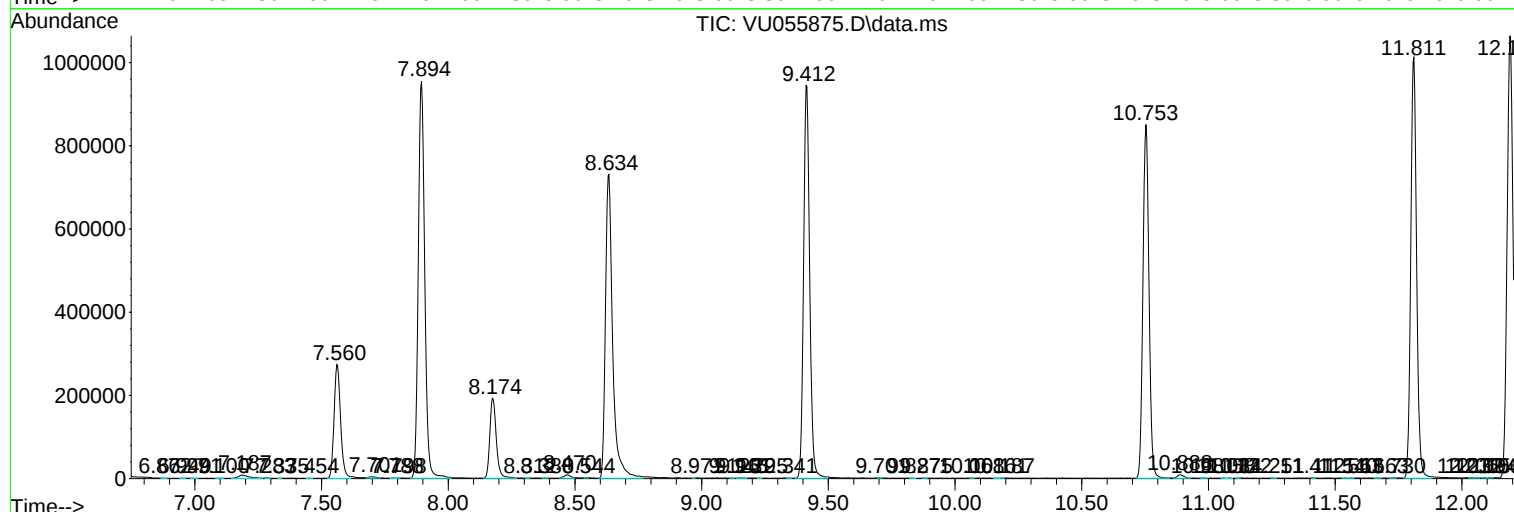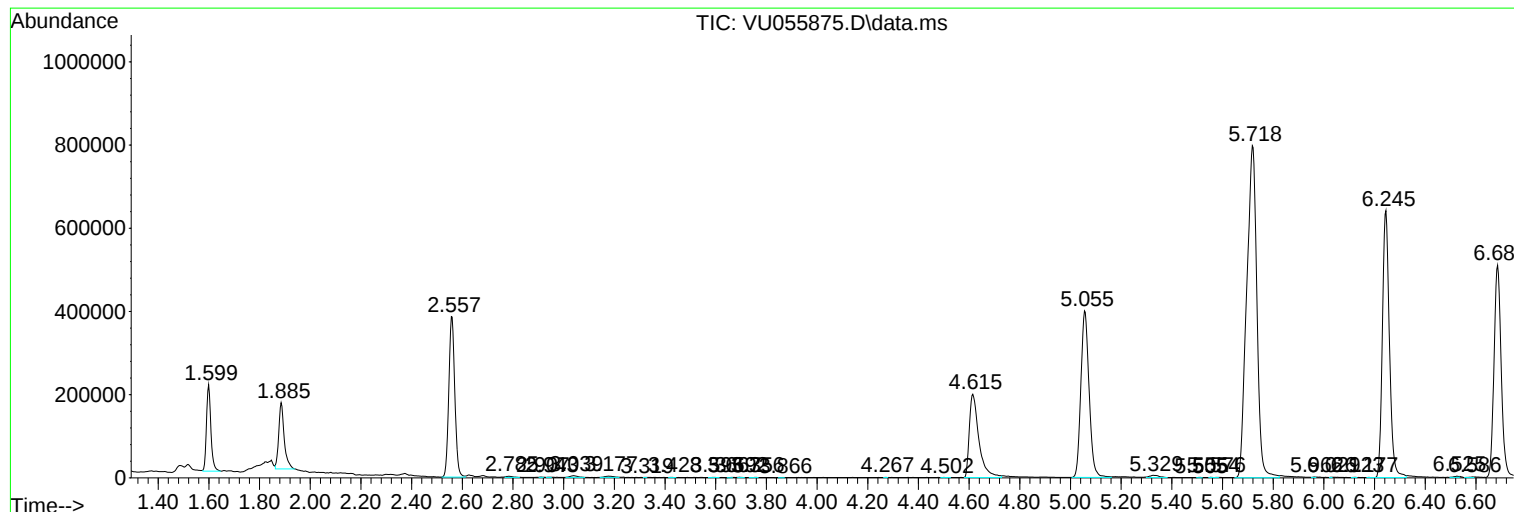

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055875.D
Acq On : 25 Oct 2023 13:32
Operator : MD/SY
Sample : 04952-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055875.D
Acq On : 25 Oct 2023 13:32
Operator : MD/SY
Sample : 04952-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------