

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055876.D
 Acq On : 25 Oct 2023 13:56
 Operator : MD/SY
 Sample : VIBLK036
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	115	rVB	197695	238404	11.19%	1.375%
2	1.885	178	185	206	rVB	154396	248617	11.67%	1.434%
3	2.557	382	394	408	rBV	369829	605611	28.43%	3.494%
4	2.621	410	414	426	rVB	9526	15494	0.73%	0.089%
5	2.785	459	465	474	rVB	2207	3440	0.16%	0.020%
6	2.895	492	499	502	rBV4	1603	2225	0.10%	0.013%
7	2.959	517	519	523	rVB3	735	424	0.02%	0.002%
8	3.042	533	545	555	rBV5	4890	9302	0.44%	0.054%
9	3.177	578	587	589	rBV4	3816	5450	0.26%	0.031%
10	3.300	620	625	629	rBV2	499	604	0.03%	0.003%
11	3.708	750	752	760	rVB	760	772	0.04%	0.004%
12	3.756	760	767	769	rBV	354	440	0.02%	0.003%
13	3.997	838	842	843	rBV	1217	623	0.03%	0.004%
14	4.515	1000	1003	1008	rVB3	506	451	0.02%	0.003%
15	4.615	1014	1034	1068	rBV	196122	521545	24.48%	3.009%
16	4.994	1149	1152	1154	rBV2	679	456	0.02%	0.003%
17	5.055	1155	1171	1199	rVV	380322	872770	40.97%	5.035%
18	5.261	1232	1235	1238	rVB3	654	430	0.02%	0.002%
19	5.329	1246	1256	1269	rBV3	5404	11832	0.56%	0.068%
20	5.377	1269	1271	1279	rVB4	1186	1229	0.06%	0.007%
21	5.419	1279	1284	1286	rBV2	644	537	0.03%	0.003%
22	5.489	1303	1306	1311	rVB2	481	393	0.02%	0.002%
23	5.531	1316	1319	1324	rBV	445	379	0.02%	0.002%
24	5.586	1332	1336	1343	rBV3	549	487	0.02%	0.003%
25	5.718	1354	1377	1408	rBV2	770075	2130178	100.00%	12.289%
26	5.981	1457	1459	1463	rVB3	975	525	0.02%	0.003%
27	6.113	1497	1500	1502	rBV2	473	385	0.02%	0.002%
28	6.245	1527	1541	1564	rBV	687070	1320438	61.99%	7.617%
29	6.425	1595	1597	1601	rVB2	789	415	0.02%	0.002%
30	6.528	1621	1629	1638	rBV10	3011	5490	0.26%	0.032%
31	6.685	1664	1678	1699	rBV	492446	974595	45.75%	5.622%
32	6.804	1710	1715	1726	rVB8	2335	3520	0.17%	0.020%
33	6.885	1737	1740	1745	rBV4	835	962	0.05%	0.006%
34	6.975	1764	1768	1771	rBV3	409	373	0.02%	0.002%
35	7.029	1781	1785	1788	rBV2	601	491	0.02%	0.003%
36	7.119	1808	1813	1821	rBV6	1592	2290	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055876.D
 Acq On : 25 Oct 2023 13:56
 Operator : MD/SY
 Sample : VIBLK036
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.184	1823	1833	1835	rBV5	5914	7726	0.36%	0.045%
38	7.399	1898	1900	1905	rVB	534	423	0.02%	0.002%
39	7.483	1922	1926	1929	rBV3	667	467	0.02%	0.003%
40	7.560	1937	1950	1969	rBV	264695	474304	22.27%	2.736%
41	7.695	1984	1992	2007	rVB6	3567	7907	0.37%	0.046%
42	7.894	2040	2054	2073	rBV	924106	1605240	75.36%	9.260%
43	8.103	2117	2119	2127	rVB3	971	1051	0.05%	0.006%
44	8.177	2127	2142	2163	rBV	188371	330397	15.51%	1.906%
45	8.338	2189	2192	2196	rVB3	1164	957	0.04%	0.006%
46	8.364	2196	2200	2201	rBV2	739	387	0.02%	0.002%
47	8.470	2218	2233	2243	rBV3	7482	14018	0.66%	0.081%
48	8.553	2257	2259	2262	rVB2	1213	538	0.03%	0.003%
49	8.631	2270	2283	2318	rBV	711975	1385139	65.02%	7.991%
50	8.795	2325	2334	2347	rVB8	9419	19061	0.89%	0.110%
51	8.978	2387	2391	2395	rBV3	607	580	0.03%	0.003%
52	8.997	2395	2397	2401	rBV	801	495	0.02%	0.003%
53	9.074	2418	2421	2424	rVV3	859	646	0.03%	0.004%
54	9.097	2425	2428	2430	rVV2	857	483	0.02%	0.003%
55	9.113	2431	2433	2437	rVV4	670	397	0.02%	0.002%
56	9.274	2479	2483	2486	rBV2	446	375	0.02%	0.002%
57	9.332	2497	2501	2502	rBV2	648	493	0.02%	0.003%
58	9.415	2513	2527	2559	rBV	987279	1679542	78.85%	9.689%
59	9.698	2611	2615	2620	rVB4	1182	1170	0.05%	0.007%
60	9.817	2649	2652	2656	rVB2	835	581	0.03%	0.003%
61	9.852	2656	2663	2666	rBV3	925	967	0.05%	0.006%
62	9.930	2681	2687	2692	rBV3	530	667	0.03%	0.004%
63	10.090	2734	2737	2739	rBV4	575	379	0.02%	0.002%
64	10.187	2763	2767	2771	rBV4	855	740	0.03%	0.004%
65	10.242	2781	2784	2791	rBV2	703	850	0.04%	0.005%
66	10.274	2791	2794	2797	rBV3	554	379	0.02%	0.002%
67	10.328	2801	2811	2813	rBV4	3089	3629	0.17%	0.021%
68	10.418	2837	2839	2842	rVB2	889	484	0.02%	0.003%
69	10.489	2858	2861	2869	rVB5	840	898	0.04%	0.005%
70	10.685	2919	2922	2924	rBV5	574	414	0.02%	0.002%
71	10.753	2930	2943	2966	rBV	840743	1369203	64.28%	7.899%
72	10.891	2978	2986	2996	rVB3	6358	9966	0.47%	0.057%
73	11.052	3031	3036	3037	rBV2	548	489	0.02%	0.003%
74	11.412	3146	3148	3152	rVB4	1148	797	0.04%	0.005%
75	11.489	3167	3172	3173	rBV2	1221	951	0.04%	0.005%
76	11.637	3216	3218	3224	rVB3	602	386	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055876.D
 Acq On : 25 Oct 2023 13:56
 Operator : MD/SY
 Sample : VIBLK036
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.708	3227	3240	3243	rBV6	2099	3531	0.17%	0.020%
78	11.807	3257	3271	3302	rBV	1056149	1708650	80.21%	9.857%
79	12.010	3331	3334	3335	rBV3	709	423	0.02%	0.002%
80	12.084	3351	3357	3359	rBV3	1293	1293	0.06%	0.007%
81	12.190	3375	3390	3418	rBV	1036540	1698243	79.72%	9.797%
82	12.444	3467	3469	3472	rBV3	850	510	0.02%	0.003%
83	12.489	3479	3483	3485	rBV3	947	798	0.04%	0.005%
84	12.502	3485	3487	3492	rVB	1127	676	0.03%	0.004%
85	12.537	3495	3498	3503	rBV4	672	680	0.03%	0.004%
86	12.614	3520	3522	3527	rBV4	809	567	0.03%	0.003%
87	12.701	3546	3549	3553	rBV3	722	534	0.03%	0.003%
88	12.769	3563	3570	3574	rBV5	1010	1389	0.07%	0.008%
89	12.901	3604	3611	3614	rBV5	2582	3052	0.14%	0.018%
90	13.003	3640	3643	3645	rBV2	586	399	0.02%	0.002%
91	13.081	3663	3667	3671	rBV3	608	647	0.03%	0.004%
92	13.386	3760	3762	3768	rVB2	593	391	0.02%	0.002%
93	13.669	3846	3850	3855	rBV3	618	742	0.03%	0.004%
94	13.852	3902	3907	3909	rBV3	1070	1046	0.05%	0.006%
95	14.116	3984	3989	3992	rBV3	1150	1294	0.06%	0.007%
96	15.084	4288	4290	4293	rVB3	1240	562	0.03%	0.003%
97	15.267	4345	4347	4348	rBV	955	469	0.02%	0.003%
98	15.293	4351	4355	4359	rVV6	1498	1564	0.07%	0.009%
99	15.399	4386	4388	4393	rVB4	1313	605	0.03%	0.003%
100	15.547	4431	4434	4439	rBV5	1616	1354	0.06%	0.008%




Sum of corrected areas: 17334572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055876.D
Acq On : 25 Oct 2023 13:56
Operator : MD/SY
Sample : VIBLK036
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

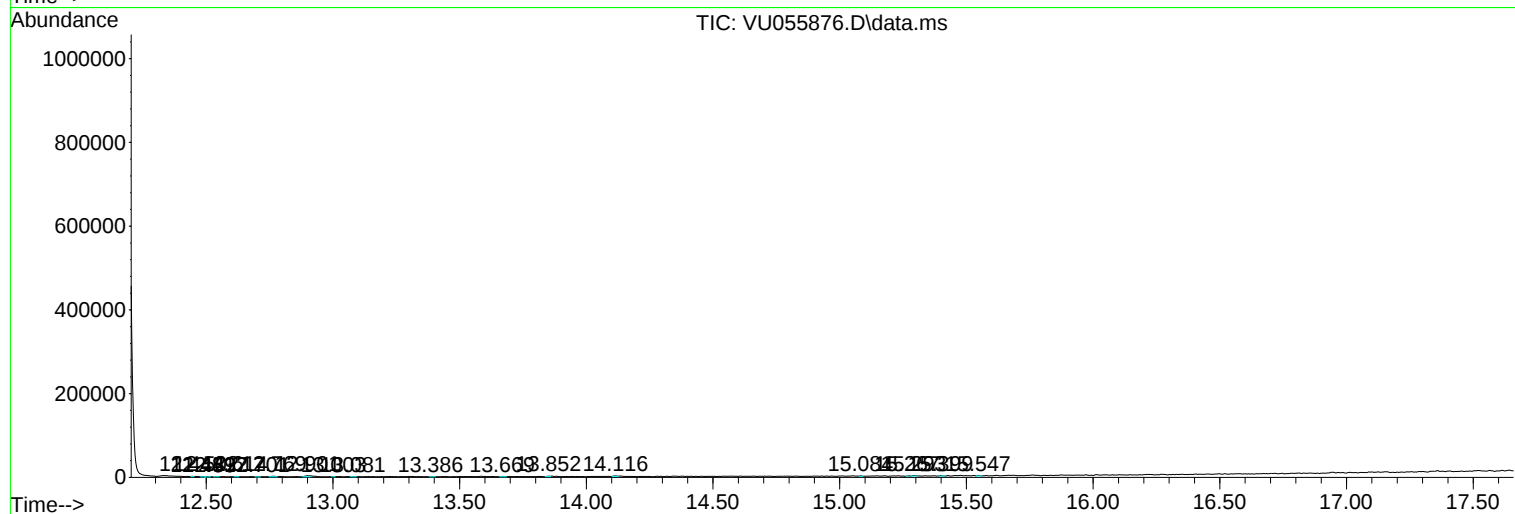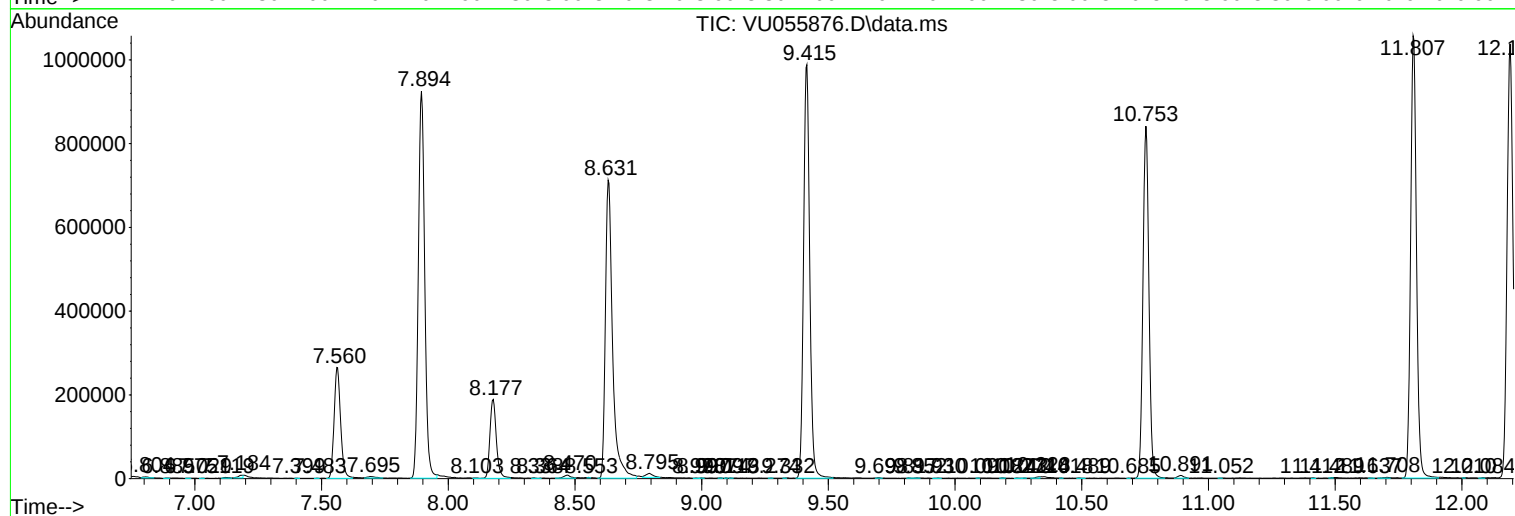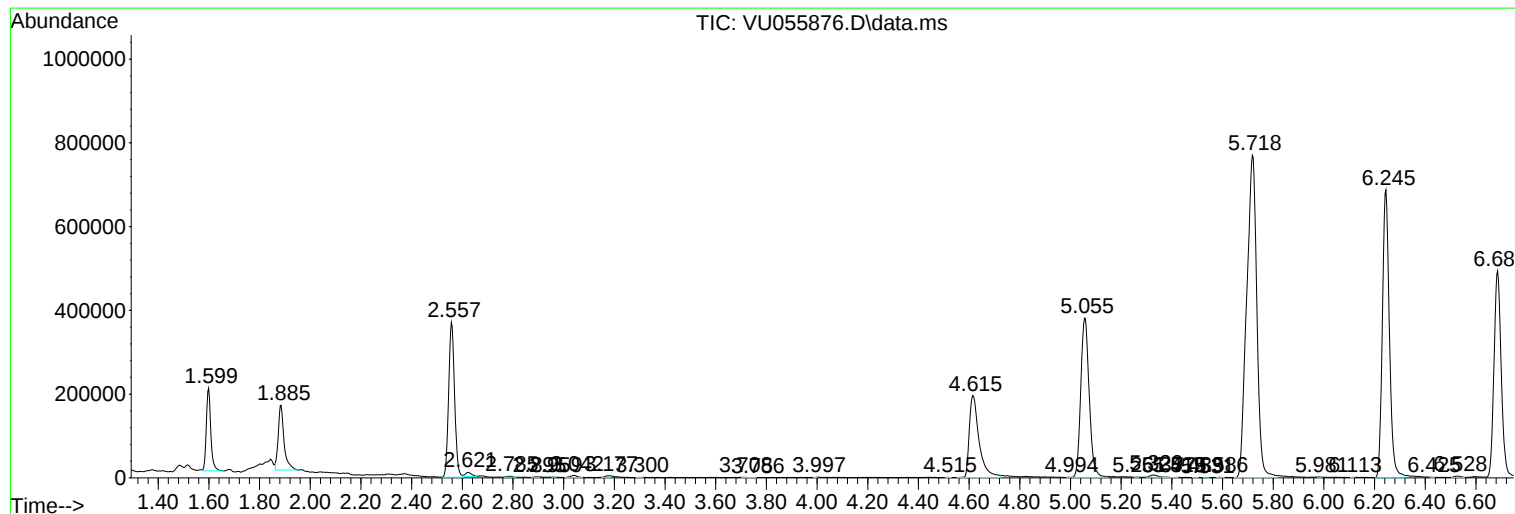

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055876.D
Acq On : 25 Oct 2023 13:56
Operator : MD/SY
Sample : VIBLK036
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055876.D
Acq On : 25 Oct 2023 13:56
Operator : MD/SY
Sample : VIBLK036
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc