

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055879.D
 Acq On : 25 Oct 2023 15:09
 Operator : MD/SY
 Sample : 04946-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	110	rVB	205156	233732	0.32%	0.254%
2	1.895	180	188	207	rVB	165500	250746	0.34%	0.272%
3	2.303	300	315	329	rBV2	27695	66639	0.09%	0.072%
4	2.509	377	379	382	rBV2	574	364	0.00%	0.000%
5	2.560	383	395	410	rBV	381273	624195	0.85%	0.678%
6	2.727	444	447	448	rBV3	602	349	0.00%	0.000%
7	2.782	452	464	474	rVV3	4475	9661	0.01%	0.010%
8	2.895	494	499	501	rVV3	650	540	0.00%	0.001%
9	3.039	537	544	559	rVB8	4579	8284	0.01%	0.009%
10	3.181	571	588	604	rBV	13013	32681	0.04%	0.035%
11	3.354	628	642	652	rVB5	4756	8577	0.01%	0.009%
12	3.393	652	654	660	rVB2	550	397	0.00%	0.000%
13	3.563	703	707	711	rBV2	526	378	0.00%	0.000%
14	3.653	729	735	738	rBV	466	487	0.00%	0.001%
15	3.740	757	762	767	rVB2	353	404	0.00%	0.000%
16	4.059	858	861	867	rVB	532	463	0.00%	0.001%
17	4.097	867	873	876	rBV2	516	411	0.00%	0.000%
18	4.142	883	887	890	rBV2	361	347	0.00%	0.000%
19	4.615	1022	1034	1038	rBV	206276	364752	0.50%	0.396%
20	5.058	1155	1172	1196	rBV	402244	926759	1.27%	1.006%
21	5.187	1210	1212	1216	rVB	1173	654	0.00%	0.001%
22	5.216	1217	1221	1226	rVV7	975	926	0.00%	0.001%
23	5.271	1234	1238	1240	rBV3	702	517	0.00%	0.001%
24	5.329	1247	1256	1270	rVB4	5637	11898	0.02%	0.013%
25	5.441	1286	1291	1296	rBV3	592	645	0.00%	0.001%
26	5.521	1302	1316	1330	rBV3	16875	37416	0.05%	0.041%
27	5.721	1351	1378	1403	rBV2	782406	2180296	2.98%	2.367%
28	5.962	1451	1453	1455	rBV3	655	417	0.00%	0.000%
29	6.036	1473	1476	1483	rVB3	949	890	0.00%	0.001%
30	6.097	1491	1495	1498	rBV3	379	350	0.00%	0.000%
31	6.181	1517	1521	1524	rVB3	433	375	0.00%	0.000%
32	6.245	1524	1541	1575	rBV	694025	1347512	1.84%	1.463%
33	6.431	1596	1599	1600	rBV2	706	368	0.00%	0.000%
34	6.470	1608	1611	1617	rBV3	400	503	0.00%	0.001%
35	6.538	1617	1632	1663	rBV	558731	1072852	1.47%	1.165%
36	6.685	1665	1678	1699	rBV	507887	994028	1.36%	1.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055879.D
 Acq On : 25 Oct 2023 15:09
 Operator : MD/SY
 Sample : 04946-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.898	1741	1744	1746	rBV2	510	346	0.00%	0.000%
38	7.142	1815	1820	1822	rBV4	564	474	0.00%	0.001%
39	7.193	1822	1836	1849	rBV7	7462	18615	0.03%	0.020%
40	7.322	1874	1876	1878	rBV7	609	355	0.00%	0.000%
41	7.396	1895	1899	1902	rBV2	455	389	0.00%	0.000%
42	7.496	1927	1930	1933	rBV	502	356	0.00%	0.000%
43	7.560	1938	1950	1972	rBV	272096	491802	0.67%	0.534%
44	7.698	1984	1993	2009	rVB6	4031	9351	0.01%	0.010%
45	7.753	2009	2010	2015	rVB2	504	373	0.00%	0.000%
46	7.788	2017	2021	2024	rBV3	668	591	0.00%	0.001%
47	7.894	2041	2054	2078	rBV	970587	1686247	2.31%	1.830%
48	8.081	2106	2112	2118	rVB5	1015	1167	0.00%	0.001%
49	8.177	2129	2142	2165	rBV	192005	337111	0.46%	0.366%
50	8.470	2222	2233	2241	rBV	5436	9685	0.01%	0.011%
51	8.554	2241	2259	2275	rBV	42259993	73045152	100.00%	79.291%
52	8.631	2276	2283	2322	rVB	748064	1536709	2.10%	1.668%
53	9.023	2402	2405	2410	rVB4	964	678	0.00%	0.001%
54	9.113	2430	2433	2435	rVV2	980	421	0.00%	0.000%
55	9.200	2457	2460	2463	rVB4	573	360	0.00%	0.000%
56	9.222	2463	2467	2468	rBV3	795	506	0.00%	0.001%
57	9.264	2477	2480	2483	rBV3	652	378	0.00%	0.000%
58	9.319	2494	2497	2498	rBV	918	371	0.00%	0.000%
59	9.412	2513	2526	2553	rBV	1033385	1741105	2.38%	1.890%
60	9.528	2560	2562	2569	rVB7	2758	2351	0.00%	0.003%
61	9.695	2609	2614	2616	rVV4	923	858	0.00%	0.001%
62	9.833	2654	2657	2662	rVB3	410	367	0.00%	0.000%
63	9.923	2680	2685	2690	rBV4	605	740	0.00%	0.001%
64	10.097	2735	2739	2741	rBV2	409	368	0.00%	0.000%
65	10.123	2743	2747	2749	rVV4	1040	832	0.00%	0.001%
66	10.135	2749	2751	2755	rVV2	763	529	0.00%	0.001%
67	10.193	2766	2769	2772	rBV3	692	503	0.00%	0.001%
68	10.267	2787	2792	2794	rBV3	371	387	0.00%	0.000%
69	10.335	2809	2813	2816	rVB	566	383	0.00%	0.000%
70	10.354	2816	2819	2824	rBV3	652	791	0.00%	0.001%
71	10.422	2835	2840	2843	rBV2	427	411	0.00%	0.000%
72	10.470	2850	2855	2856	rBV	629	515	0.00%	0.001%
73	10.499	2861	2864	2866	rVV3	514	390	0.00%	0.000%
74	10.525	2869	2872	2877	rVB2	536	398	0.00%	0.000%
75	10.582	2886	2890	2895	rBV4	652	525	0.00%	0.001%
76	10.676	2917	2919	2922	rVB	734	377	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055879.D
 Acq On : 25 Oct 2023 15:09
 Operator : MD/SY
 Sample : 04946-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	10.695	2922	2925	2927	rBV3	678	374	0.00%	0.000%
78	10.753	2930	2943	2966	rBV	850411	1388792	1.90%	1.508%
79	10.888	2978	2985	2994	rBV3	5116	8152	0.01%	0.009%
80	11.071	3039	3042	3045	rBV3	516	405	0.00%	0.000%
81	11.090	3045	3048	3051	rVV2	570	363	0.00%	0.000%
82	11.267	3096	3103	3108	rBV2	648	941	0.00%	0.001%
83	11.293	3108	3111	3113	rVV	549	377	0.00%	0.000%
84	11.319	3117	3119	3124	rVV2	525	385	0.00%	0.000%
85	11.409	3142	3147	3152	rBV3	1155	1076	0.00%	0.001%
86	11.476	3166	3168	3171	rVB3	1078	576	0.00%	0.001%
87	11.753	3252	3254	3258	rBV5	607	359	0.00%	0.000%
88	11.807	3258	3271	3299	rBV	1136634	1830470	2.51%	1.987%
89	12.190	3377	3390	3409	rBV	1085630	1809650	2.48%	1.964%
90	12.335	3430	3435	3439	rBV7	1830	2235	0.00%	0.002%
91	12.428	3462	3464	3466	rVB3	832	398	0.00%	0.000%
92	13.094	3667	3671	3675	rBV3	613	557	0.00%	0.001%
93	13.200	3700	3704	3705	rBV	491	351	0.00%	0.000%
94	13.296	3732	3734	3738	rBV2	594	399	0.00%	0.000%
95	13.402	3764	3767	3770	rBV3	718	467	0.00%	0.001%
96	14.338	4056	4058	4066	rVB5	859	759	0.00%	0.001%
97	14.846	4212	4216	4219	rVB3	893	695	0.00%	0.001%
98	14.958	4249	4251	4253	rBV3	1041	561	0.00%	0.001%
99	15.129	4301	4304	4308	rBV3	1329	942	0.00%	0.001%
100	15.392	4384	4386	4389	rBV3	1415	865	0.00%	0.001%




Sum of corrected areas: 92123229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055879.D
Acq On : 25 Oct 2023 15:09
Operator : MD/SY
Sample : 04946-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

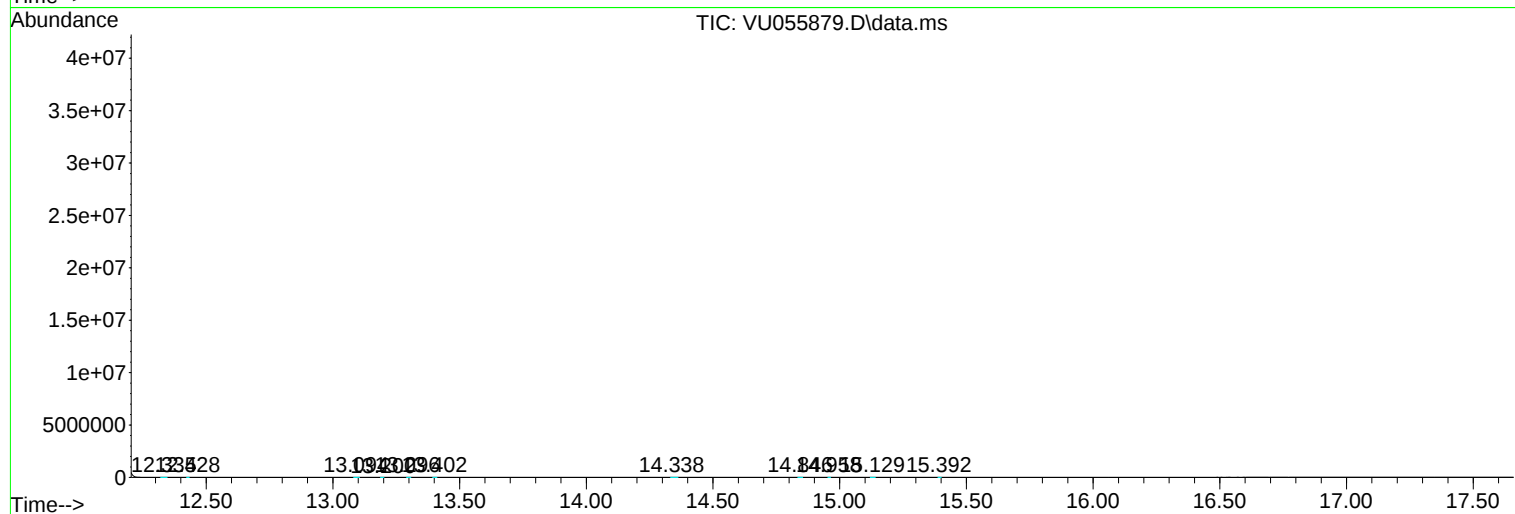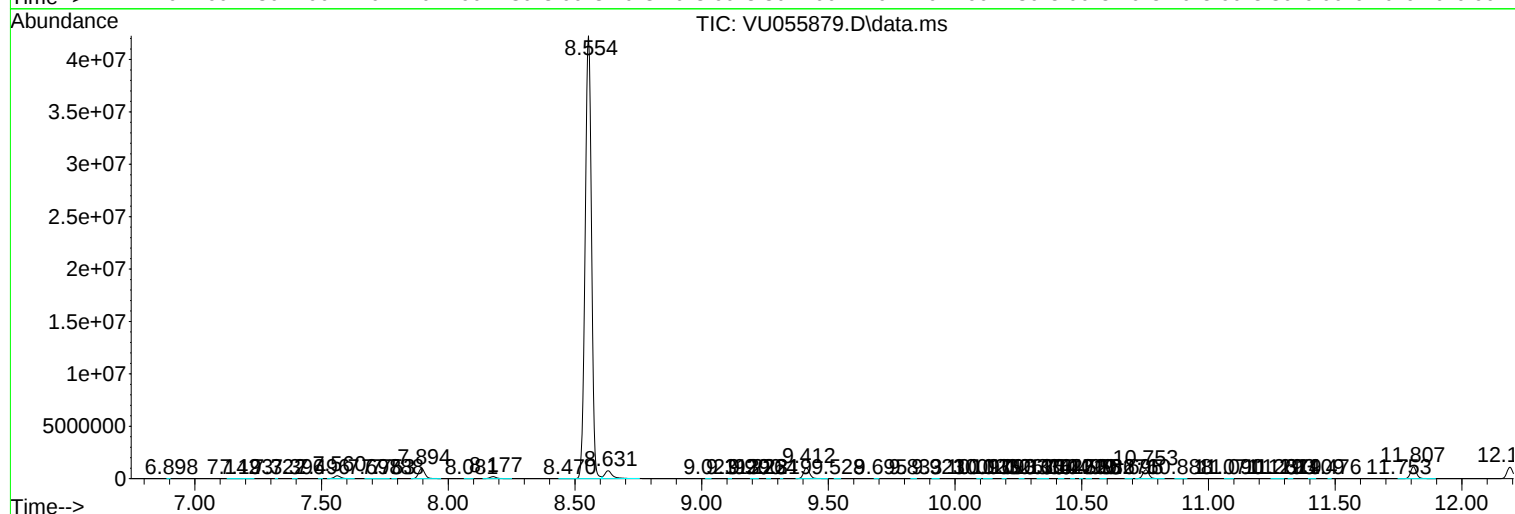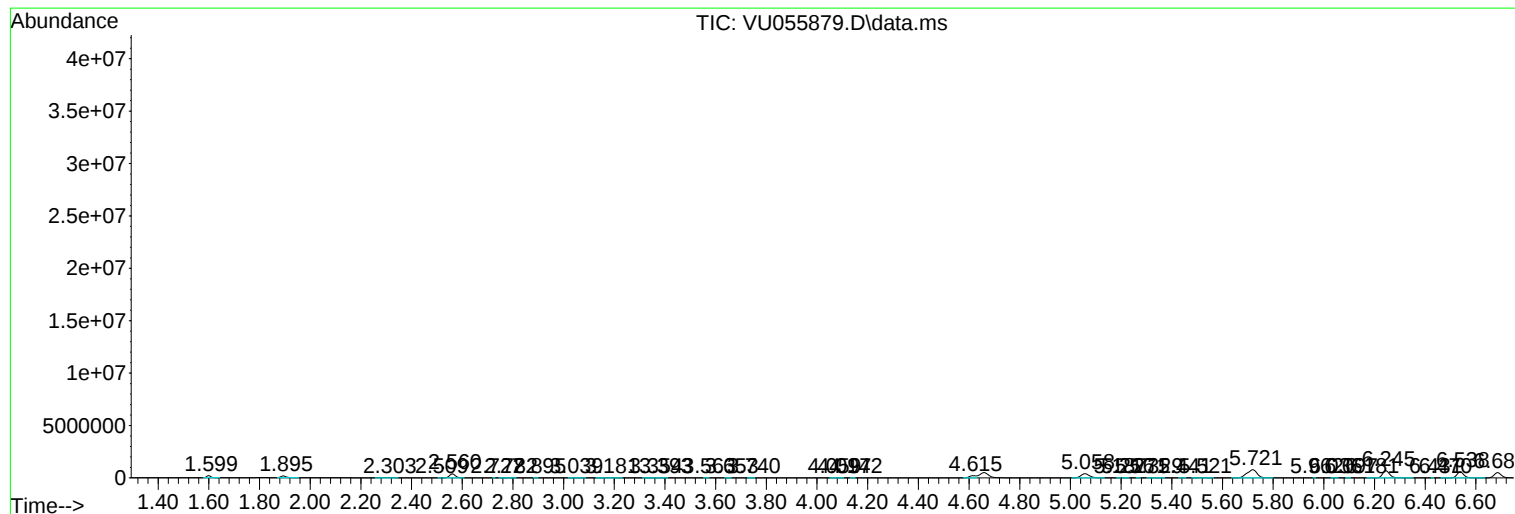

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055879.D
Acq On : 25 Oct 2023 15:09
Operator : MD/SY
Sample : 04946-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055879.D
Acq On : 25 Oct 2023 15:09
Operator : MD/SY
Sample : 04946-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------