

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055885.D
 Acq On : 25 Oct 2023 17:33
 Operator : MD/SY
 Sample : 04952-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	52	59	60	rBV2	30592	31971	1.26%	0.167%
2	1.599	89	96	117	rVB	322579	382160	15.11%	2.000%
3	1.891	180	187	211	rVB	221732	332953	13.16%	1.742%
4	2.560	382	395	411	rBV	523884	857031	33.88%	4.485%
5	2.788	460	466	476	rVB	4480	7452	0.29%	0.039%
6	2.865	486	490	491	rBV2	824	445	0.02%	0.002%
7	2.888	495	497	506	rVB7	488	530	0.02%	0.003%
8	2.962	518	520	530	rVB5	652	840	0.03%	0.004%
9	3.036	535	543	554	rBV6	4304	8288	0.33%	0.043%
10	3.177	577	587	596	rBV4	4977	9884	0.39%	0.052%
11	3.303	622	626	628	rBV2	592	480	0.02%	0.003%
12	3.666	737	739	743	rVB2	606	383	0.02%	0.002%
13	4.026	846	851	854	rBV3	375	374	0.01%	0.002%
14	4.258	919	923	928	rBV	410	345	0.01%	0.002%
15	4.444	977	981	987	rBV2	493	646	0.03%	0.003%
16	4.512	996	1002	1003	rBV2	438	381	0.02%	0.002%
17	4.537	1007	1010	1016	rBV2	708	455	0.02%	0.002%
18	4.615	1023	1034	1067	rBV	184802	469303	18.55%	2.456%
19	5.058	1155	1172	1201	rBV	432191	977822	38.66%	5.117%
20	5.332	1244	1257	1270	rBV2	7155	16151	0.64%	0.085%
21	5.483	1300	1304	1307	rBV2	493	371	0.01%	0.002%
22	5.605	1338	1342	1343	rBV	581	339	0.01%	0.002%
23	5.721	1356	1378	1412	rBV2	925100	2529506	100.00%	13.237%
24	5.959	1449	1452	1453	rBV2	1145	641	0.03%	0.003%
25	6.010	1465	1468	1471	rVB2	693	427	0.02%	0.002%
26	6.036	1471	1476	1479	rBV6	1349	1403	0.06%	0.007%
27	6.065	1483	1485	1491	rVB4	493	384	0.02%	0.002%
28	6.106	1495	1498	1501	rBV	636	540	0.02%	0.003%
29	6.245	1527	1541	1578	rBV	675600	1320886	52.22%	6.912%
30	6.425	1594	1597	1600	rVB3	618	385	0.02%	0.002%
31	6.524	1618	1628	1638	rBV9	2295	4428	0.18%	0.023%
32	6.685	1663	1678	1708	rBV	560104	1108096	43.81%	5.799%
33	7.058	1789	1794	1796	rBV3	476	412	0.02%	0.002%
34	7.193	1818	1836	1842	rBV5	5906	13450	0.53%	0.070%
35	7.389	1892	1897	1899	rBV4	521	435	0.02%	0.002%
36	7.431	1906	1910	1916	rBV2	373	373	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055885.D
 Acq On : 25 Oct 2023 17:33
 Operator : MD/SY
 Sample : 04952-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.563	1937	1951	1976	rBV	305193	555794	21.97%	2.908%
38	7.701	1988	1994	2015	rVB8	3437	8431	0.33%	0.044%
39	7.788	2015	2021	2022	rBV3	670	500	0.02%	0.003%
40	7.894	2040	2054	2080	rBV	1140645	2004114	79.23%	10.487%
41	8.177	2130	2142	2165	rBV	213243	369881	14.62%	1.936%
42	8.309	2181	2183	2187	rVB4	718	418	0.02%	0.002%
43	8.373	2201	2203	2209	rVB4	616	510	0.02%	0.003%
44	8.418	2215	2217	2221	rVB2	986	578	0.02%	0.003%
45	8.470	2221	2233	2241	rBV4	3565	6001	0.24%	0.031%
46	8.508	2241	2245	2246	rBV3	895	587	0.02%	0.003%
47	8.550	2250	2258	2271	rVB4	12454	22786	0.90%	0.119%
48	8.630	2271	2283	2317	rBV	677871	1297736	51.30%	6.791%
49	8.868	2354	2357	2360	rVB3	727	451	0.02%	0.002%
50	9.110	2428	2432	2435	rBV2	852	528	0.02%	0.003%
51	9.238	2470	2472	2478	rVB3	539	458	0.02%	0.002%
52	9.280	2481	2485	2490	rBV3	570	540	0.02%	0.003%
53	9.309	2490	2494	2497	rBV3	717	609	0.02%	0.003%
54	9.335	2497	2502	2506	rVB3	1027	1069	0.04%	0.006%
55	9.415	2511	2527	2552	rBV	982612	1660496	65.65%	8.689%
56	9.624	2589	2592	2597	rVB2	648	542	0.02%	0.003%
57	9.695	2610	2614	2618	rBV2	668	650	0.03%	0.003%
58	9.833	2653	2657	2661	rVB3	779	644	0.03%	0.003%
59	9.856	2661	2664	2669	rVB3	662	485	0.02%	0.003%
60	9.884	2670	2673	2679	rVB	369	338	0.01%	0.002%
61	9.917	2679	2683	2686	rBV2	659	590	0.02%	0.003%
62	9.978	2700	2702	2706	rVB2	726	534	0.02%	0.003%
63	10.032	2715	2719	2722	rVV3	602	464	0.02%	0.002%
64	10.116	2738	2745	2747	rBV3	677	776	0.03%	0.004%
65	10.167	2755	2761	2762	rBV2	520	431	0.02%	0.002%
66	10.187	2762	2767	2770	rBV4	848	865	0.03%	0.005%
67	10.473	2848	2856	2858	rBV	753	778	0.03%	0.004%
68	10.753	2930	2943	2965	rBV	845851	1377431	54.45%	7.208%
69	10.884	2979	2984	2985	rBV4	2195	1728	0.07%	0.009%
70	11.466	3163	3165	3167	rBV	594	364	0.01%	0.002%
71	11.521	3178	3182	3188	rVB3	676	595	0.02%	0.003%
72	11.560	3191	3194	3198	rBV2	510	429	0.02%	0.002%
73	11.749	3250	3253	3256	rVB2	736	388	0.02%	0.002%
74	11.807	3259	3271	3303	rBV	1080905	1724626	68.18%	9.025%
75	12.019	3335	3337	3340	rBV3	700	380	0.02%	0.002%
76	12.093	3356	3360	3369	rVB10	2449	3114	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
 Data File : VU055885.D
 Acq On : 25 Oct 2023 17:33
 Operator : MD/SY
 Sample : 04952-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOAS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	12.190	3376	3390	3415	rBV	1168511	1924601	76.09%	10.071%
78	12.466	3474	3476	3481	rBV4	849	717	0.03%	0.004%
79	12.614	3519	3522	3526	rVB2	1119	875	0.03%	0.005%
80	12.724	3554	3556	3560	rVB2	804	371	0.01%	0.002%
81	12.759	3560	3567	3570	rBV5	937	1129	0.04%	0.006%
82	12.920	3613	3617	3623	rVB5	607	700	0.03%	0.004%
83	12.978	3633	3635	3636	rBV2	932	421	0.02%	0.002%
84	13.109	3671	3676	3679	rBV3	728	758	0.03%	0.004%
85	13.154	3687	3690	3694	rVB3	619	396	0.02%	0.002%
86	13.228	3710	3713	3715	rBV2	438	356	0.01%	0.002%
87	13.302	3728	3736	3742	rBV5	1334	2067	0.08%	0.011%
88	13.457	3777	3784	3791	rBV7	3095	4475	0.18%	0.023%
89	13.769	3879	3881	3883	rBV	766	443	0.02%	0.002%
90	13.933	3929	3932	3938	rVV5	993	914	0.04%	0.005%
91	13.958	3938	3940	3944	rVB2	1055	568	0.02%	0.003%
92	14.100	3981	3984	3986	rBV3	1034	778	0.03%	0.004%
93	14.286	4040	4042	4045	rBV4	946	614	0.02%	0.003%
94	14.527	4115	4117	4119	rBV2	662	382	0.02%	0.002%
95	14.714	4173	4175	4178	rBV3	745	549	0.02%	0.003%
96	14.756	4186	4188	4191	rBV2	743	432	0.02%	0.002%
97	14.881	4220	4227	4232	rBV5	1655	2028	0.08%	0.011%
98	15.019	4268	4270	4271	rBV2	893	426	0.02%	0.002%
99	15.100	4293	4295	4298	rBV2	1195	735	0.03%	0.004%
100	15.412	4384	4392	4405	rBV3	22657	37362	1.48%	0.196%




Sum of corrected areas: 19109706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055885.D
Acq On : 25 Oct 2023 17:33
Operator : MD/SY
Sample : 04952-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

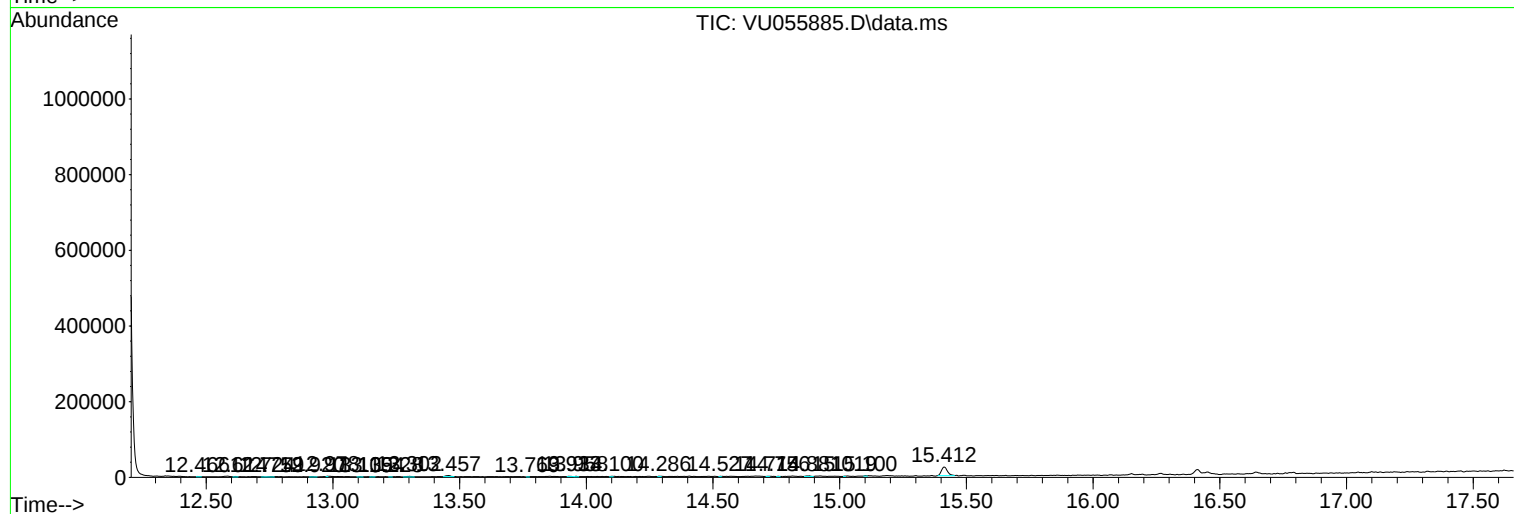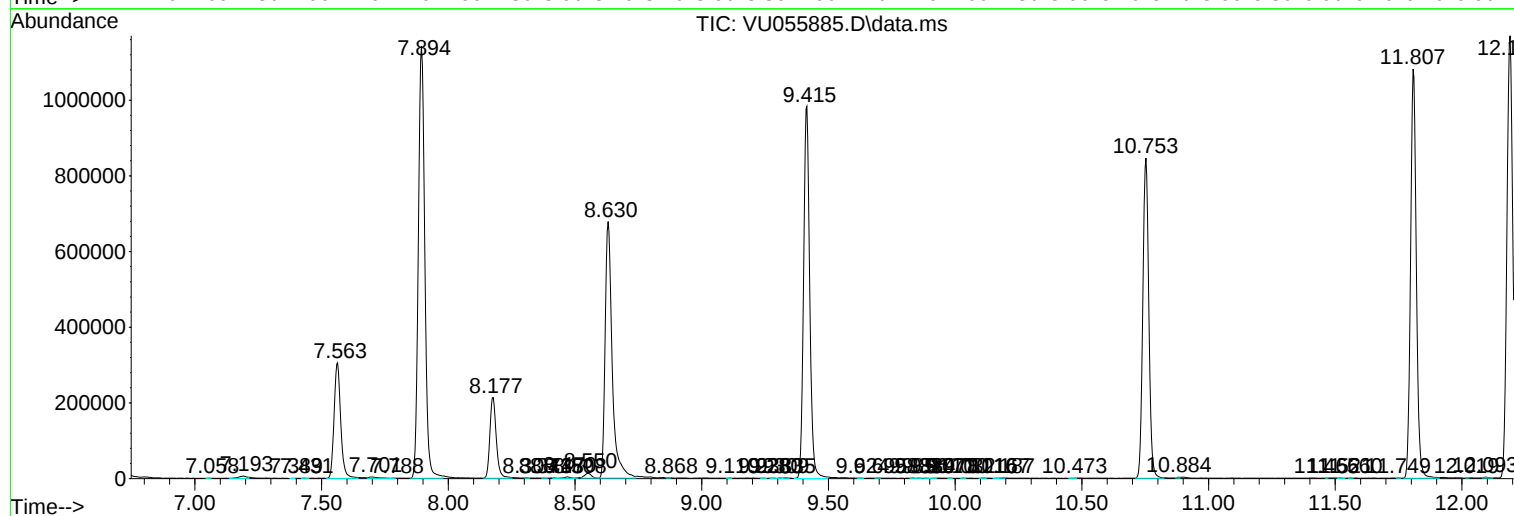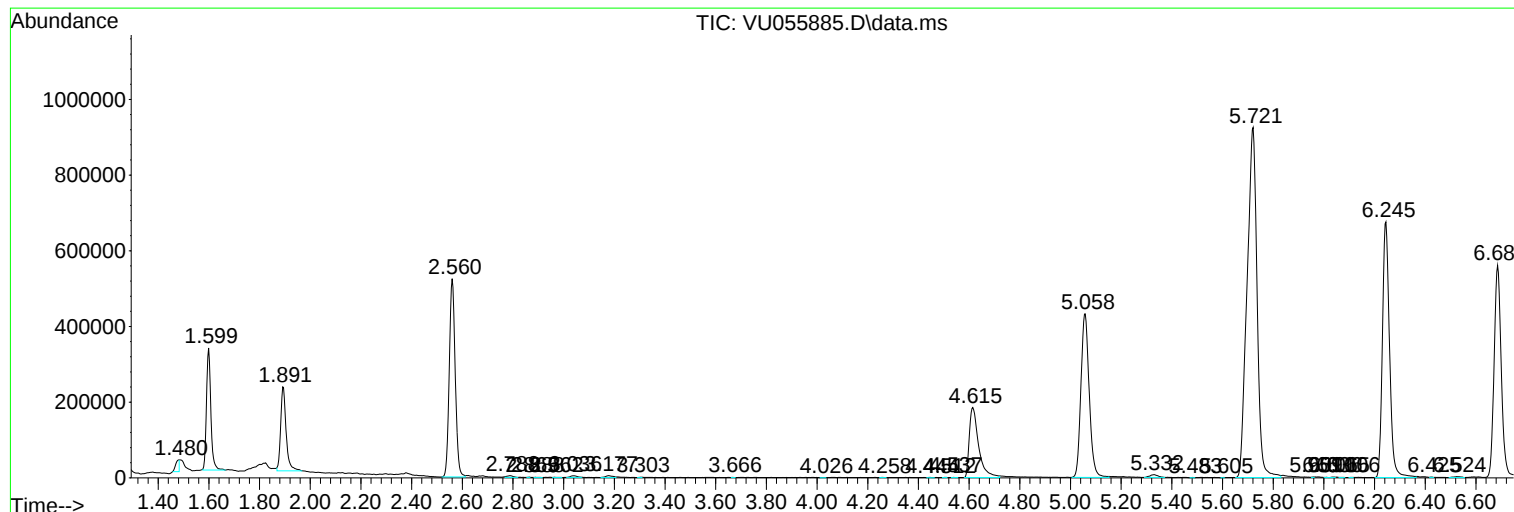

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055885.D
Acq On : 25 Oct 2023 17:33
Operator : MD/SY
Sample : 04952-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055885.D
Acq On : 25 Oct 2023 17:33
Operator : MD/SY
Sample : 04952-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------