
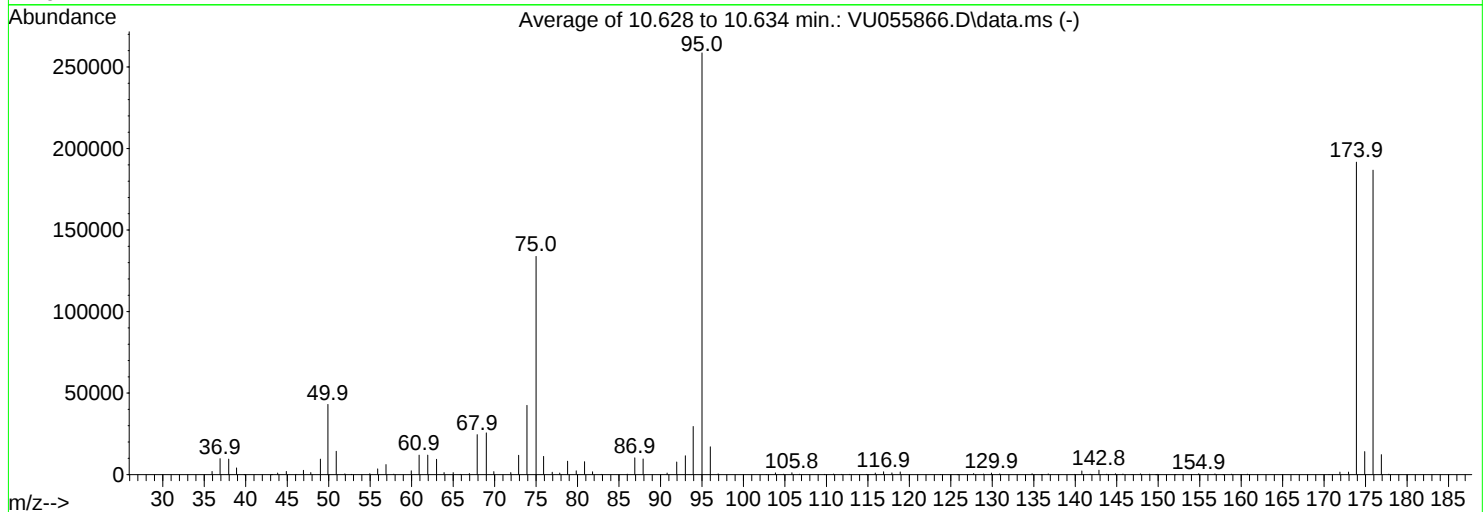


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102523\
Data File : VU055866.D
Acq On : 25 Oct 2023 08:30
Operator : MD/SY
Sample : BFB027
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB027

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Fri Oct 27 02:48:43 2023

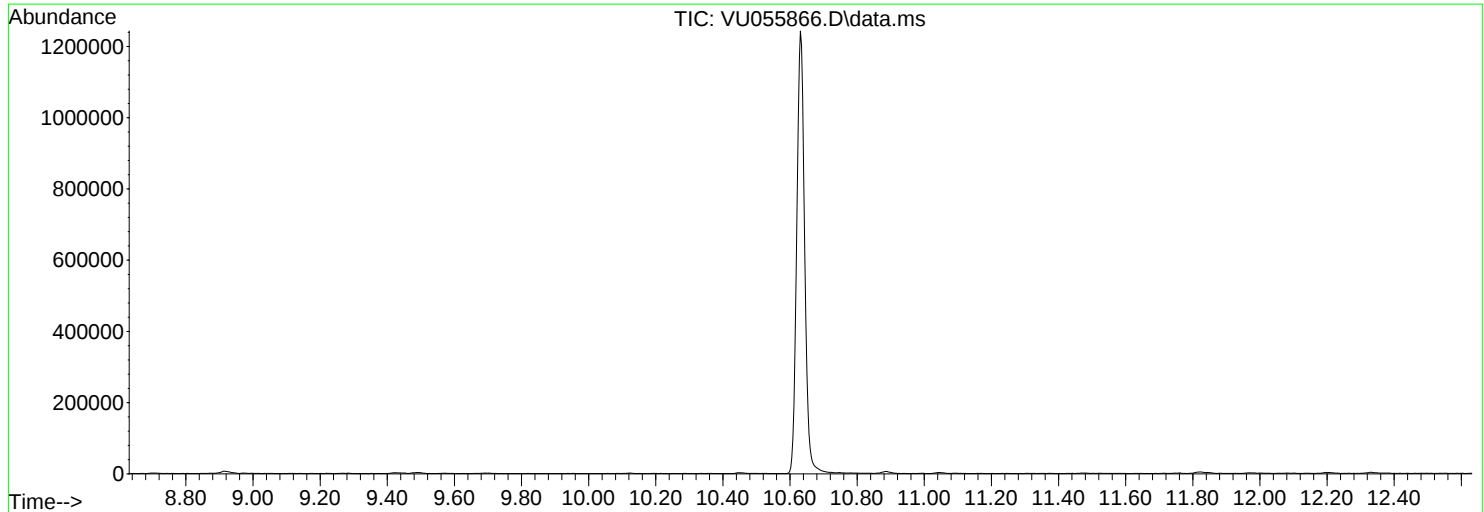

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	43048	PASS
75	95	30	80	51.8	133888	PASS
95	95	100	100	100.0	258688	PASS
96	95	5	9	6.6	17053	PASS
173	174	0.00	2	0.8	1565	PASS
174	95	50	120	74.1	191616	PASS
175	174	5	9	7.4	14141	PASS
176	174	95	101	97.5	186795	PASS
177	176	5	9	6.5	12226	PASS

m/z	Abundance
39.80	362.0
43.90	632.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	1858.0
36.90	9759.0
37.90	9450.0
38.90	4230.0
39.90	375.0
43.10	102.0
43.90	1651.0
44.90	1978.0
46.00	271.0
46.90	2464.0
47.90	1039.0
49.00	9440.0
49.90	42944.0
50.90	13894.0
51.90	573.0
52.80	196.0
54.90	599.0
55.90	3536.0
56.90	6084.0
57.90	247.0
59.90	2229.0
60.90	12092.0
62.00	11764.0
63.00	9183.0
63.90	1242.0
65.00	1345.0
65.80	137.0
67.00	726.0
67.90	24104.0
69.00	25192.0
69.90	1772.0
72.00	1233.0
72.90	11970.0
73.90	40928.0
75.00	132160.0
75.90	10766.0
77.00	1607.0
77.80	885.0
78.80	8124.0
79.90	2354.0
80.90	7957.0
81.80	1591.0
82.80	174.0
86.00	262.0
86.90	10135.0
87.90	9368.0
90.80	988.0
92.00	7741.0
93.00	11433.0
93.90	28792.0
95.00	250944.0
96.00	16576.0
96.90	448.0
102.80	143.0
103.80	988.0
104.90	299.0
105.80	1145.0
106.70	285.0
109.80	180.0
110.80	281.0
111.80	223.0
112.80	202.0
114.80	241.0
115.90	956.0
116.90	1801.0
117.90	1092.0
118.90	1776.0
123.70	148.0
125.80	122.0
127.80	674.0
128.90	361.0
129.90	860.0
130.90	430.0
134.80	590.0
136.70	442.0
139.90	208.0
140.80	2282.0
141.80	295.0
142.90	2609.0
143.80	271.0
144.80	544.0
145.80	427.0
147.90	499.0
148.90	295.0
149.70	161.0
152.00	150.0
152.90	113.0
154.90	618.0
156.90	476.0
158.80	340.0
160.80	232.0
170.60	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

171.90	1664.0
173.00	1656.0
173.90	182208.0
174.90	13870.0
175.90	177280.0
176.90	11592.0
177.80	360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	2040.0
36.90	10189.0
38.00	9926.0
38.90	4227.0
39.80	393.0
43.90	1682.0
44.90	1994.0
46.10	245.0
46.90	2712.0
47.80	1299.0
49.00	9881.0
49.90	44176.0
50.90	14802.0
52.00	466.0
52.70	249.0
55.00	597.0
55.90	3648.0
56.90	6363.0
57.90	308.0
60.00	2445.0
60.90	12346.0
61.90	12357.0
63.00	9854.0
63.90	1386.0
65.00	1328.0
65.90	173.0
66.90	670.0
67.90	25360.0
69.00	26464.0
69.90	1902.0
72.00	1313.0
72.90	12314.0
73.90	43936.0
75.00	138112.0
75.90	11565.0
77.00	1546.0
77.80	1024.0
78.80	8589.0
79.80	2447.0
80.90	8113.0
81.80	1861.0
82.80	208.0
86.00	312.0
86.90	10698.0
87.90	10038.0
90.80	1007.0
92.00	7939.0
93.00	12171.0
94.00	30496.0
95.00	266944.0
96.00	17448.0
97.00	373.0
102.70	173.0
103.90	1101.0
104.90	267.0
105.80	1168.0
106.80	282.0
109.80	222.0
110.90	391.0
111.80	256.0
112.80	175.0
114.90	238.0
115.90	1064.0
116.90	1806.0
117.90	1120.0
118.90	1801.0
123.70	150.0
127.70	678.0
128.90	362.0
129.90	990.0
130.90	517.0
134.80	633.0
135.90	114.0
136.80	487.0
139.90	195.0
140.80	2382.0
141.80	299.0
142.90	2812.0
143.80	340.0
144.90	580.0
145.70	434.0
146.90	113.0
147.80	479.0
148.90	283.0
149.90	228.0
152.90	143.0
154.00	107.0
154.90	696.0
155.80	129.0
156.80	518.0
158.90	338.0
160.70	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

171.90	1628.0
172.90	1549.0
173.90	197376.0
174.90	14550.0
175.90	192960.0
176.90	12674.0
177.80	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	2034.0
36.90	9647.0
38.00	9236.0
38.90	3932.0
39.80	454.0
43.80	1578.0
44.90	1887.0
46.10	192.0
47.00	2714.0
47.80	1531.0
49.00	9358.0
49.90	42024.0
50.90	14327.0
52.00	331.0
52.70	269.0
55.00	552.0
55.90	3390.0
56.90	6134.0
57.80	308.0
60.00	2429.0
60.90	11626.0
61.90	11866.0
63.00	9374.0
63.90	1234.0
65.00	1250.0
65.80	171.0
66.90	631.0
67.90	24024.0
69.00	25144.0
69.90	2011.0
71.90	1387.0
72.90	11240.0
73.90	42680.0
75.00	131392.0
75.90	11313.0
76.90	1225.0
77.90	1048.0
78.80	8055.0
79.80	2444.0
80.80	7773.0
81.80	1959.0
82.90	235.0
86.00	319.0
86.90	10154.0
87.90	9531.0
90.80	936.0
91.90	7469.0
93.00	11250.0
93.90	29272.0
95.00	258176.0
96.00	17136.0
96.90	313.0
97.10	318.0
102.70	150.0
103.90	1121.0
104.80	241.0
105.90	1117.0
106.80	253.0
109.80	206.0
110.90	399.0
111.90	222.0
112.80	135.0
114.90	262.0
115.90	1057.0
116.90	1662.0
117.90	967.0
118.90	1553.0
123.80	156.0
127.70	723.0
129.00	384.0
129.90	985.0
130.90	456.0
134.80	544.0
136.80	459.0
140.00	168.0
140.80	2255.0
141.80	290.0
142.80	2837.0
143.80	378.0
144.90	584.0
145.70	375.0
146.80	125.0
147.80	494.0
149.00	232.0
149.90	281.0
152.90	157.0
154.00	120.0
154.90	632.0
155.70	155.0
156.90	434.0
157.80	104.0
158.90	311.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

160.70	297.0
170.60	104.0
171.90	1538.0
173.00	1491.0
173.90	195264.0
174.90	14002.0
175.90	190144.0
176.90	12412.0
177.80	237.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027