

Data File : VU027824.D
Acq On : 26 Oct 2018 11:36
Operator : MD/SY
Sample : J5635-25ME
Misc : 4.91g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A40G1ME

Quant Time: Oct 27 01:44:58 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 01:41:17 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	100688	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	100143	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	57262	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26261	33.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.04%
7) Chloroethane-d5	1.64	69	23633	39.18	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.36%
11) 1,1-Dichloroethene-d2	2.24	63	38053	26.97	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	53.94%#
21) 2-Butanone-d5	4.19	46	54901	82.23	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.23%
24) Chloroform-d	4.65	84	52264	37.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.22%
26) 1,2-Dichloroethane-d4	5.31	65	40025	41.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.08%
32) Benzene-d6	5.33	84	98363	34.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.98%#
36) 1,2-Dichloropropane-d6	6.33	67	36068	35.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	70.84%
41) Toluene-d8	7.57	98	92607	35.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	70.40%#
43) trans-1,3-Dichloropropene-	7.85	79	17361	35.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.22%
47) 2-Hexanone-d5	8.32	63	44677	85.74	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.74%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	55010	41.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.68%
64) 1,2-Dichlorobenzene-d4	11.86	152	43524	37.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	74.22%#

Target Compounds


						Qvalue
13) Acetone	2.34	43	733	1.576	ug/L #	46
15) Methyl Acetate	2.62	43	774	0.791	ug/L #	58
35) Methylcyclohexane	6.33	83	7930	6.148	ug/L #	14
37) 1,2-Dichloropropane	6.33	63	4038	4.587	ug/L #	90
39) cis-1,3-Dichloropropene	7.23	75	1017	0.750	ug/L #	70
44) trans-1,3-Dichloropropene	7.85	75	710	0.554	ug/L	95
56) Isopropylbenzene	10.17	105	1714	0.509	ug/L #	86
59) 1,2,3-Trichloropropane	11.49	75	8815	8.474	ug/L	100
62) 1,3-Dichlorobenzene	11.42	146	2251	1.311	ug/L	93
63) 1,4-Dichlorobenzene	11.51	146	15484	8.844	ug/L	98
66) 1,2-Dibromo-3-chloropropan	12.38	75	1172	3.185	ug/L #	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU027824.D
Acq On : 26 Oct 2018 11:36
Operator : MD/SY
Sample : J5635-25ME
Misc : 4.91g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A40G1ME

Quant Time: Oct 27 01:44:58 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 01:41:17 2018
Response via : Initial Calibration

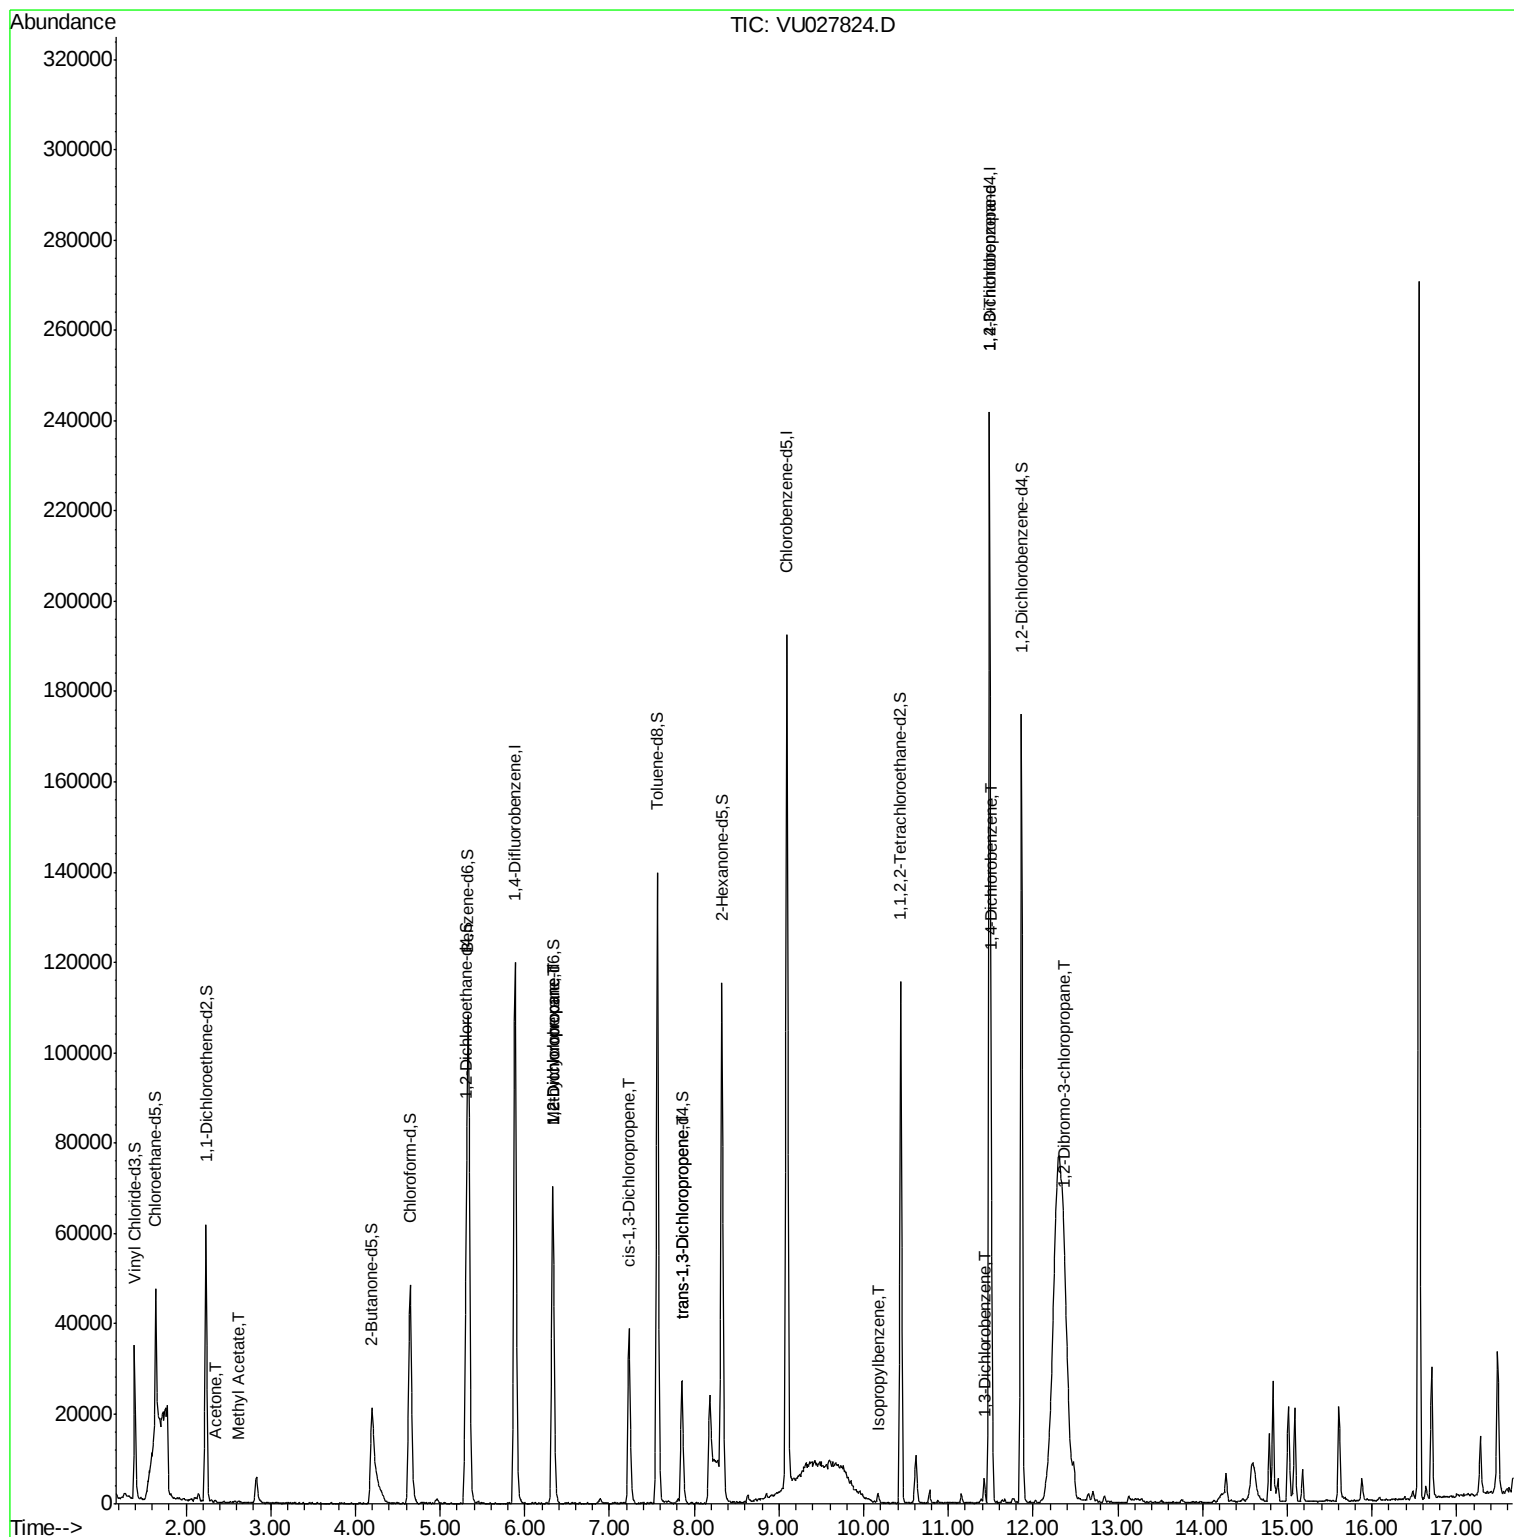

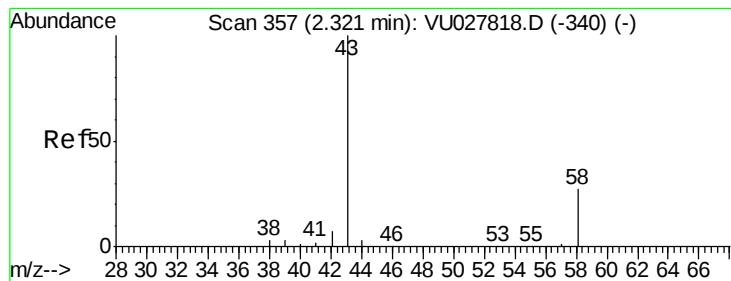

#13

Acetone

Concen: 1.576 ug/L

RT: 2.34 min Scan# 364

Delta R.T. 0.02 min

Lab File: VU027824.D

Acq: 26 Oct 2018 11:36

Instrument :

MSVOA_U

ClientSampleId :





A40G1ME

Tgt Ion: 43 Resp: 733

Ion Ratio Lower Upper

43 100

58 0.0 0.0 57.4

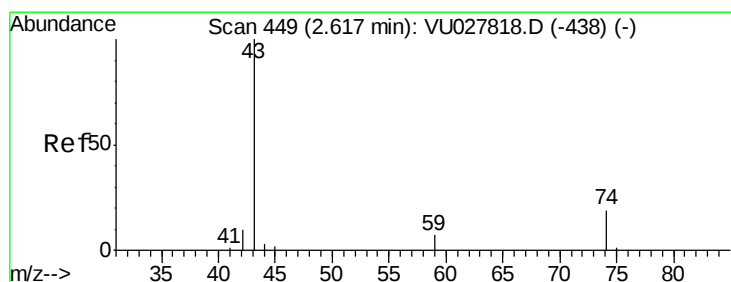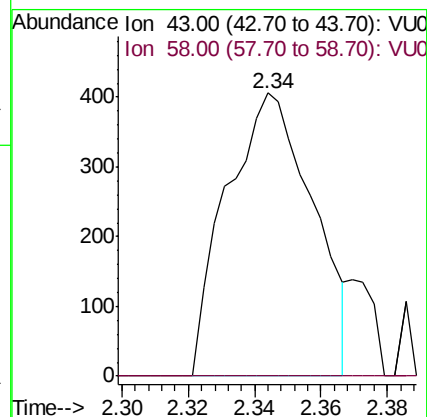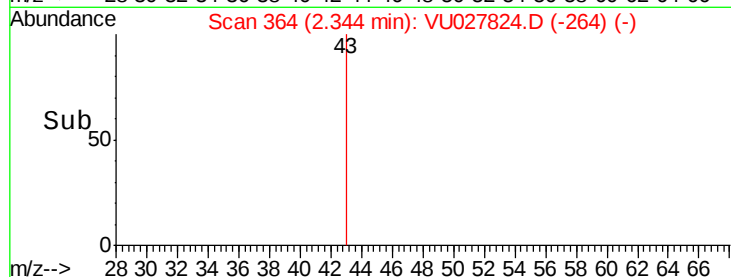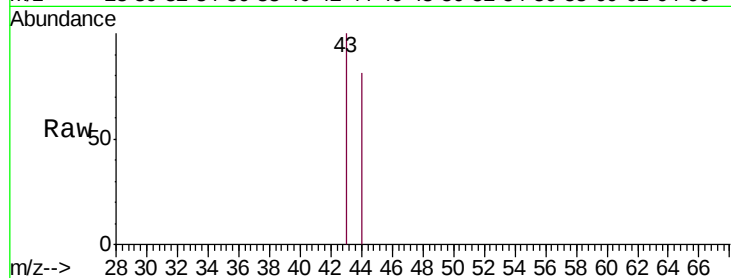

#15

Methyl Acetate

Concen: 0.791 ug/L

RT: 2.62 min Scan# 451

Delta R.T. 0.01 min

Lab File: VU027824.D




Acq: 26 Oct 2018 11:36


Tgt Ion: 43 Resp: 774

Ion Ratio Lower Upper

43 100

74 0.0 15.1 22.7#

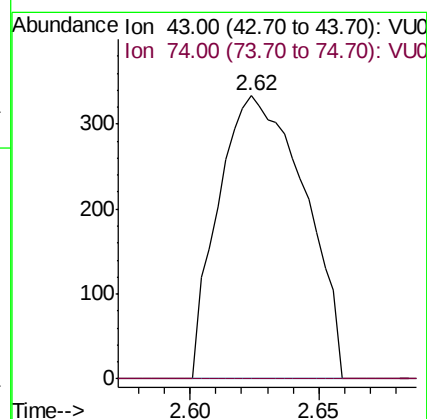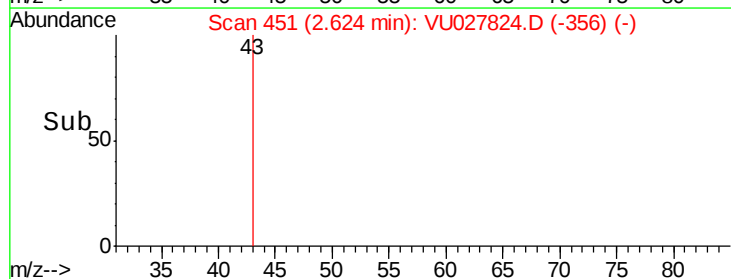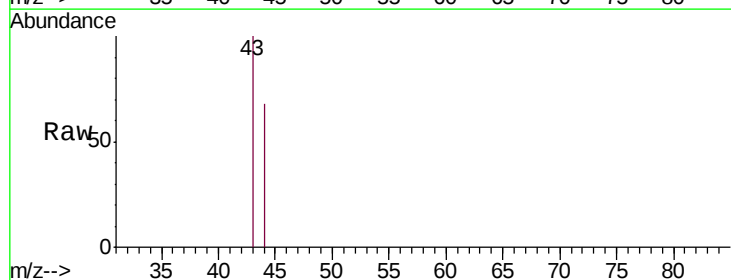


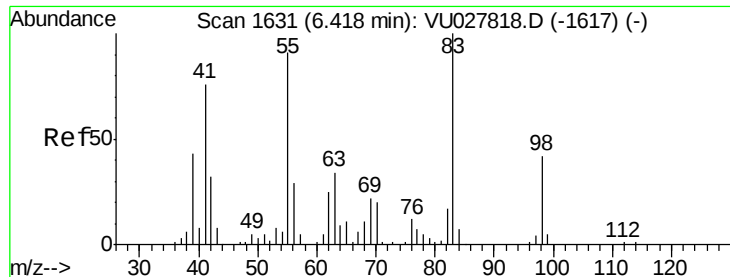




#35
Methylcyclohexane
Concen: 6.148 ug/L
RT: 6.33 min Scan# 1603
Delta R.T. -0.09 min
Lab File: VU027824.D
Acq: 26 Oct 2018 11:36

Instrument :
MSVOA_U
ClientSampleId :
A40G1ME

Tgt Ion: 83 Resp: 7930
Ion Ratio Lower Upper
83 100
55 0.0 71.9 107.9#
98 0.0 34.6 52.0#

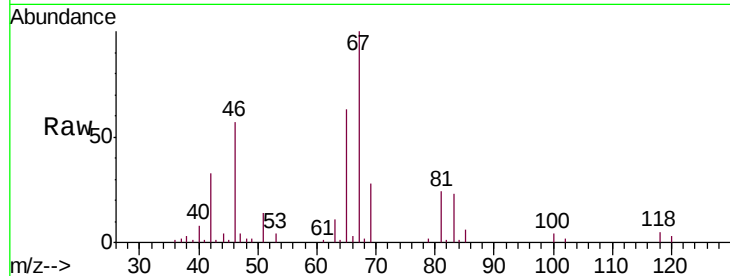


Abundance Ion 83.00 (82.70 to 83.70): VU0
Ion 55.00 (54.70 to 55.70): VU0
Ion 98.00 (97.70 to 98.70): VU0

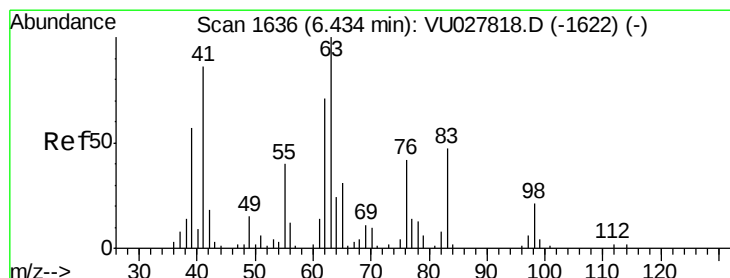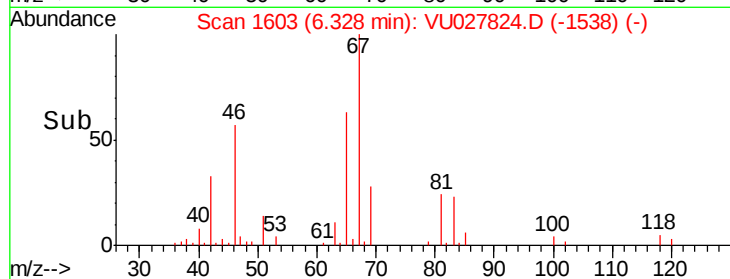
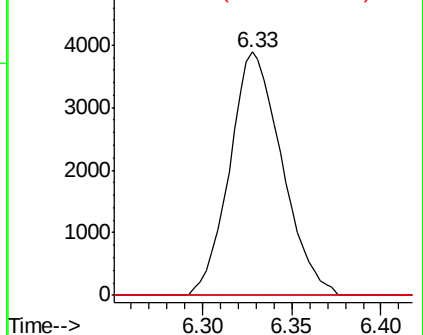



#37
1,2-Dichloropropane
Concen: 4.587 ug/L
RT: 6.33 min Scan# 1604
Delta R.T. -0.10 min
Lab File: VU027824.D
Acq: 26 Oct 2018 11:36

Tgt Ion: 63 Resp: 4038
Ion Ratio Lower Upper
63 100
112 0.0 2.6 3.8#

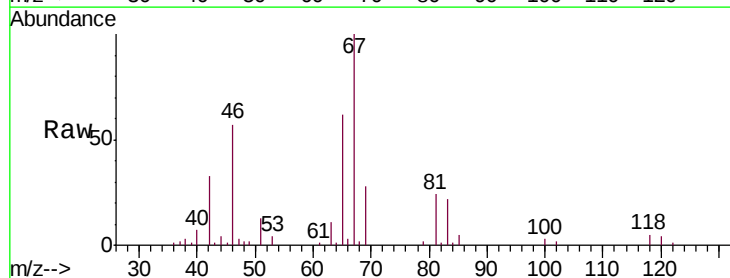

Abundance Ion 63.00 (62.70 to 63.70): VU0
Ion 112.00 (111.70 to 112.70): V

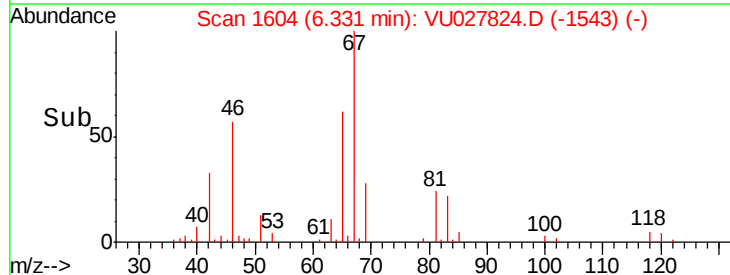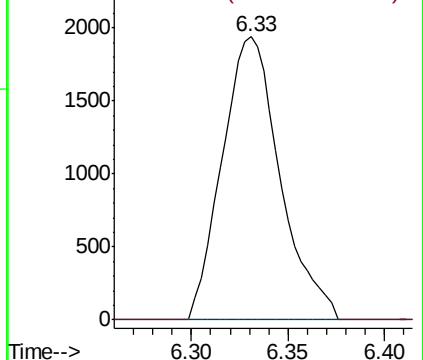




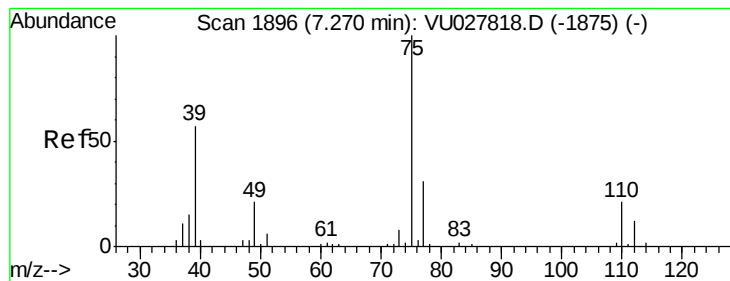


#39

cis-1,3-Dichloropropene
Concen: 0.750 ug/L
RT: 7.23 min Scan# 1883
Delta R.T. -0.04 min
Lab File: VU027824.D
Acq: 26 Oct 2018 11:36

Instrument :
MSVOA_U
ClientSampleId :
A40G1ME




Tgt Ion: 75 Resp: 1017
Ion Ratio Lower Upper
75 100
77 48.8 22.5 41.7#

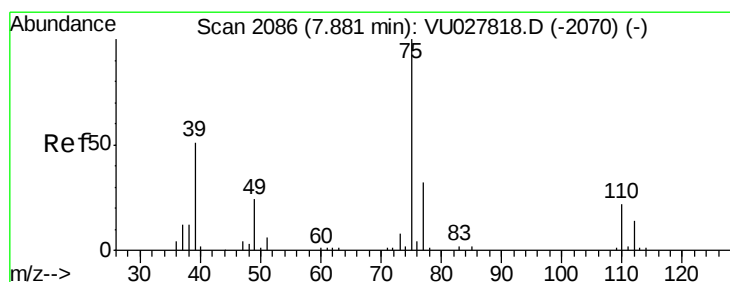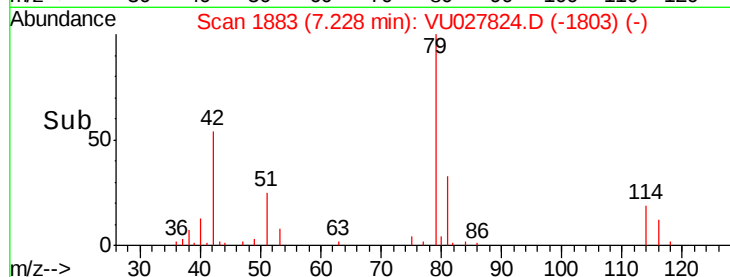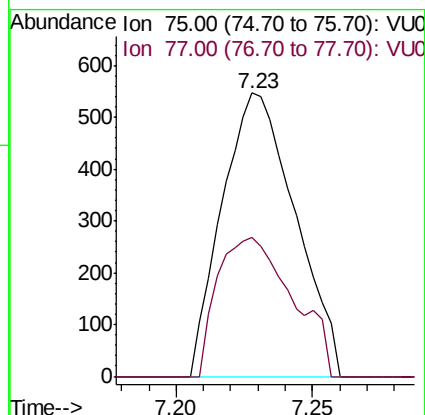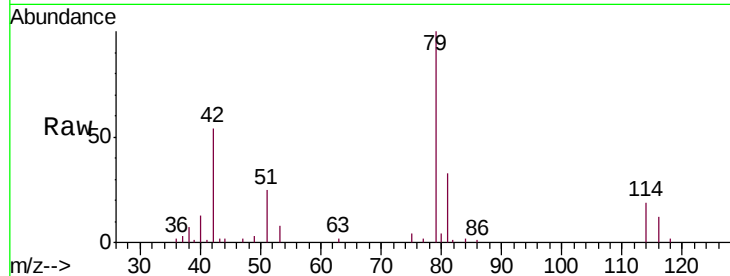


#44

trans-1,3-Dichloropropene
Concen: 0.554 ug/L
RT: 7.85 min Scan# 2076
Delta R.T. -0.03 min
Lab File: VU027824.D
Acq: 26 Oct 2018 11:36

Tgt Ion: 75 Resp: 710
Ion Ratio Lower Upper
75 100
77 29.7 22.8 42.4

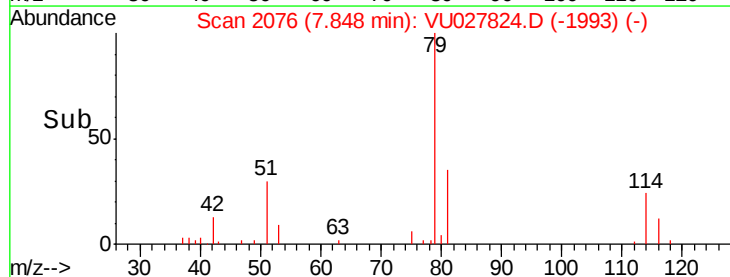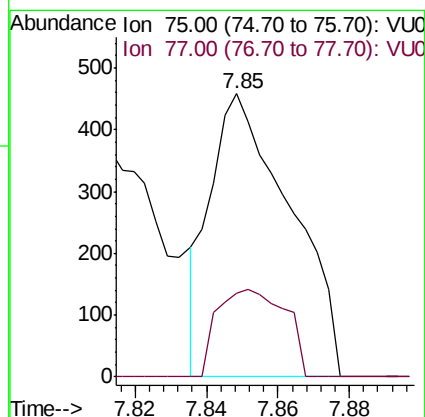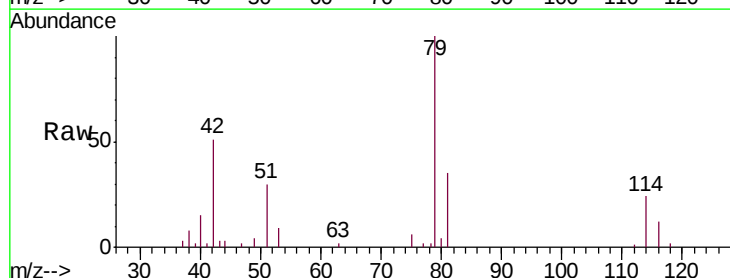

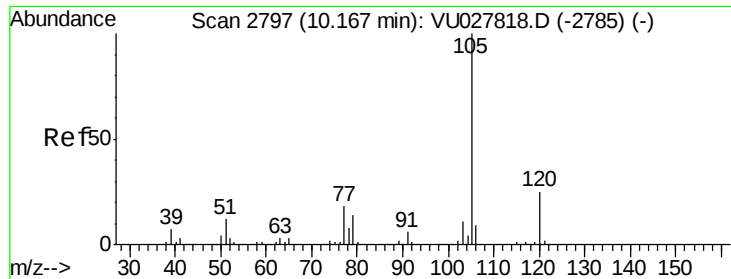

#56

Isopropylbenzene

Concen: 0.509 ug/L

RT: 10.17 min Scan# 2798

Delta R.T. 0.00 min

Lab File: VU027824.D

Acq: 26 Oct 2018 11:36


Instrument :

MSVOA_U

ClientSampleId :

A40G1ME




Tgt Ion:	105	Resp:	1714
Ion	Ratio	Lower	Upper
105	100		
120	22.3	21.0	31.6
77	27.0	13.7	20.5#

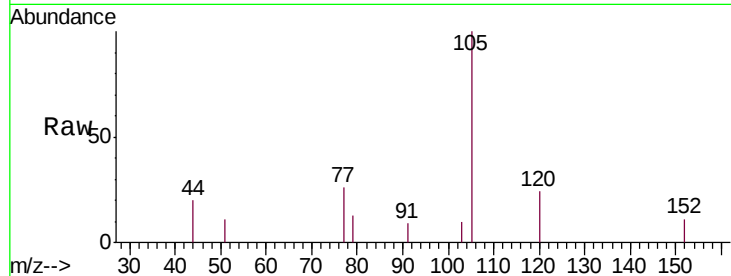

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU

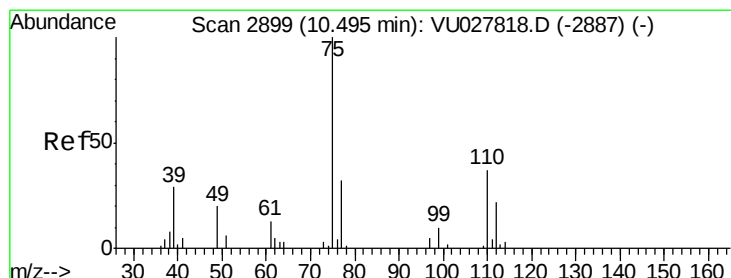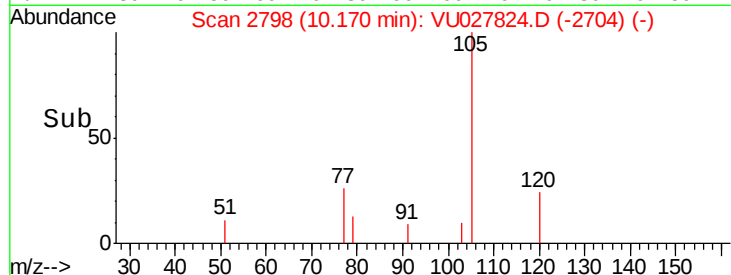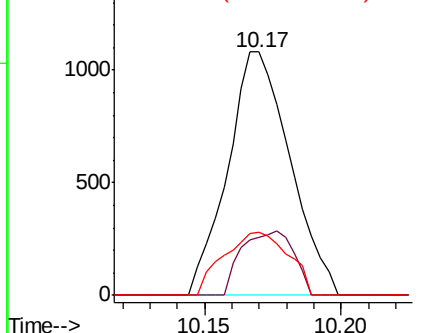

#59

1,2,3-Trichloropropane

Concen: 8.474 ug/L


RT: 11.49 min Scan# 3208

Delta R.T. 0.99 min

Lab File: VU027824.D



Acq: 26 Oct 2018 11:36


Tgt Ion:	75	Resp:	8815
Ion	Ratio	Lower	Upper
75	100		
77	33.0	26.5	39.7

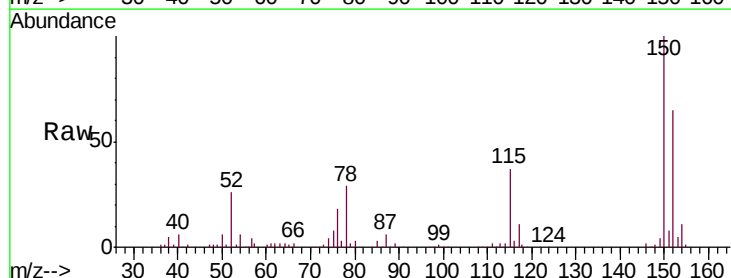

Abundance Ion 75.00 (74.70 to 75.70): VU

Ion 77.00 (76.70 to 77.70): VU

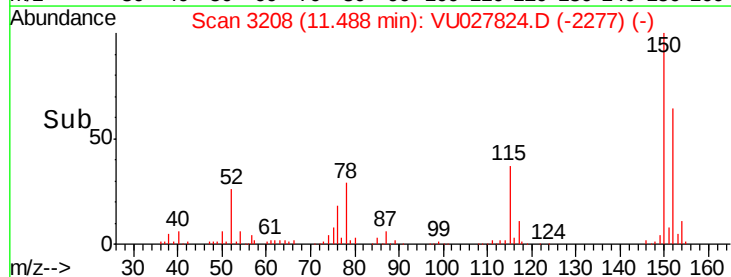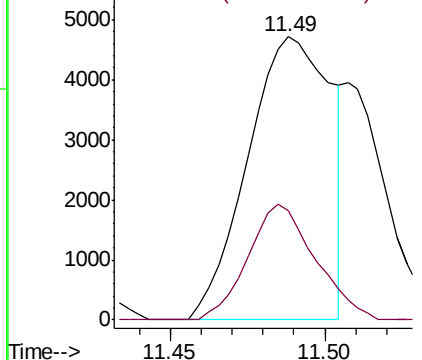


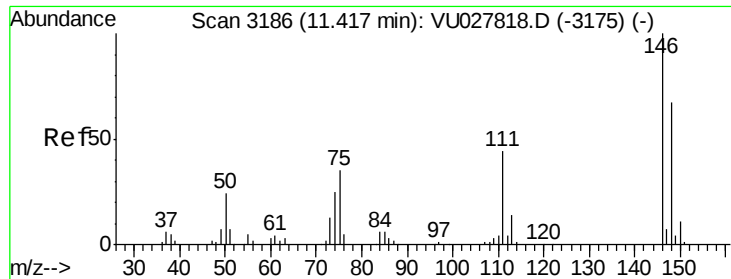




#62
 1,3-Dichlorobenzene
 Concen: 1.311 ug/L
 RT: 11.42 min Scan# 3187
 Delta R.T. 0.00 min
 Lab File: VU027824.D
 Acq: 26 Oct 2018 11:36

Instrument :
 MSVOA_U
 ClientSampleId :
 A40G1ME

Tgt Ion:146 Resp: 2251
 Ion Ratio Lower Upper
 146 100
 111 46.8 28.1 52.3
 148 66.5 43.7 81.1

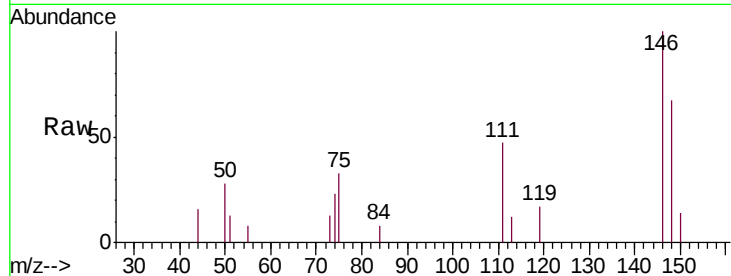


Abundance Ion 146.00 (145.70 to 146.70): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

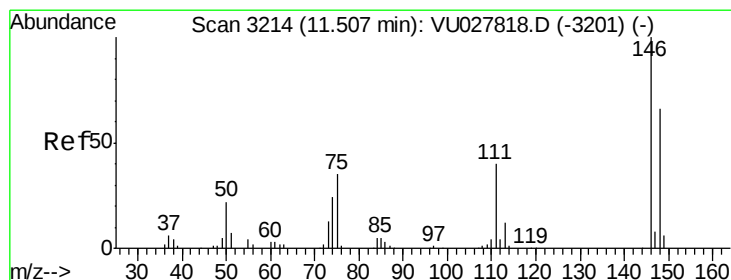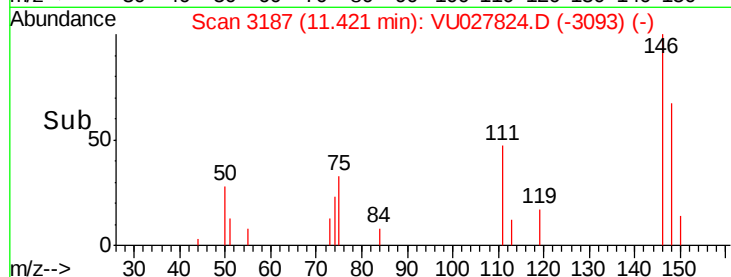
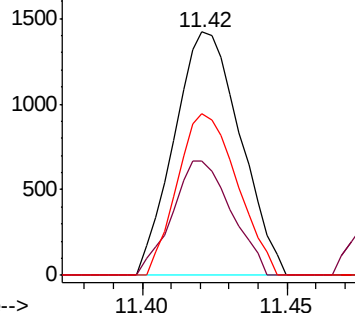



#63
 1,4-Dichlorobenzene
 Concen: 8.844 ug/L
 RT: 11.51 min Scan# 3215
 Delta R.T. 0.00 min
 Lab File: VU027824.D
 Acq: 26 Oct 2018 11:36

Tgt Ion:146 Resp: 15484
 Ion Ratio Lower Upper
 146 100
 111 41.1 27.5 51.1
 148 62.5 44.1 81.9

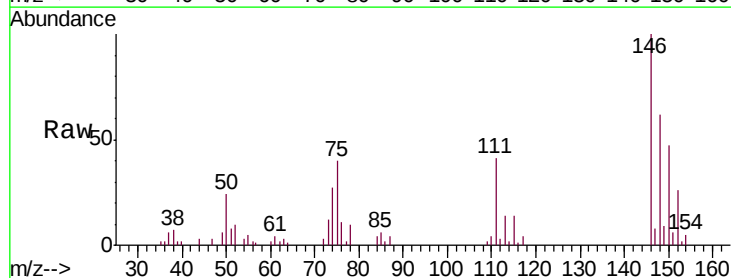

Abundance Ion 146.00 (145.70 to 146.70): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

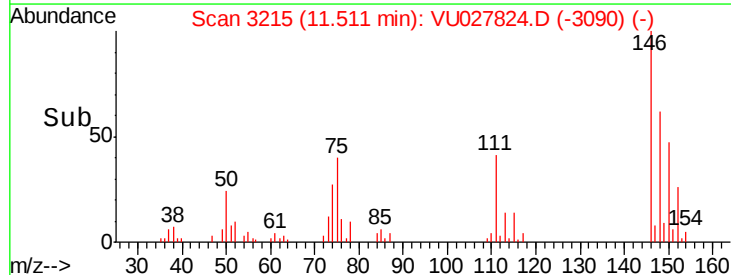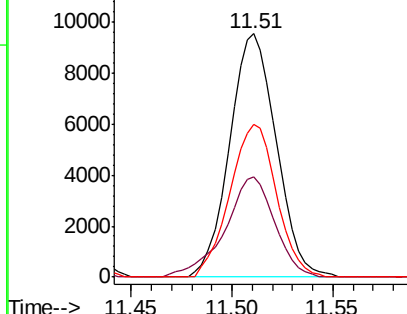

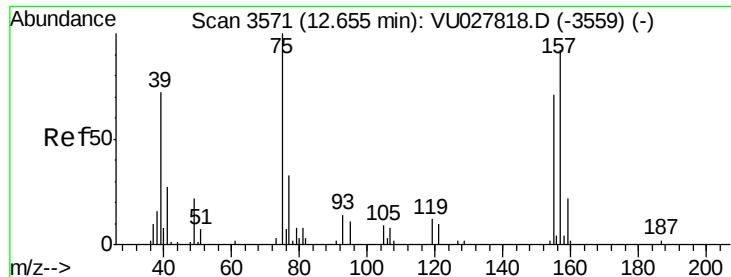

#66

1,2-Dibromo-3-chloropropane

Concen: 3.185 ug/L

RT: 12.38 min Scan# 3484

Delta R.T. -0.28 min

Lab File: VU027824.D

Acq: 26 Oct 2018 11:36

Instrument :

MSVOA_U

ClientSampleId :

A40G1ME



Tgt Ion: 75 Resp: 1172

Ion Ratio Lower Upper

75 100

155 47.4 57.4 86.2#

157 0.0 75.9 113.9#

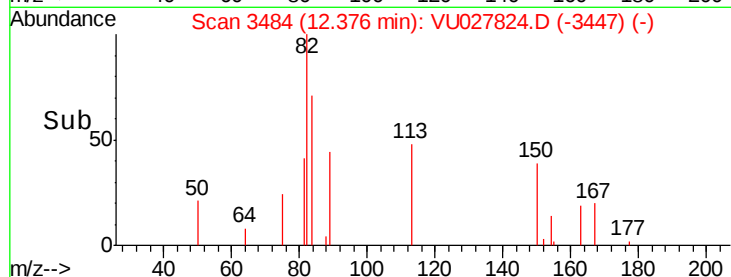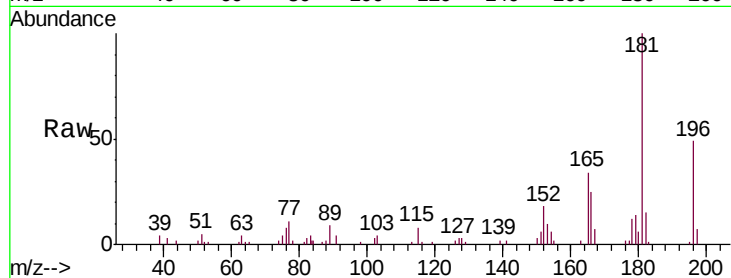

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 155.00 (154.70 to 155.70): V

Ion 157.00 (156.70 to 157.70): V

