

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102618\
 Data File : VU027832.D
 Acq On : 26 Oct 2018 14:42
 Operator : MD/SY
 Sample : J5668-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBQ7

Quant Time: Oct 27 02:58:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 27 01:41:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	111670	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	102432	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	48841	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	31376	36.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.22%
7) Chloroethane-d5	1.68	69	26481	39.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.18%
11) 1,1-Dichloroethene-d2	2.27	63	46985	30.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.06%
21) 2-Butanone-d5	4.18	46	74593	100.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.74%
24) Chloroform-d	4.65	84	67941	43.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.00%
26) 1,2-Dichloroethane-d4	5.31	65	48579	44.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.82%
32) Benzene-d6	5.34	84	129381	44.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.70%
36) 1,2-Dichloropropane-d6	6.33	67	48252	46.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.66%
41) Toluene-d8	7.57	98	116301	43.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.44%
43) trans-1,3-Dichloropropene-	7.85	79	22331	44.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.30%
47) 2-Hexanone-d5	8.31	63	53604	100.58	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.58%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	63977	47.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	44161	44.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.28%


Target Compounds					Ovalue
13) Acetone	2.32	43	4515	8.754 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102618\
Data File : VU027832.D
Acq On : 26 Oct 2018 14:42
Operator : MD/SY
Sample : J5668-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBQ7

Quant Time: Oct 27 02:58:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 01:41:17 2018
Response via : Initial Calibration

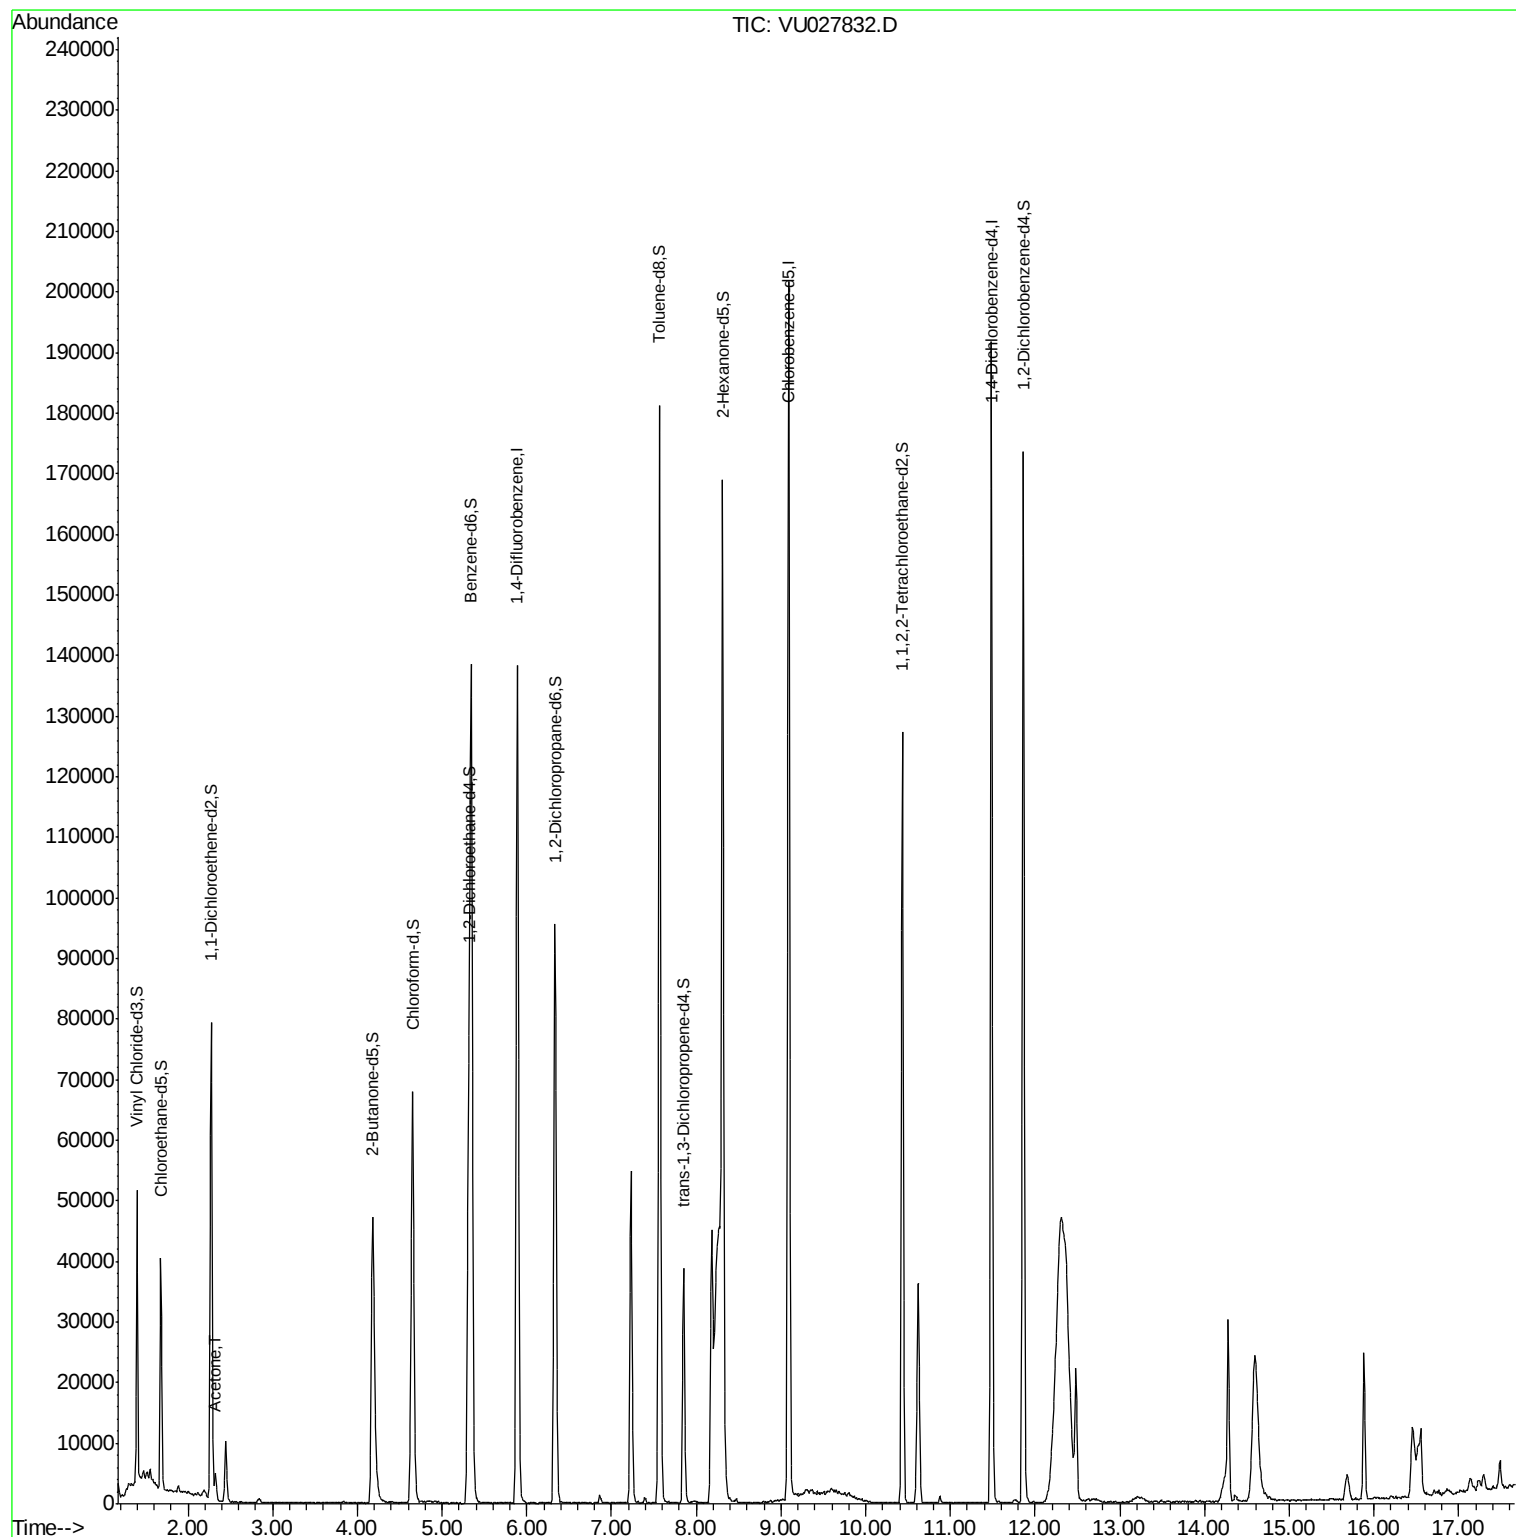

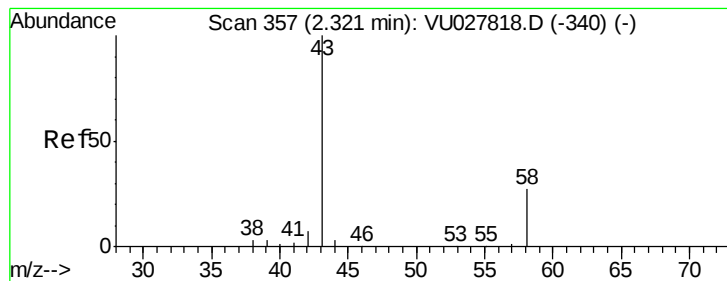

#13
 Acetone
 Concen: 8.754 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU027832.D
 Acq: 26 Oct 2018 14:42

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBQ7

Tot Ion: 43 Resp: 4515
 Ion Ratio Lower Upper
 43 100
 58 26.7 0.0 57.4

