

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U102618\
 Data File : VU027837.D
 Acq On : 26 Oct 2018 16:38
 Operator : MD/SY
 Sample : J5668-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBS1

Quant Time: Oct 27 03:44:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 27 01:41:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	122623	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	112698	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	50984	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	28082	29.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	58.86%#
7) Chloroethane-d5	1.68	69	24850	33.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	67.66%#
11) 1,1-Dichloroethene-d2	2.28	63	43099	25.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	50.16%#
21) 2-Butanone-d5	4.18	46	69454	85.42	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.42%
24) Chloroform-d	4.65	84	62148	36.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.46%
26) 1,2-Dichloroethane-d4	5.31	65	45951	38.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.38%
32) Benzene-d6	5.34	84	121365	37.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.62%
36) 1,2-Dichloropropane-d6	6.33	67	45031	39.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	78.60%
41) Toluene-d8	7.57	98	108118	36.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.04%#
43) trans-1,3-Dichloropropene-	7.85	79	19814	35.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.22%
47) 2-Hexanone-d5	8.31	63	51664	88.11	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.11%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	60672	41.00	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	42408	40.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.22%


Target Compounds					Ovalue
13) Acetone	2.32	43	5163	9.116 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102618\
Data File : VU027837.D
Acq On : 26 Oct 2018 16:38
Operator : MD/SY
Sample : J5668-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBS1

Quant Time: Oct 27 03:44:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 01:41:17 2018
Response via : Initial Calibration

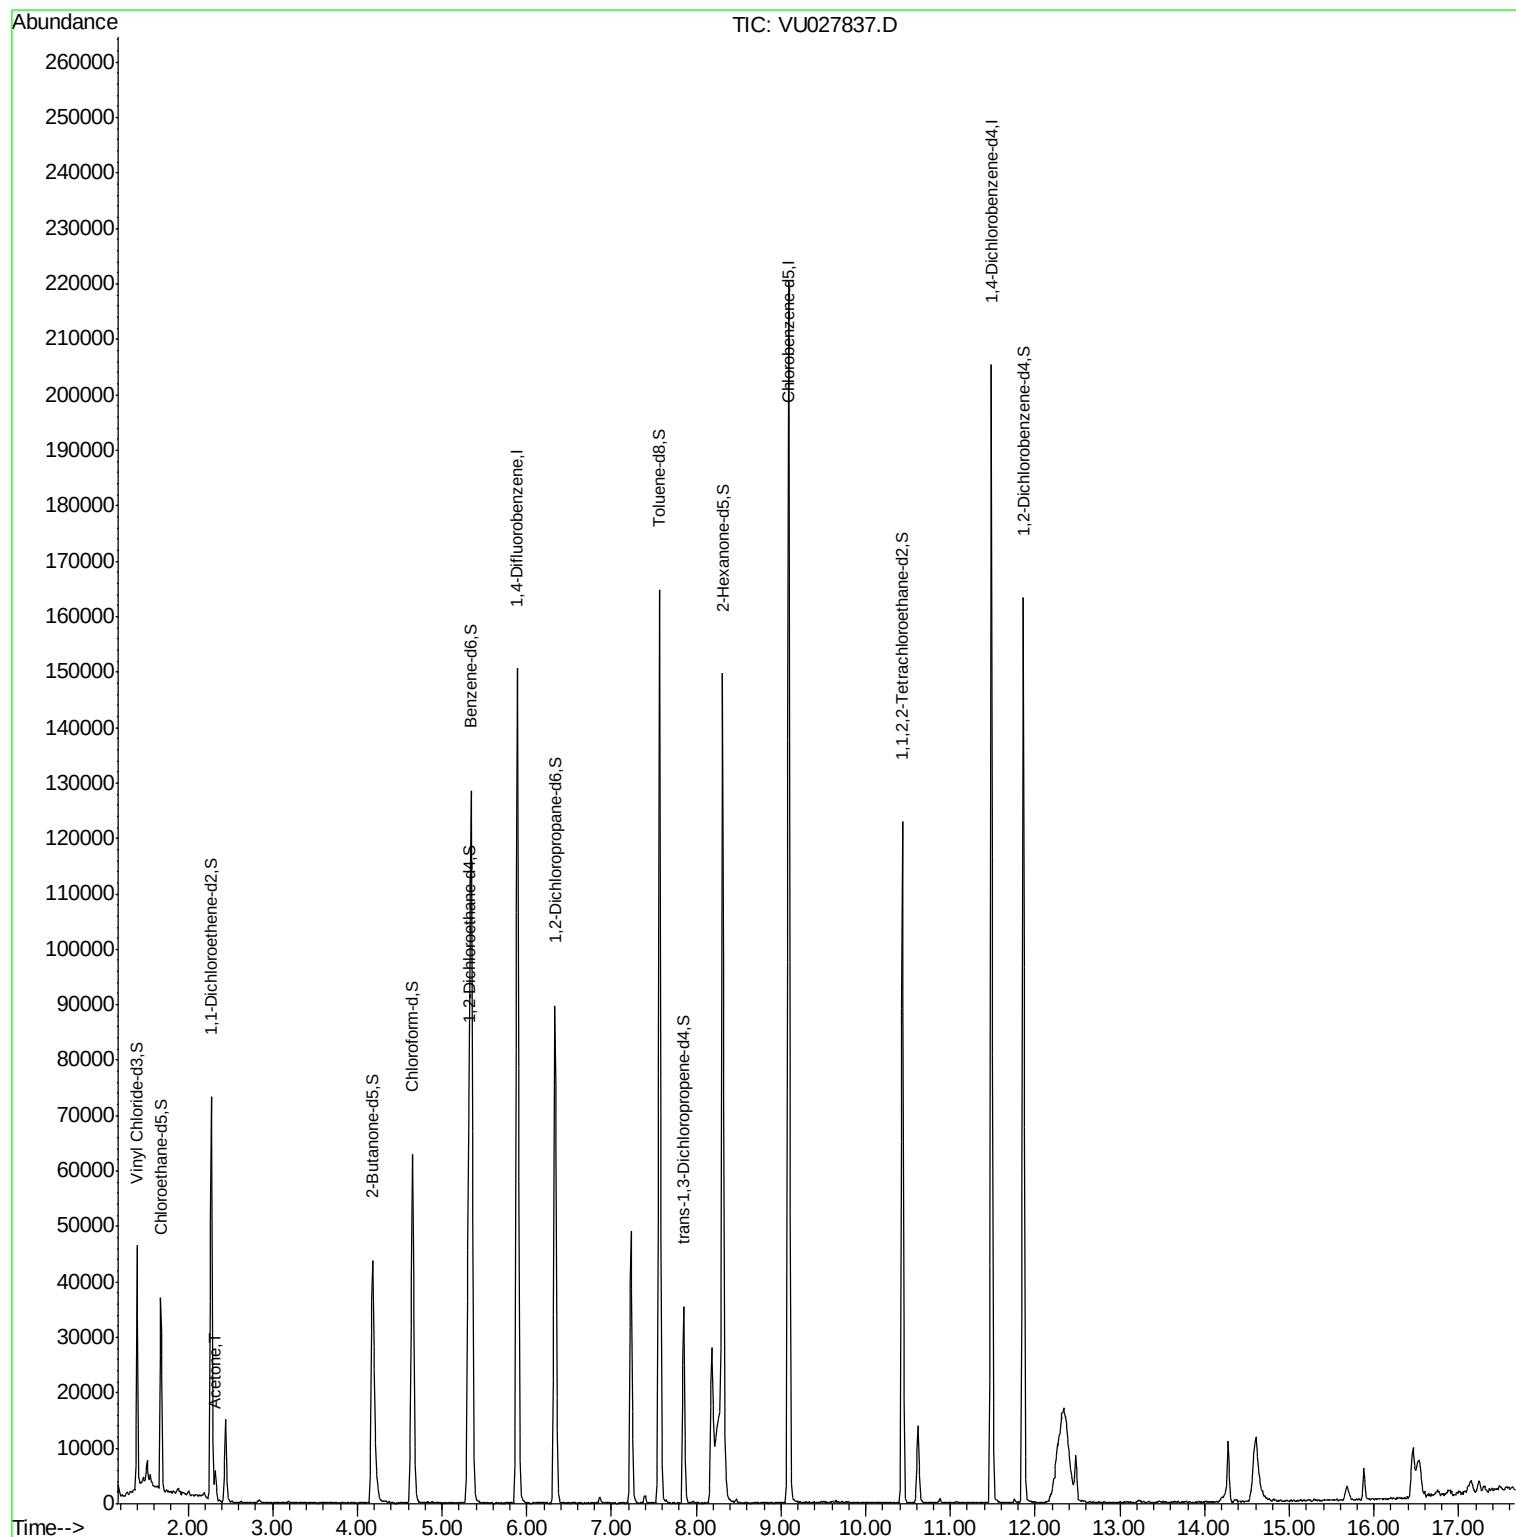

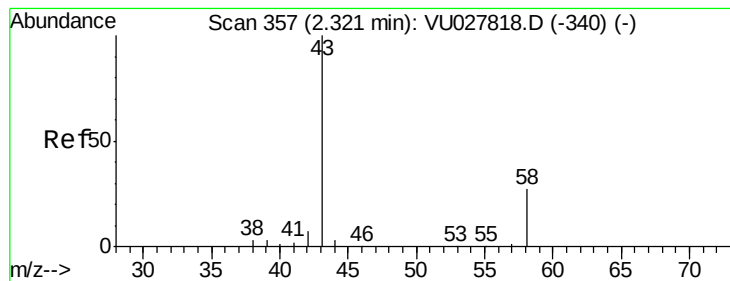

#13
 Acetone
 Concen: 9.116 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU027837.D
 Acq: 26 Oct 2018 16:38

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBS1

Tot Ion: 43 Resp: 5163
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 57.4

