


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102618\
Data File : VU027817.D
Acq On : 26 Oct 2018 07:43
Operator : MD/SY
Sample : BFB49
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Title : VOC Analysis
Last Update : Sat Oct 27 01:41:17 2018

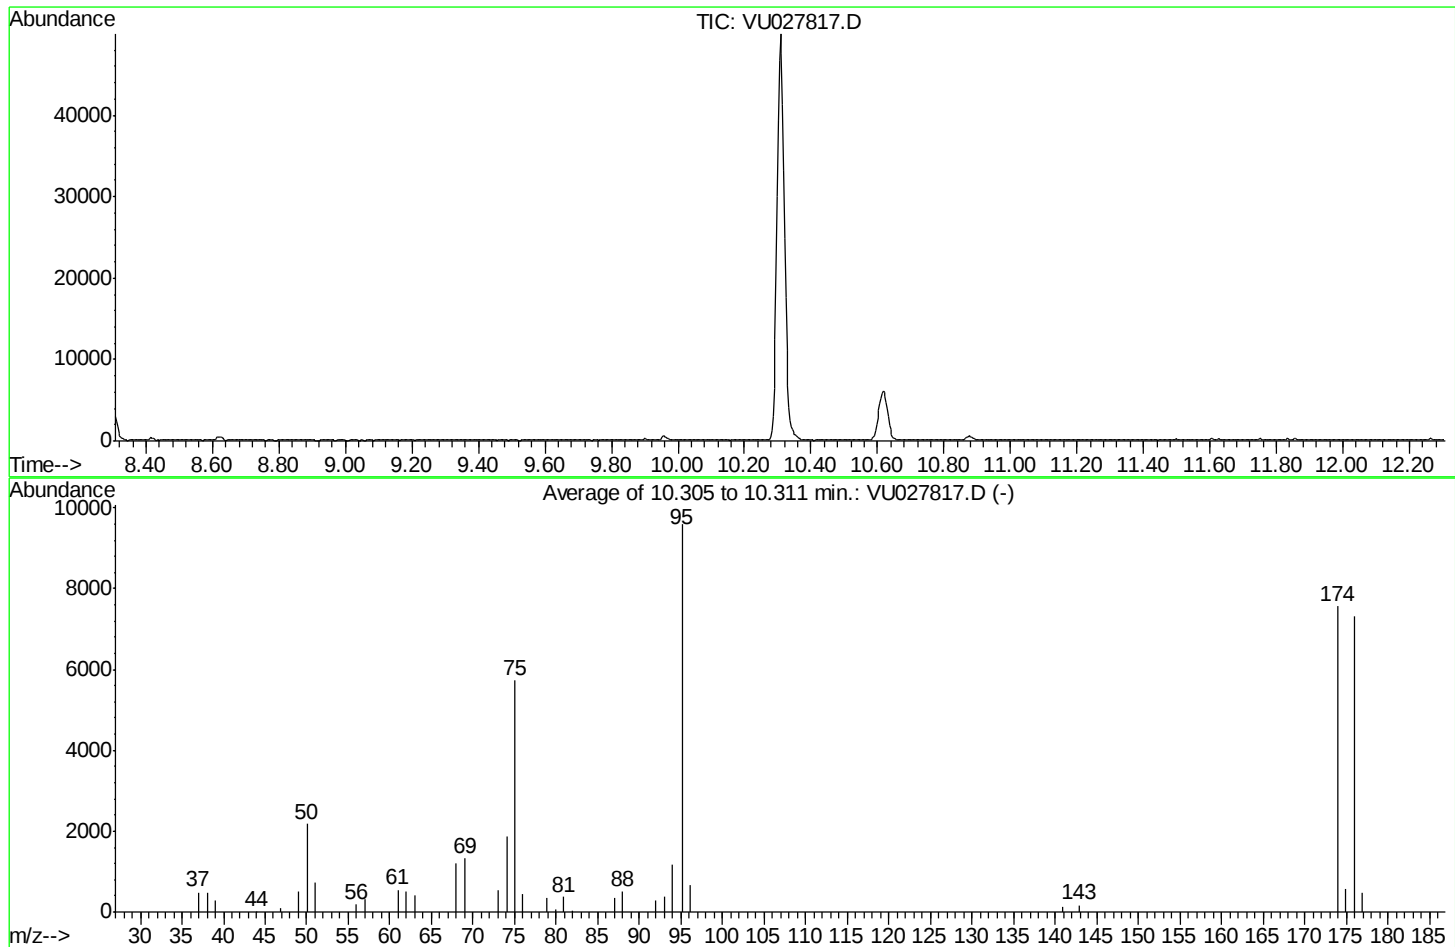

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	2176	PASS
75	95	30	80	59.6	5720	PASS
95	95	100	100	100.0	9592	PASS
96	95	5	9	7.0	674	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	7556	PASS
175	174	5	9	7.7	580	PASS
176	174	95	101	96.6	7302	PASS
177	176	5	9	6.5	475	PASS

m/z	Abundance
44.00	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
37.00	507.0
38.00	547.0
39.00	288.0
44.00	200.0
46.90	132.0
49.00	498.0
50.10	2181.0
51.00	795.0
56.00	182.0
56.90	298.0
61.00	561.0
62.00	489.0
63.00	422.0
68.00	1221.0
69.00	1359.0
73.00	513.0
74.10	1791.0
75.10	5754.0
76.00	433.0
78.90	382.0
80.90	335.0
86.90	369.0
88.00	508.0
92.00	346.0
93.00	383.0
94.00	1128.0
95.10	9225.0
96.00	650.0
140.90	108.0
142.90	167.0
174.00	7009.0
174.90	508.0
176.00	6891.0
176.90	447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
37.00	510.0
38.00	472.0
39.00	296.0
44.00	205.0
46.90	129.0
49.00	541.0
50.00	2251.0
51.00	750.0
56.00	184.0
57.00	345.0
61.00	551.0
62.00	535.0
63.00	437.0
68.00	1279.0
69.00	1362.0
73.00	564.0
74.10	1923.0
75.10	5949.0
76.00	469.0
78.90	378.0
80.00	105.0
80.90	396.0
81.90	101.0
86.90	363.0
88.00	527.0
92.00	313.0
93.00	380.0
94.00	1235.0
95.10	9915.0
96.00	680.0
140.90	118.0
142.90	175.0
174.00	7890.0
175.00	608.0
176.00	7533.0
176.90	505.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
37.00	452.0
38.00	404.0
39.00	234.0
44.00	212.0
49.00	500.0
50.00	2096.0
51.10	666.0
56.00	170.0
57.00	353.0
61.00	523.0
62.00	528.0
63.00	409.0
68.00	1152.0
69.10	1234.0
73.00	544.0
74.10	1877.0
75.00	5459.0
76.00	440.0
78.90	330.0
80.00	116.0
80.90	391.0
87.00	344.0
88.00	446.0
91.90	245.0
93.00	366.0
94.00	1191.0
95.10	9638.0
96.10	694.0
140.90	113.0
142.90	148.0
174.00	7771.0
175.00	626.0
176.00	7483.0
176.90	473.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49