

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102619\
 Data File : VU035525.D
 Acq On : 26 Oct 2019 17:54
 Operator : JC/SP
 Sample : K5538-02 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF6M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	6	10	17	rVB	6602	6187	0.26%	0.035%
2	1.617	79	86	99	rVB	326782	353864	15.03%	2.017%
3	1.932	176	184	199	rBV	259591	342751	14.56%	1.953%
4	2.597	379	391	408	rBV	473004	780802	33.17%	4.450%
5	2.790	449	451	452	rBV	820	318	0.01%	0.002%
6	2.957	500	503	504	rBV	510	313	0.01%	0.002%
7	3.028	523	525	529	rBV2	534	314	0.01%	0.002%
8	3.080	536	541	542	rBV2	1686	1304	0.06%	0.007%
9	3.170	565	569	572	rBV2	349	287	0.01%	0.002%
10	3.234	572	589	604	rBV2	17237	41349	1.76%	0.236%
11	3.385	634	636	641	rVB4	475	335	0.01%	0.002%
12	3.539	682	684	686	rVV2	407	264	0.01%	0.002%
13	3.549	686	687	690	rVV2	613	287	0.01%	0.002%
14	3.568	690	693	698	rVB3	366	317	0.01%	0.002%
15	3.735	741	745	751	rVB4	606	623	0.03%	0.004%
16	3.764	751	754	757	rBV	525	365	0.02%	0.002%
17	3.803	764	766	771	rBV2	338	311	0.01%	0.002%
18	3.858	776	783	789	rBV3	590	701	0.03%	0.004%
19	4.015	829	832	834	rVV	405	296	0.01%	0.002%
20	4.031	834	837	840	rVB	329	264	0.01%	0.002%
21	4.125	859	866	869	rBV2	253	372	0.02%	0.002%
22	4.240	897	902	908	rVB3	468	417	0.02%	0.002%
23	4.276	908	913	921	rBV3	385	494	0.02%	0.003%
24	4.353	934	937	940	rBV2	469	274	0.01%	0.002%
25	4.440	961	964	967	rBV2	357	316	0.01%	0.002%
26	4.626	1019	1022	1026	rVB	517	427	0.02%	0.002%
27	4.694	1026	1043	1071	rBV	222779	553957	23.53%	3.157%
28	5.115	1158	1174	1193	rBV	408668	895333	38.03%	5.102%
29	5.327	1238	1240	1241	rBV2	978	401	0.02%	0.002%
30	5.456	1278	1280	1286	rVB3	272	259	0.01%	0.001%
31	5.581	1314	1319	1323	rVB4	571	605	0.03%	0.003%
32	5.629	1331	1334	1337	rBV4	590	428	0.02%	0.002%
33	5.771	1356	1378	1417	rBV2	901717	2354283	100.00%	13.416%
34	6.292	1470	1540	1590	rBV	836737	2176052	92.43%	12.401%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102619\
 Data File : VU035525.D
 Acq On : 26 Oct 2019 17:54
 Operator : JC/SP
 Sample : K5538-02 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF6M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
 Title : VOC Analysis

35	6.735	1663	1678	1704	rBV	545890	1075766	45.69%	6.130%
36	7.092	1782	1789	1799	rVB3	2918	4653	0.20%	0.027%
37	7.603	1934	1948	1976	rBV	284611	529809	22.50%	3.019%
38	7.935	2036	2051	2072	rBV	1042848	1854978	78.79%	10.571%
39	8.214	2123	2138	2164	rBV	198787	365385	15.52%	2.082%
40	8.497	2219	2226	2232	rBV6	1280	2060	0.09%	0.012%
41	8.623	2260	2265	2267	rBV5	966	714	0.03%	0.004%
42	8.681	2268	2283	2331	rBV	368544	1074994	45.66%	6.126%
43	8.890	2342	2348	2349	rBV4	579	615	0.03%	0.004%
44	9.092	2409	2411	2414	rBV2	465	286	0.01%	0.002%
45	9.121	2417	2420	2421	rVV2	388	262	0.01%	0.001%
46	9.144	2425	2427	2431	rVB2	605	402	0.02%	0.002%
47	9.166	2431	2434	2435	rBV2	532	318	0.01%	0.002%
48	9.253	2452	2461	2469	rBV8	2471	4417	0.19%	0.025%
49	9.295	2473	2474	2479	rVB3	488	290	0.01%	0.002%
50	9.324	2479	2483	2484	rBV3	405	281	0.01%	0.002%
51	9.340	2486	2488	2495	rVB4	604	516	0.02%	0.003%
52	9.375	2495	2499	2502	rBV2	545	408	0.02%	0.002%
53	9.449	2509	2522	2557	rBV	986383	1788344	75.96%	10.191%
54	9.597	2565	2568	2571	rBV4	898	804	0.03%	0.005%
55	9.665	2586	2589	2590	rBV2	529	255	0.01%	0.001%
56	9.722	2601	2607	2616	rVB6	1694	2461	0.10%	0.014%
57	9.767	2617	2621	2624	rBV5	536	497	0.02%	0.003%
58	9.854	2644	2648	2651	rBV2	433	370	0.02%	0.002%
59	10.005	2692	2695	2698	rVB3	455	295	0.01%	0.002%
60	10.121	2724	2731	2732	rBV5	1047	936	0.04%	0.005%
61	10.182	2747	2750	2754	rVB3	642	430	0.02%	0.002%
62	10.275	2773	2779	2783	rBV3	506	551	0.02%	0.003%
63	10.365	2805	2807	2812	rVB2	711	354	0.02%	0.002%
64	10.420	2822	2824	2827	rBV2	433	339	0.01%	0.002%
65	10.488	2841	2845	2848	rBV4	553	568	0.02%	0.003%
66	10.517	2848	2854	2859	rVV2	1120	1001	0.04%	0.006%
67	10.674	2898	2903	2904	rBV2	465	328	0.01%	0.002%
68	10.787	2923	2938	2958	rBV	642657	1105361	46.95%	6.299%
69	10.886	2966	2969	2972	rBV2	450	302	0.01%	0.002%
70	11.073	3023	3027	3033	rBV3	733	752	0.03%	0.004%
71	11.102	3034	3036	3038	rVV2	694	364	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102619\
 Data File : VU035525.D
 Acq On : 26 Oct 2019 17:54
 Operator : JC/SP
 Sample : K5538-02 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF6M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
 Title : VOC Analysis

72	11.127	3042	3044	3047	rVB3	724	367	0.02%	0.002%
73	11.192	3059	3064	3067	rBV2	325	268	0.01%	0.002%
74	11.243	3077	3080	3082	rBV3	523	355	0.02%	0.002%
75	11.481	3150	3154	3155	rBV3	429	297	0.01%	0.002%
76	11.549	3171	3175	3177	rBV2	412	313	0.01%	0.002%
77	11.600	3187	3191	3196	rBV2	589	478	0.02%	0.003%
78	11.658	3206	3209	3213	rBV3	380	276	0.01%	0.002%
79	11.713	3223	3226	3228	rBV2	530	357	0.02%	0.002%
80	11.774	3241	3245	3250	rVV5	1270	1284	0.05%	0.007%
81	11.841	3253	3266	3284	rVV	607905	1078586	45.81%	6.147%
82	11.915	3287	3289	3292	rBV	396	254	0.01%	0.001%
83	11.963	3300	3304	3310	rBV5	740	664	0.03%	0.004%
84	12.041	3325	3328	3333	rVB3	633	522	0.02%	0.003%
85	12.076	3333	3339	3345	rVB4	656	710	0.03%	0.004%
86	12.150	3356	3362	3364	rBV2	575	663	0.03%	0.004%
87	12.221	3370	3384	3400	rBV	648098	1119704	47.56%	6.381%
88	12.340	3419	3421	3426	rVB3	768	599	0.03%	0.003%
89	12.565	3489	3491	3493	rBV	572	336	0.01%	0.002%
90	12.706	3532	3535	3538	rBV	577	472	0.02%	0.003%
91	12.918	3596	3601	3604	rBV2	569	636	0.03%	0.004%
92	13.034	3634	3637	3642	rBV3	869	818	0.03%	0.005%
93	13.082	3649	3652	3658	rVB3	715	594	0.03%	0.003%
94	13.131	3664	3667	3670	rBV3	607	319	0.01%	0.002%
95	13.198	3685	3688	3692	rBV3	655	678	0.03%	0.004%
96	13.314	3721	3724	3727	rBV2	741	578	0.02%	0.003%
97	13.960	3922	3925	3927	rBV3	724	432	0.02%	0.002%
98	14.105	3967	3970	3972	rBV3	1004	745	0.03%	0.004%
99	14.246	4012	4014	4017	rBV2	594	435	0.02%	0.002%
100	14.658	4139	4142	4145	rBV3	1102	781	0.03%	0.004%


Sum of corrected areas: 17547857

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102619\
Data File : VU035525.D
Acq On : 26 Oct 2019 17:54
Operator : JC/SP
Sample : K5538-02 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF6M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

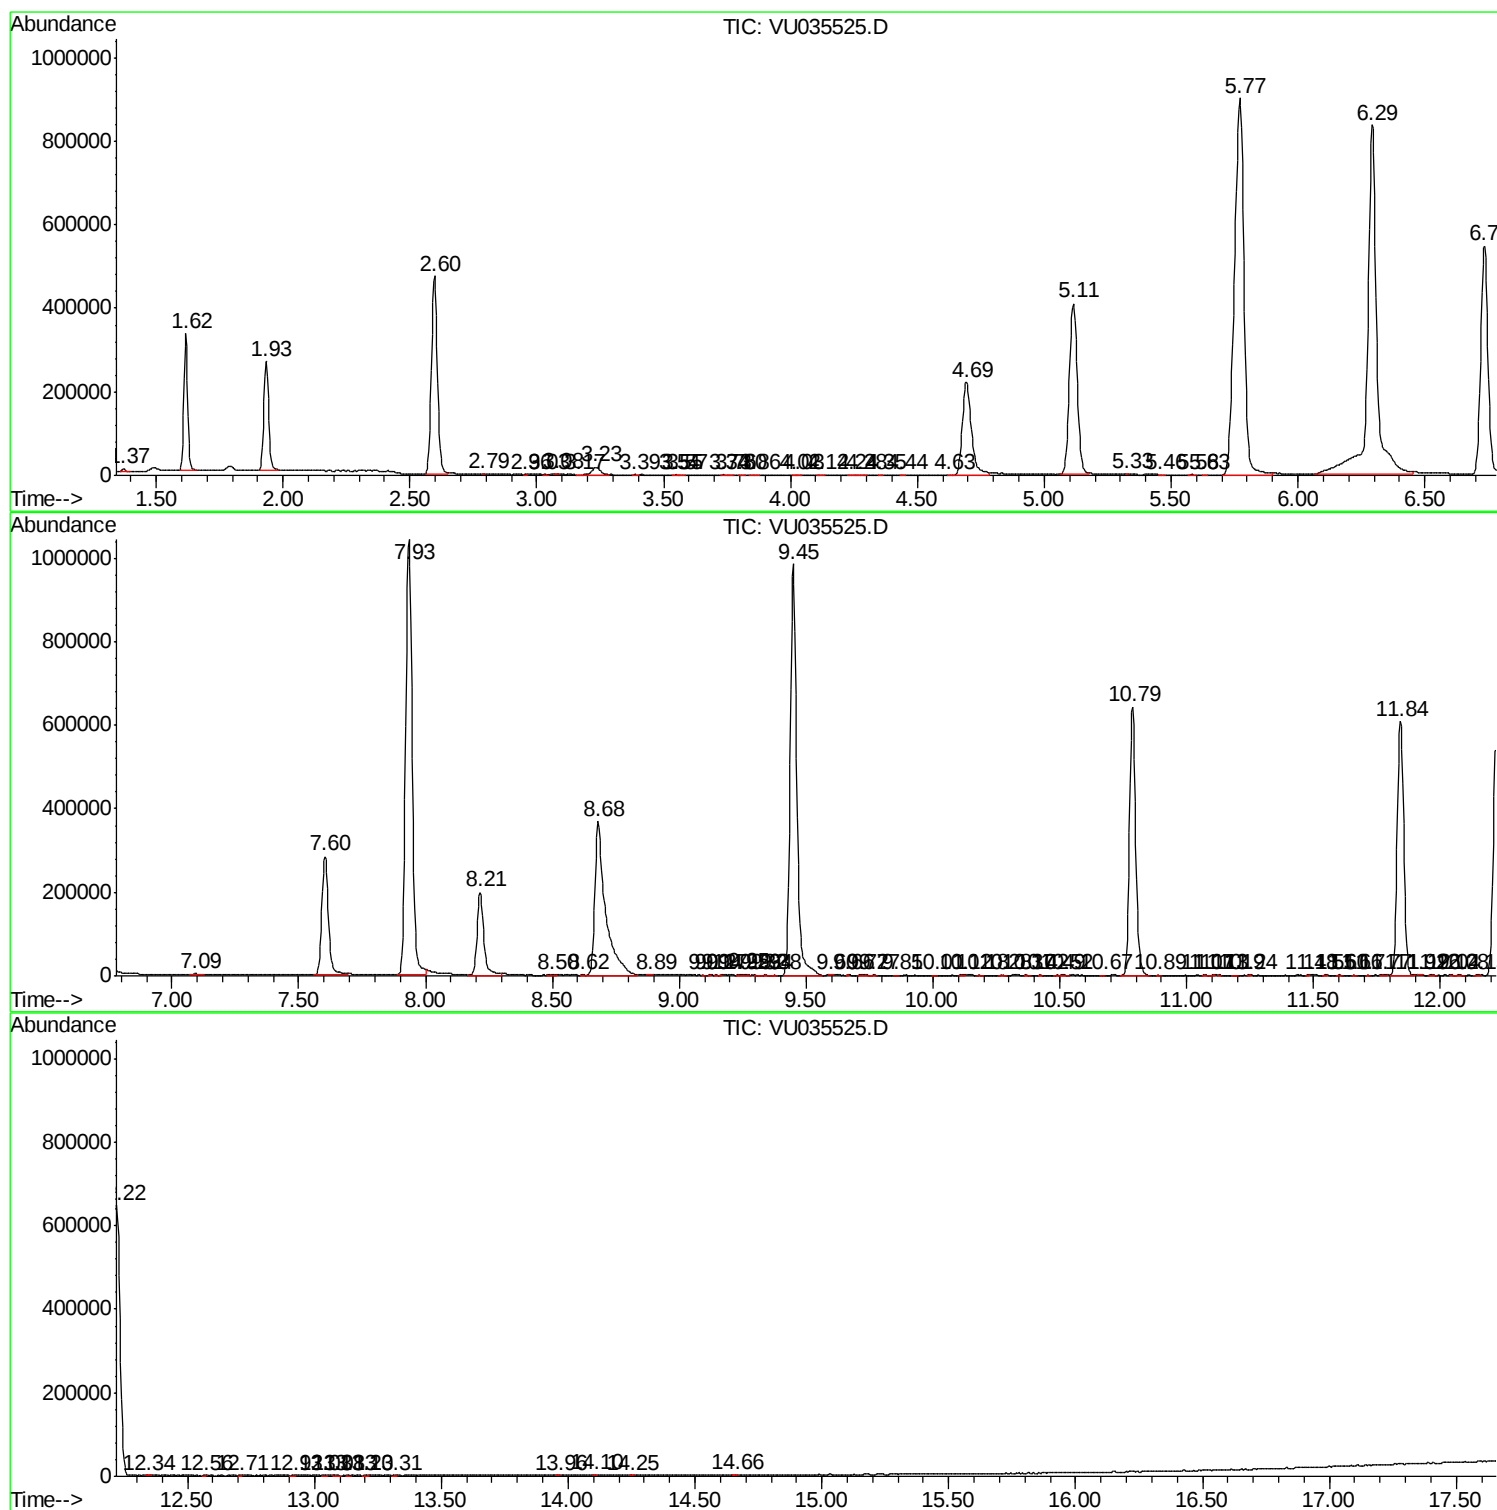

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102619\
Data File : VU035525.D
Acq On : 26 Oct 2019 17:54
Operator : JC/SP
Sample : K5538-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF6M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102619\
Data File : VU035525.D
Acq On : 26 Oct 2019 17:54
Operator : JC/SP
Sample : K5538-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF6M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
