


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102619\
Data File : VU035508.D
Acq On : 26 Oct 2019 10:09
Operator : JC/SP
Sample : BFB46
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102619WMA.M
Title : VOC Analysis
Last Update : Wed Oct 30 18:57:43 2019

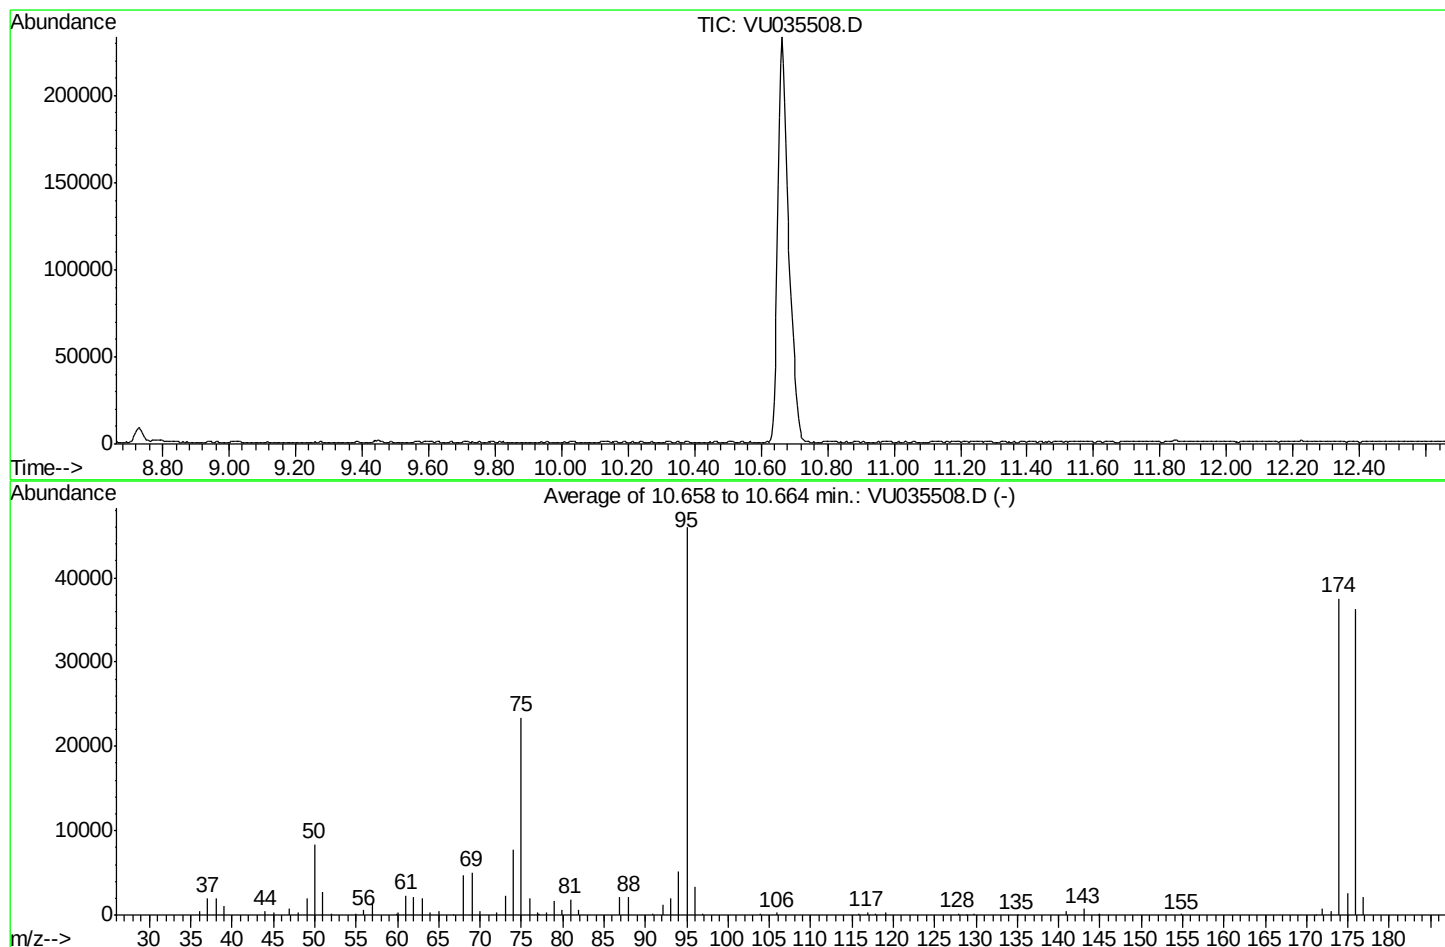

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	8415	PASS
75	95	30	80	50.9	23410	PASS
95	95	100	100	100.0	45981	PASS
96	95	5	9	7.1	3275	PASS
173	174	0.00	2	1.4	507	PASS
174	95	50	120	81.6	37506	PASS
175	174	5	9	6.8	2563	PASS
176	174	95	101	96.7	36277	PASS
177	176	5	9	5.9	2137	PASS

m/z	Abundance
36.00	493.0
37.00	2041.0
38.00	1933.0
39.00	1040.0
40.00	160.0
44.00	1308.0
45.00	224.0
46.90	737.0
47.90	286.0
49.00	1861.0
50.00	8420.0
51.00	2629.0
51.90	119.0
55.00	262.0
55.90	578.0
57.00	1327.0
59.90	414.0
61.00	2324.0
62.00	2054.0
63.00	2021.0
64.00	371.0
65.00	484.0
66.70	110.0
68.00	4651.0
69.00	4761.0
69.90	402.0
72.10	284.0
73.00	2149.0
74.00	7678.0
75.00	22192.0
76.00	1996.0
76.90	253.0
77.10	261.0
78.00	306.0
78.90	1538.0
79.90	518.0
80.90	1867.0
81.90	525.0
86.90	2163.0
87.90	1986.0
90.90	181.0
92.10	1124.0
93.00	2031.0
94.00	4975.0
95.00	43584.0
96.00	3224.0
103.80	223.0
105.90	260.0
115.80	169.0
116.80	272.0
117.70	151.0
119.00	227.0
127.90	138.0
129.80	149.0
141.00	448.0
143.00	643.0
144.70	245.0
154.90	142.0
171.90	810.0
173.00	461.0
173.90	35264.0
174.90	2482.0
175.90	33880.0
176.90	2135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	523.0
37.00	2055.0
38.00	2016.0
39.00	1146.0
40.00	168.0
44.00	1273.0
45.00	246.0
46.90	756.0
47.90	279.0
49.00	2015.0
50.00	8560.0
51.00	2776.0
52.00	120.0
55.00	185.0
56.00	601.0
57.00	1345.0
60.10	418.0
61.00	2358.0
62.00	2208.0
63.00	2091.0
64.00	400.0
65.00	523.0
68.00	4810.0
69.00	5212.0
69.90	400.0
72.10	244.0
73.00	2323.0
74.00	7954.0
75.00	24104.0
76.00	2112.0
76.90	292.0
78.00	282.0
78.90	1733.0
79.80	623.0
80.90	2009.0
81.90	580.0
86.90	2240.0
87.90	2205.0
90.80	146.0
92.00	1183.0
93.00	2088.0
94.00	5202.0
95.00	47296.0
96.00	3385.0
96.90	123.0
103.90	195.0
106.00	271.0
115.80	172.0
116.90	329.0
117.80	134.0
119.00	245.0
127.80	205.0
129.70	153.0
140.90	523.0
143.00	780.0
144.90	256.0
154.80	164.0
171.10	111.0
171.90	834.0
173.00	525.0
173.90	38312.0
174.90	2604.0
175.90	37104.0
176.90	2128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	484.0
37.00	1970.0
38.00	1953.0
39.00	1103.0
39.90	210.0
44.00	1155.0
45.00	251.0
47.00	765.0
48.00	273.0
49.00	1968.0
50.00	8265.0
51.00	2754.0
52.00	117.0
54.90	131.0
56.00	636.0
57.00	1233.0
60.10	441.0
61.00	2256.0
62.00	2244.0
63.00	2039.0
64.00	367.0
64.90	476.0
68.00	4557.0
69.00	5163.0
69.90	383.0
72.00	232.0
73.00	2294.0
74.00	7606.0
75.00	23936.0
76.00	1969.0
76.90	328.0
78.00	233.0
78.90	1707.0
79.80	652.0
80.90	1826.0
81.90	556.0
86.90	2121.0
88.00	2334.0
90.80	163.0
92.00	1272.0
93.00	2004.0
94.00	5241.0
95.00	47064.0
96.00	3217.0
96.90	125.0
103.90	214.0
106.00	255.0
115.80	169.0
117.00	359.0
117.90	144.0
119.00	254.0
127.80	250.0
128.80	119.0
129.70	164.0
135.00	119.0
140.90	520.0
143.00	760.0
144.90	321.0
154.80	141.0
171.10	134.0
171.90	764.0
173.00	536.0
173.90	38944.0
174.90	2605.0
175.90	37848.0
176.90	2150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Scan 2886 (10.619 min): VU035508.D
BFB46

m/z	Abundance
39.90	365.0
44.00	768.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46