


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
Data File : VU040943.D
Acq On : 26 Oct 2020 14:51
Operator : SY/MD
Sample : L4492-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAN8

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:11:13 PM

Quant Time: Oct 27 04:03:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 27 03:00:07 2020
Response via : Initial Calibration

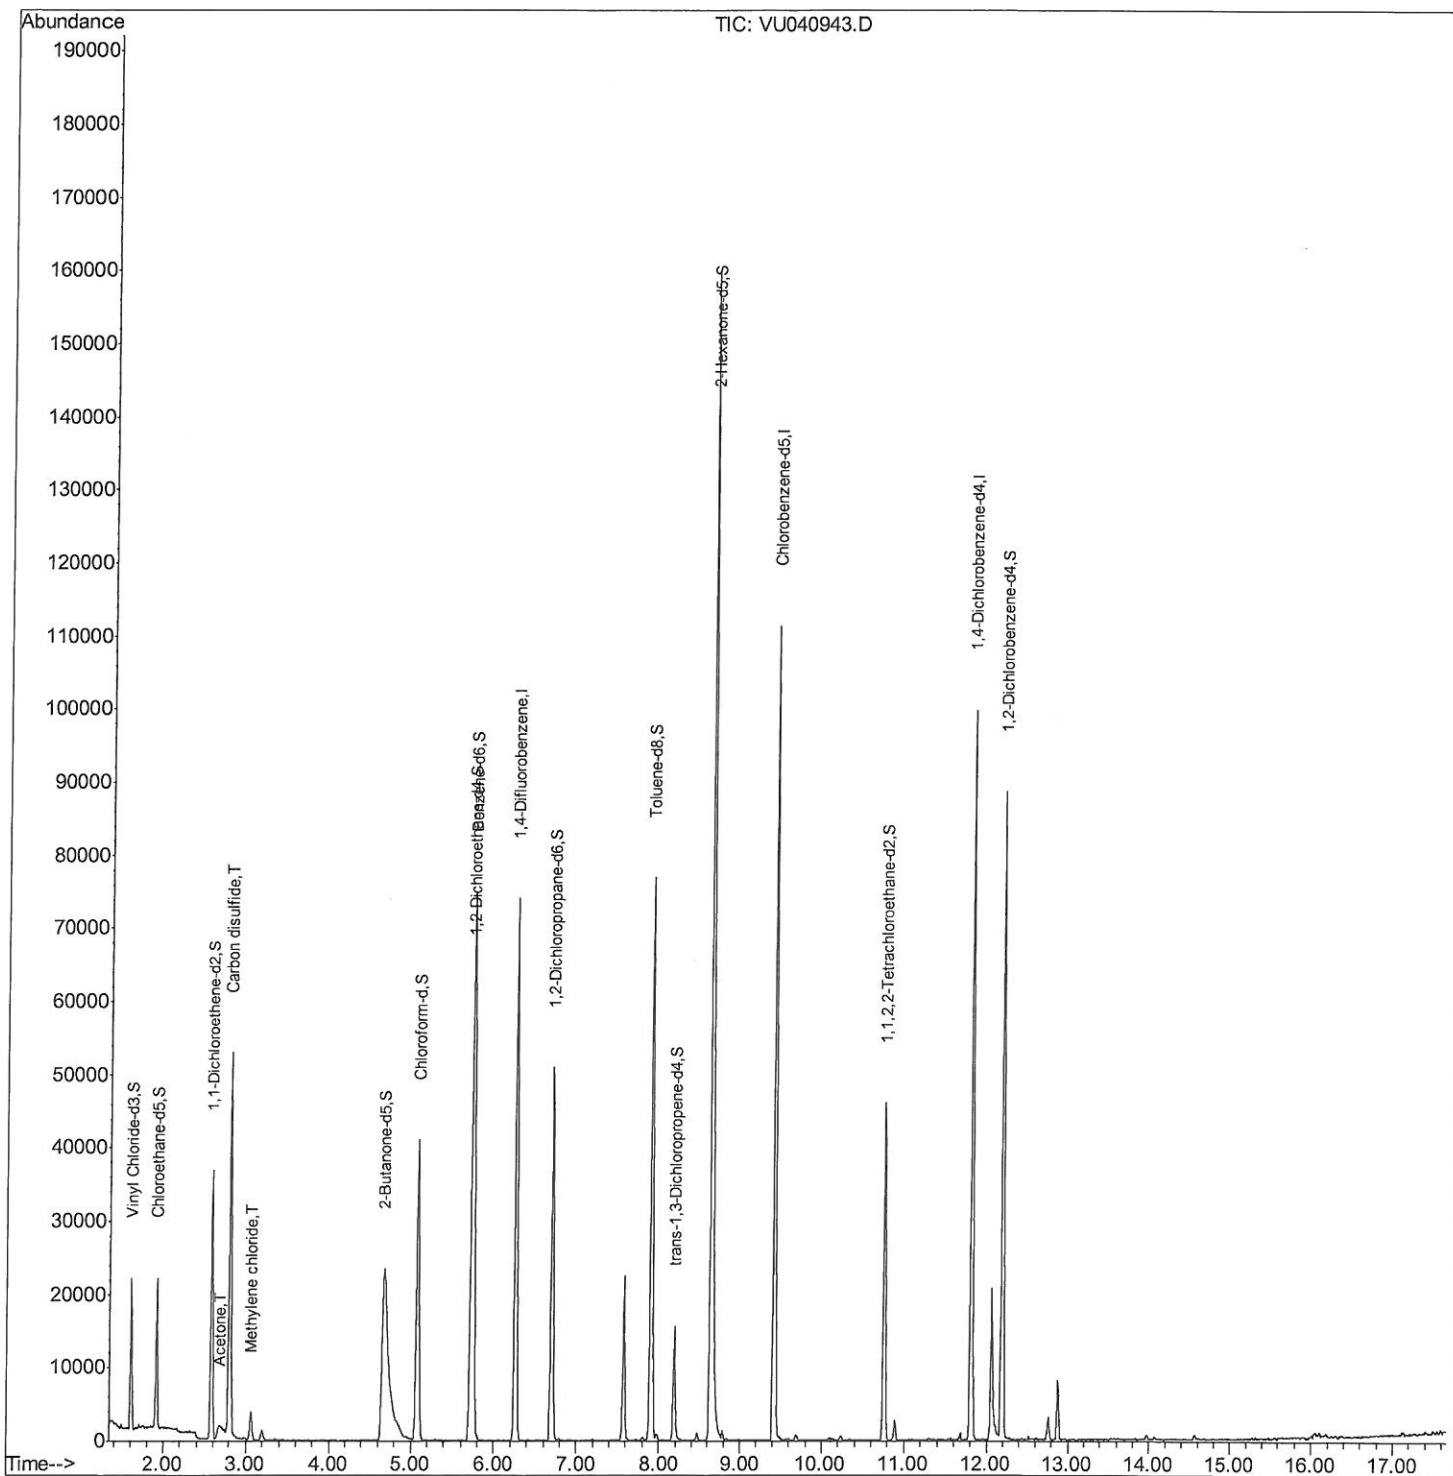

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040943.D
 Acq On : 26 Oct 2020 14:51
 Operator : SY/MD
 Sample : L4492-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0AN8

Manual Integrations
APPROVED

MMDadoda
 10/27/2020 3:11:13 PM

Quant Time: Oct 27 03:15:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 03:00:07 2020
 Response via : Initial Calibration

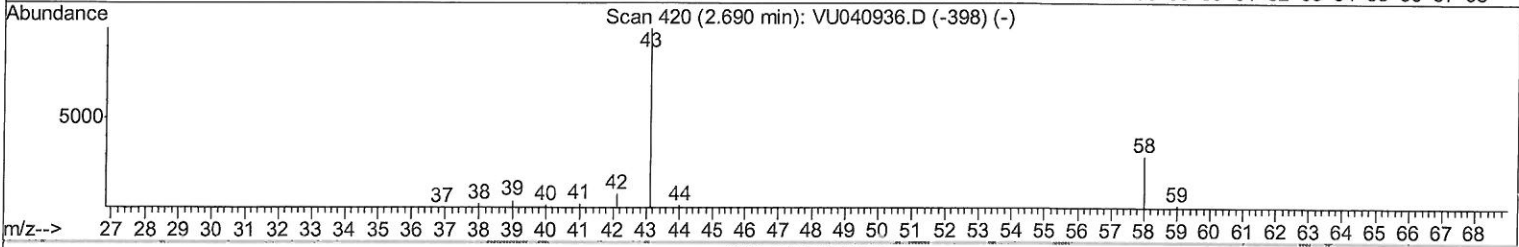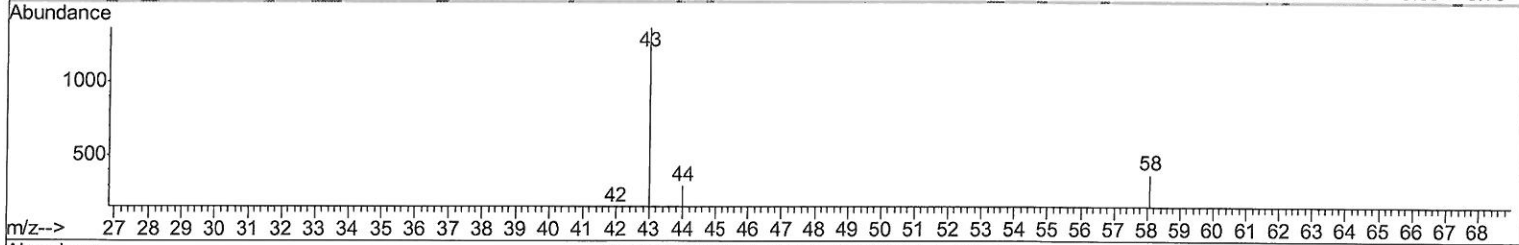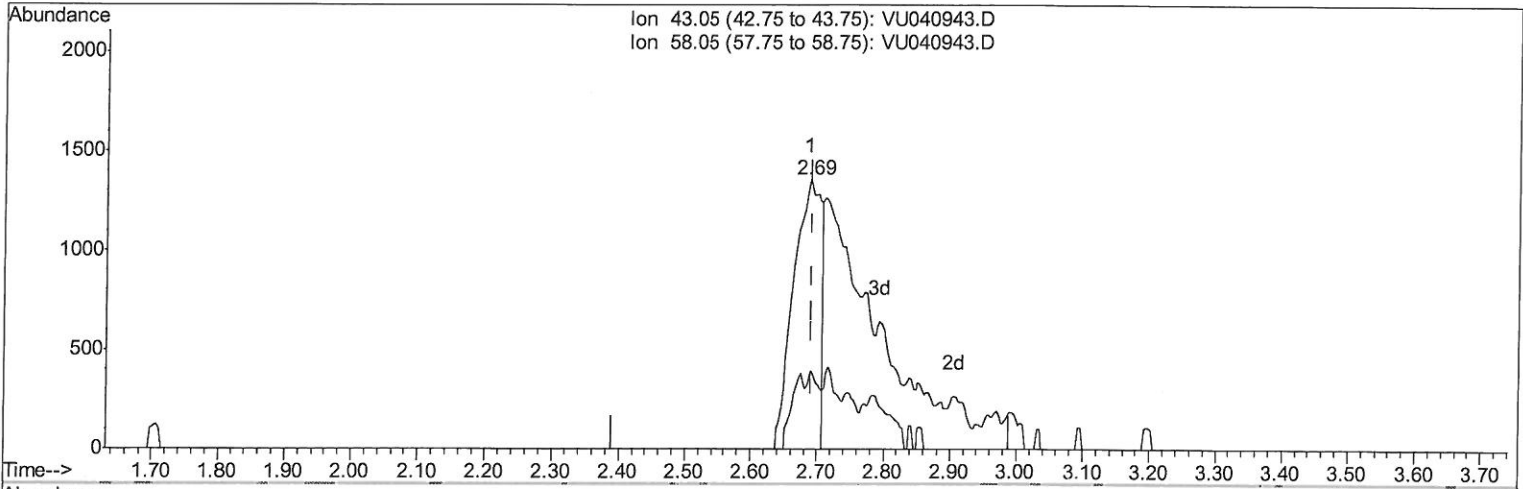

TIC: VU040943.D

(13) Acetone (T)

2.687min (-0.003) 3.75ug/L

response 3894

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	13.41
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
Data File : VU040943.D
Acq On : 26 Oct 2020 14:51
Operator : SY/MD
Sample : L4492-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAN8

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:11:13 PM

Quant Time: Oct 27 03:15:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 27 03:00:07 2020
Response via : Initial Calibration

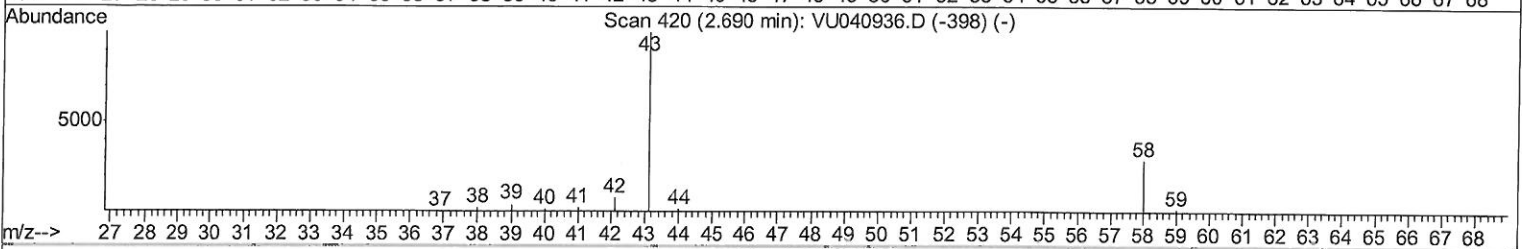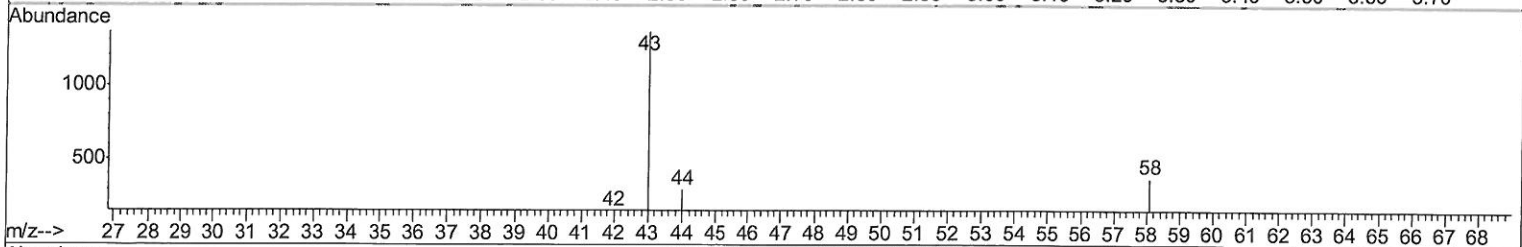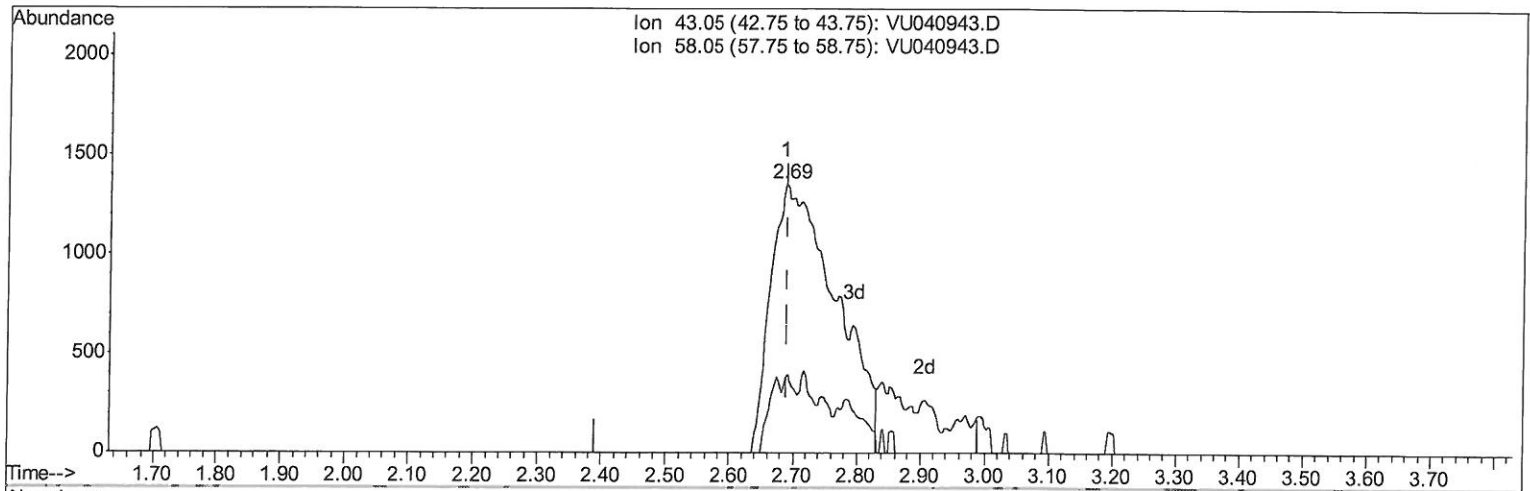

TIC: VU040943.D

(13) Acetone (T)

2.687min (-0.003) 9.22ug/L m

response 9577

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	5.45
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
10/27/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040943.D
 Acq On : 26 Oct 2020 14:51
 Operator : SY/MD
 Sample : L4492-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAN8

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:11:13 PM

Quant Time: Oct 27 04:03:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 03:00:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	54928	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	57203	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	23540	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.60	65	13776	2.98	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	59.60%		
7) Chloroethane-d5	1.92	69	13907	3.92	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	78.40%		
11) 1,1-Dichloroethene-d2	2.58	63	23411	2.59	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	51.80%#		
20) 2-Butanone-d5	4.67	46	78698	51.79	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	103.58%		
24) Chloroform-d	5.08	84	36913	4.53	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.60%		
26) 1,2-Dichloroethane-d4	5.72	65	23128	4.57	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	91.40%		
32) Benzene-d6	5.74	84	61982	4.05	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	81.00%		
36) 1,2-Dichloropropane-d6	6.70	67	22542	4.52	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	90.40%		
41) Toluene-d8	7.91	98	47034	3.39	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	67.80%#		
43) trans-1,3-Dichloropropene-	8.19	79	8645	4.00	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	80.00%		
46) 2-Hexanone-d5	8.64	63	58220	50.08	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	100.16%		
57) 1,1,2,2-Tetrachloroethane-	10.75	84	22446	4.85	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	97.00%		
64) 1,2-Dichlorobenzene-d4	12.19	152	21560	5.22	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.40%		
Target Compounds						
13) Acetone	2.69	43	9577m	9.218	ug/L	Ovalue
14) Carbon disulfide	2.81	76	65699	5.067	ug/L	99
16) Methylene chloride	3.06	84	1609	0.356	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 10/27/20