


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
Data File : VU040956.D
Acq On : 26 Oct 2020 19:53
Operator : SY/MD
Sample : L4492-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP2

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:12:12 PM

Quant Time: Oct 27 05:26:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 27 03:00:07 2020
Response via : Initial Calibration

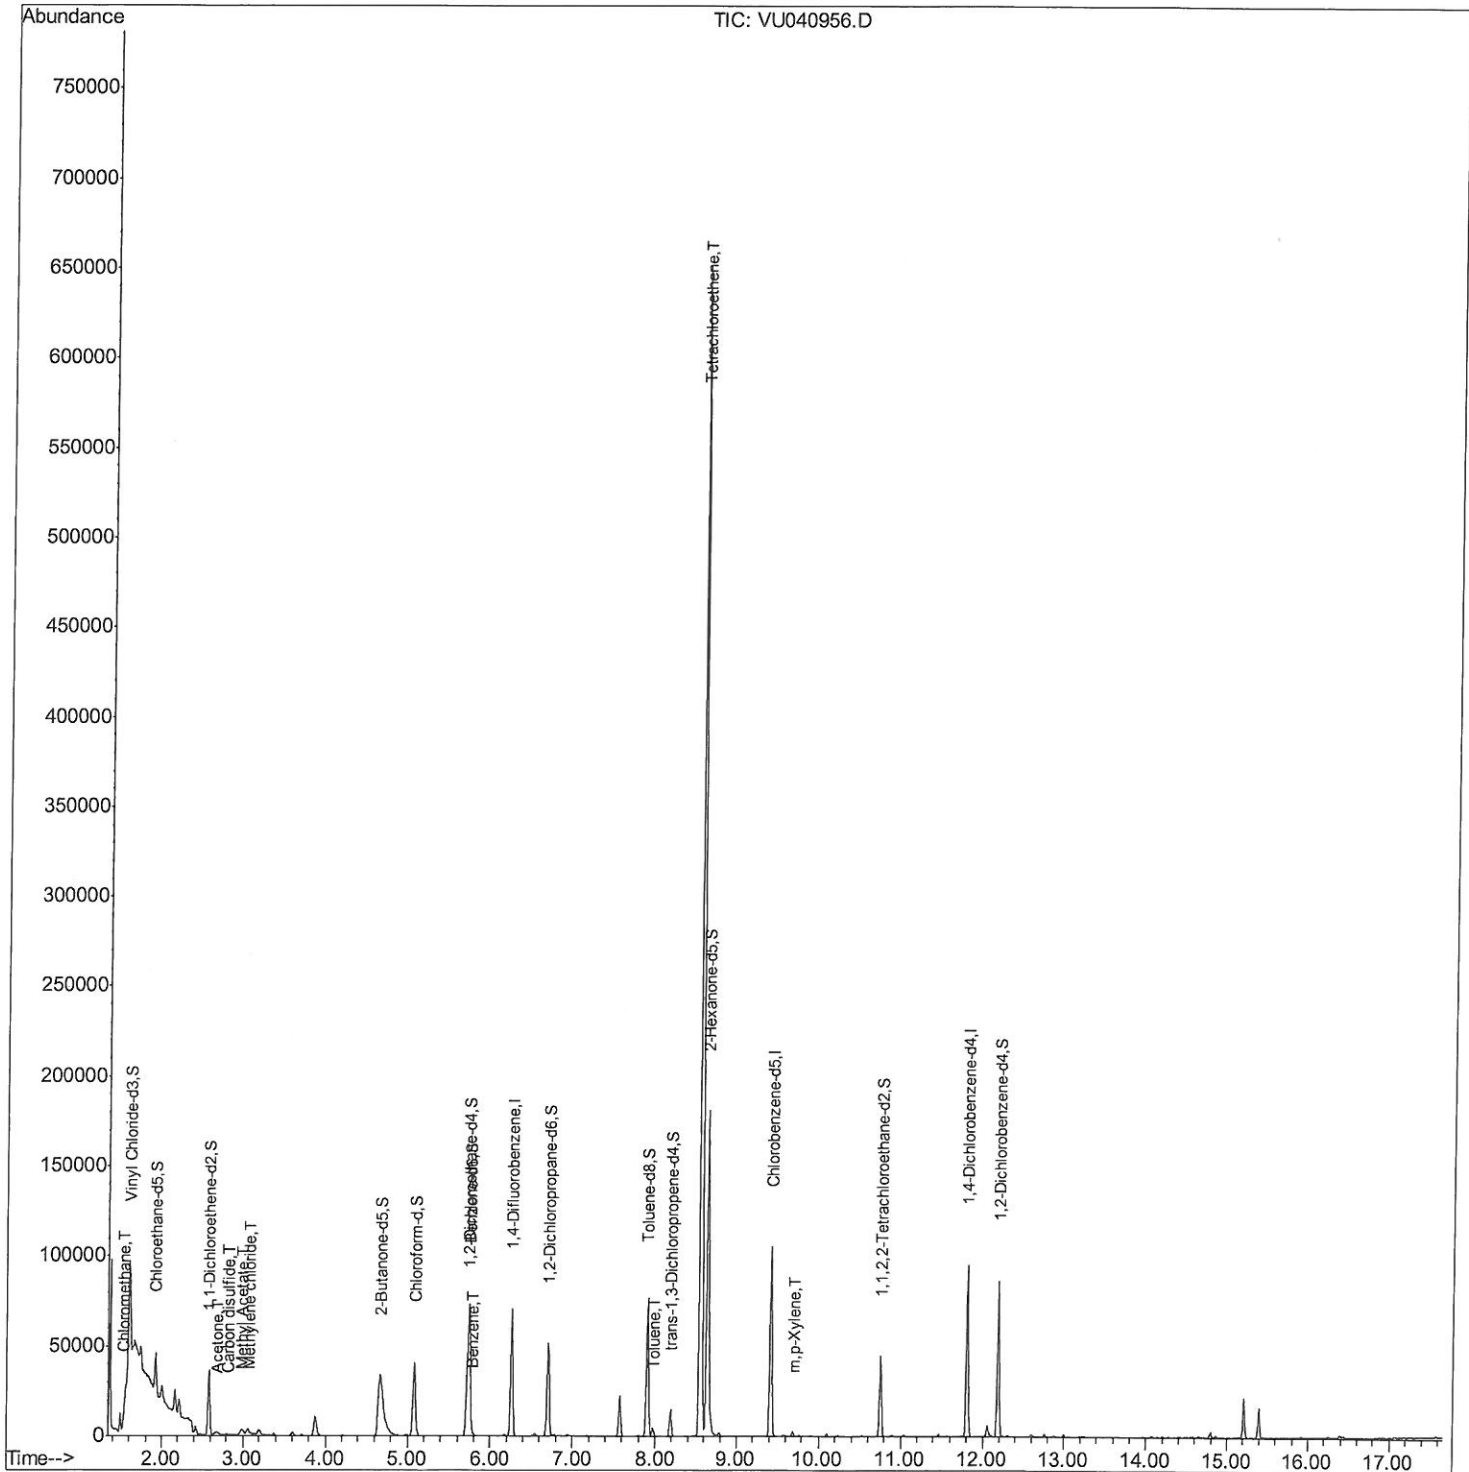

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040956.D
 Acq On : 26 Oct 2020 19:53
 Operator : SY/MD
 Sample : L4492-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0AP2

Manual Integrations
APPROVED

MMDadoda
 10/27/2020 3:12:12 PM

Quant Time: Oct 27 03:17:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 03:00:07 2020
 Response via : Initial Calibration

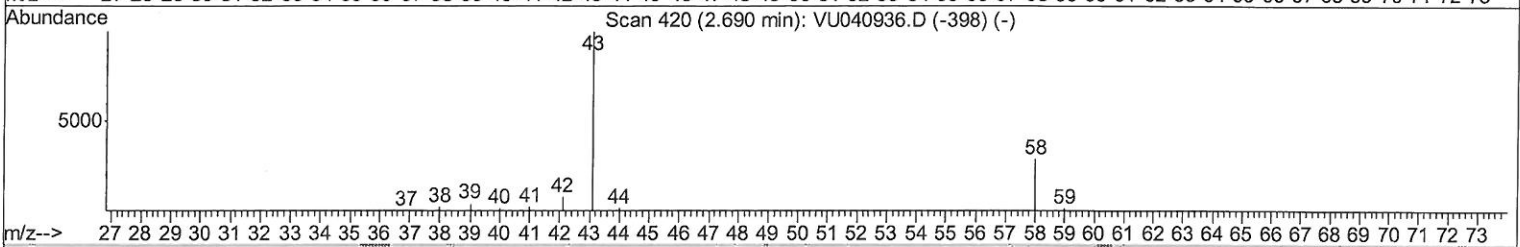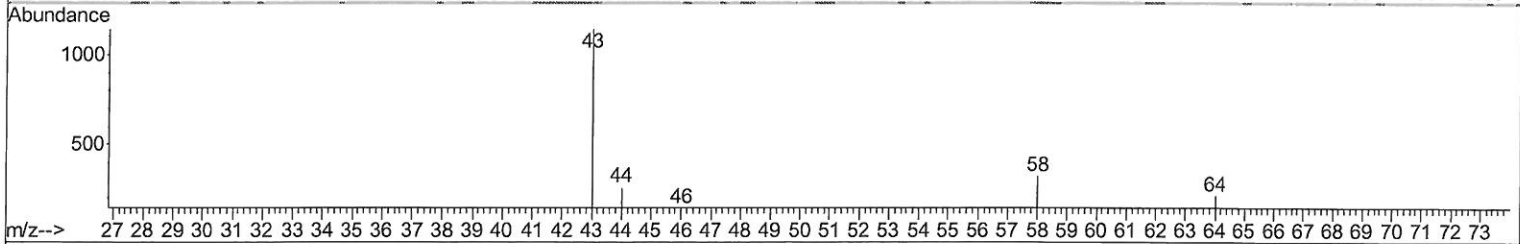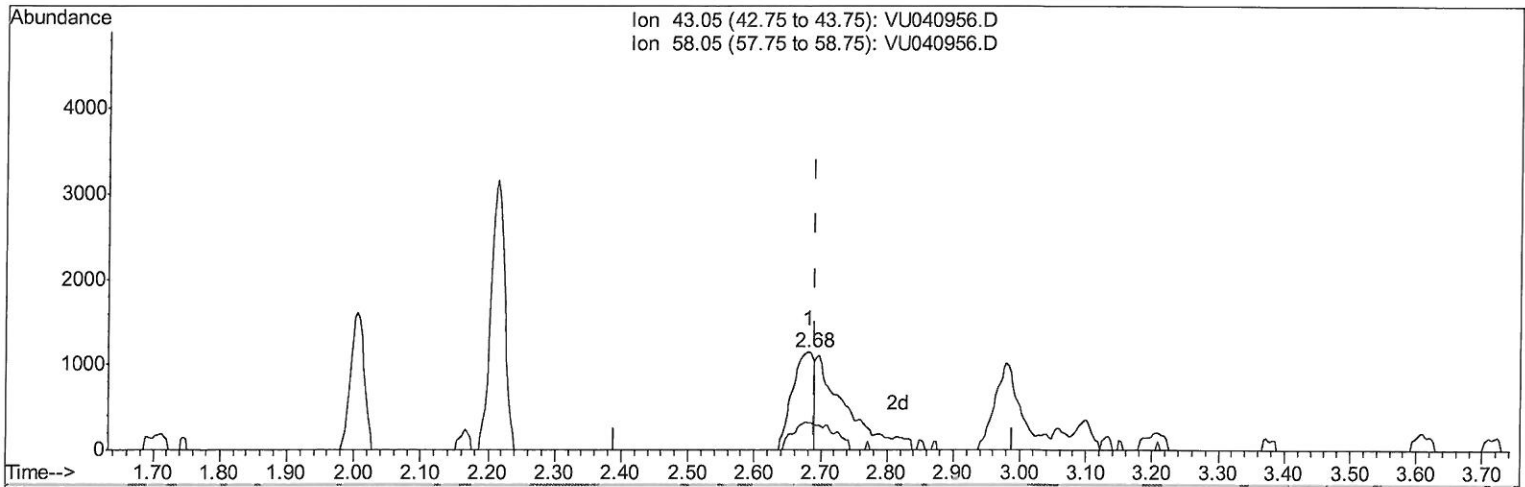

TIC: VU040956.D

(13) Acetone (T)

2.681min (-0.010) 2.65ug/L

response 2604

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	35.83#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040956.D
 Acq On : 26 Oct 2020 19:53
 Operator : SY/MD
 Sample : L4492-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0AP2

Manual Integrations
APPROVED

MMDadoda
 10/27/2020 3:12:12 PM

Quant Time: Oct 27 03:17:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 03:00:07 2020
 Response via : Initial Calibration

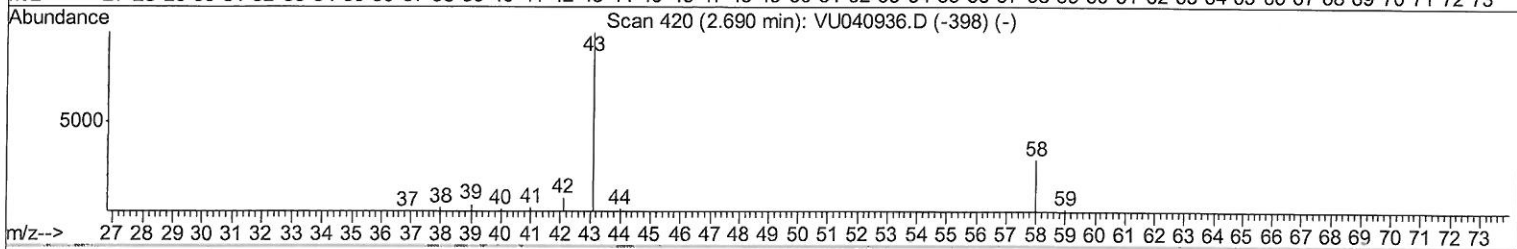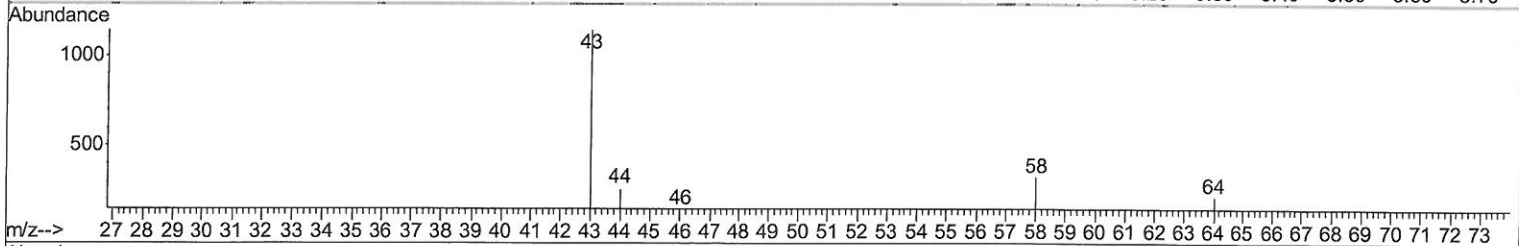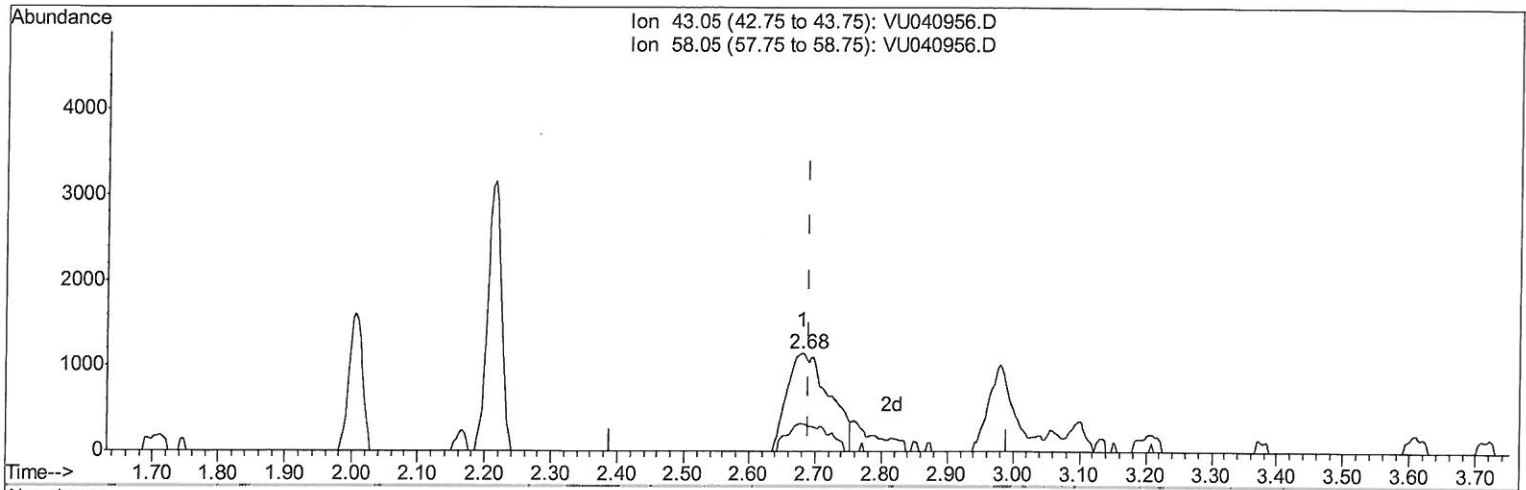

TIC: VU040956.D

(13) Acetone (T)

2.681min (-0.010) 5.17ug/L m

response 5087

Ion Exp% Act%

43.05 100 100

58.05 12.70 18.34

0.00 0.00 0.00

0.00 0.00 0.00

7 MD
10/27/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040956.D
 Acq On : 26 Oct 2020 19:53
 Operator : SY/MD
 Sample : L4492-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP2

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:12:12 PM

Quant Time: Oct 27 05:26:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 03:00:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	51981	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	54452	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	22891	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.60	65	14157	3.24	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	64.80%		
7) Chloroethane-d5	1.92	69	13582	4.05	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	81.00%		
11) 1,1-Dichloroethene-d2	2.58	63	22941	2.68	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	53.60%#		
20) 2-Butanone-d5	4.67	46	85352	59.35	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	118.70%		
24) Chloroform-d	5.08	84	36718	4.76	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.20%		
26) 1,2-Dichloroethane-d4	5.72	65	23670	4.94	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.80%		
32) Benzene-d6	5.74	84	61422	4.22	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.40%		
36) 1,2-Dichloropropane-d6	6.70	67	22445	4.73	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	94.60%		
41) Toluene-d8	7.91	98	46193	3.50	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	70.00%		
43) trans-1,3-Dichloropropene-	8.19	79	7872	3.83	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	76.60%		
46) 2-Hexanone-d5	8.64	63	60479	54.65	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	109.30%		
57) 1,1,2,2-Tetrachloroethane-	10.75	84	22174	5.04	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	100.80%		
64) 1,2-Dichlorobenzene-d4	12.19	152	20999	5.23	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.60%		
Target Compounds						
3) Chloromethane	1.53	50	1066	0.215	ug/L	87
13) Acetone	2.68	43	5087m	5.174	ug/L	96
14) Carbon disulfide	2.81	76	1745	0.142	ug/L	96
15) Methyl Acetate	2.98	43	2594	1.153	ug/L #	58
16) Methylene chloride	3.06	84	1169	0.273	ug/L	93
33) Benzene	5.79	78	1508	0.093	ug/L	100
42) Toluene	7.98	91	3404	0.206	ug/L	98
47) Tetrachloroethene	8.56	164	130952	43.011	ug/L	97
53) m,p-Xylene	9.69	106	652	0.103	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed