


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
Data File : VU040961.D
Acq On : 26 Oct 2020 23:11
Operator : SY/MD
Sample : L4492-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP5

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:12:29 PM

Quant Time: Oct 27 05:49:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 27 05:24:32 2020
Response via : Initial Calibration

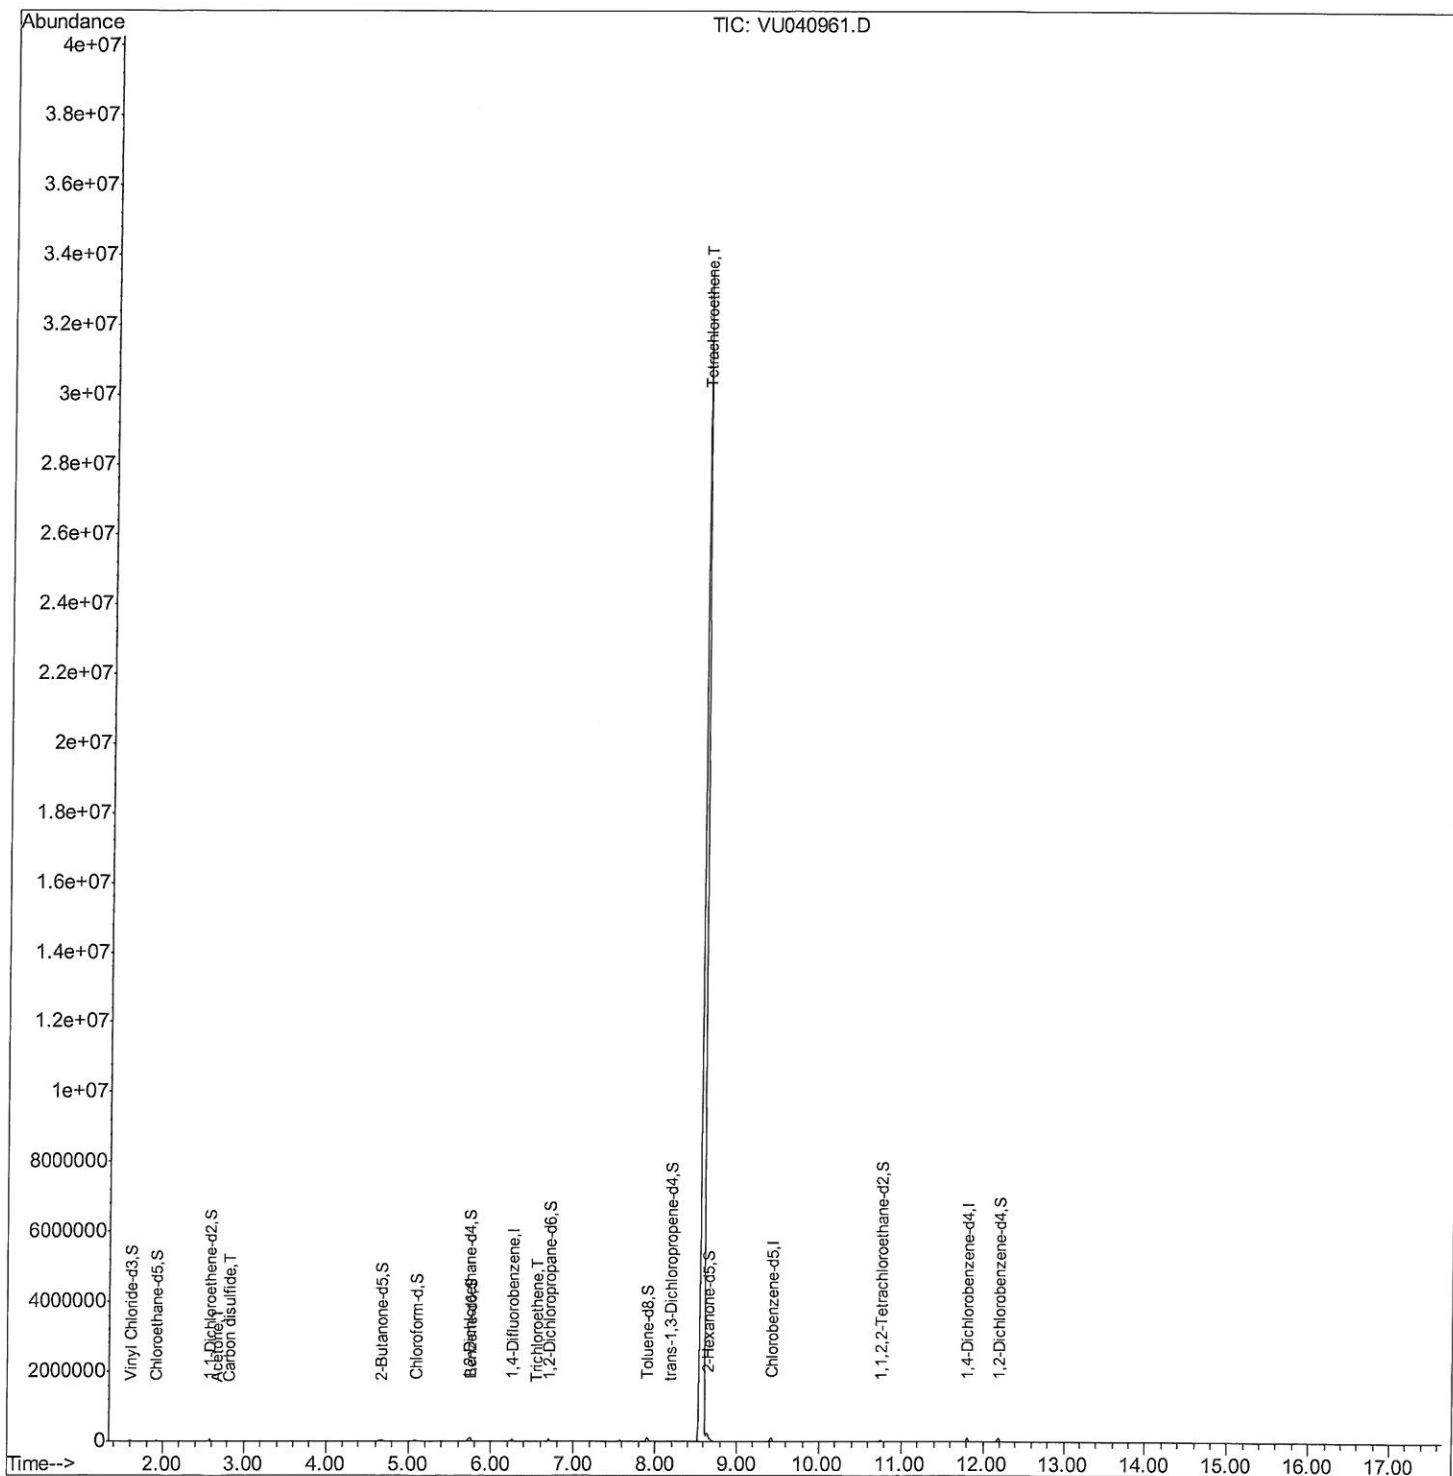

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040961.D
 Acq On : 26 Oct 2020 23:11
 Operator : SY/MD
 Sample : L4492-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP5

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:12:29 PM

Quant Time: Oct 27 05:32:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 05:24:32 2020
 Response via : Initial Calibration

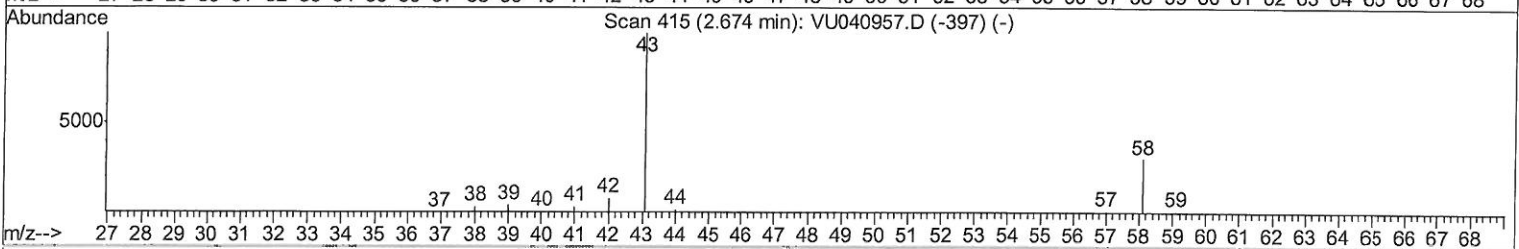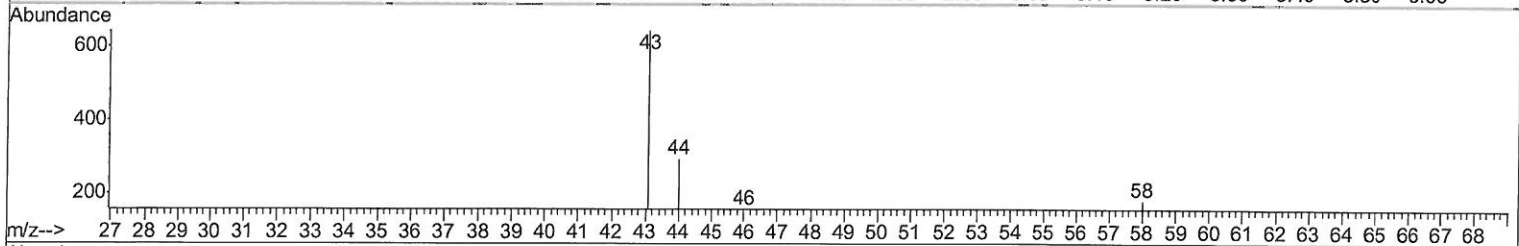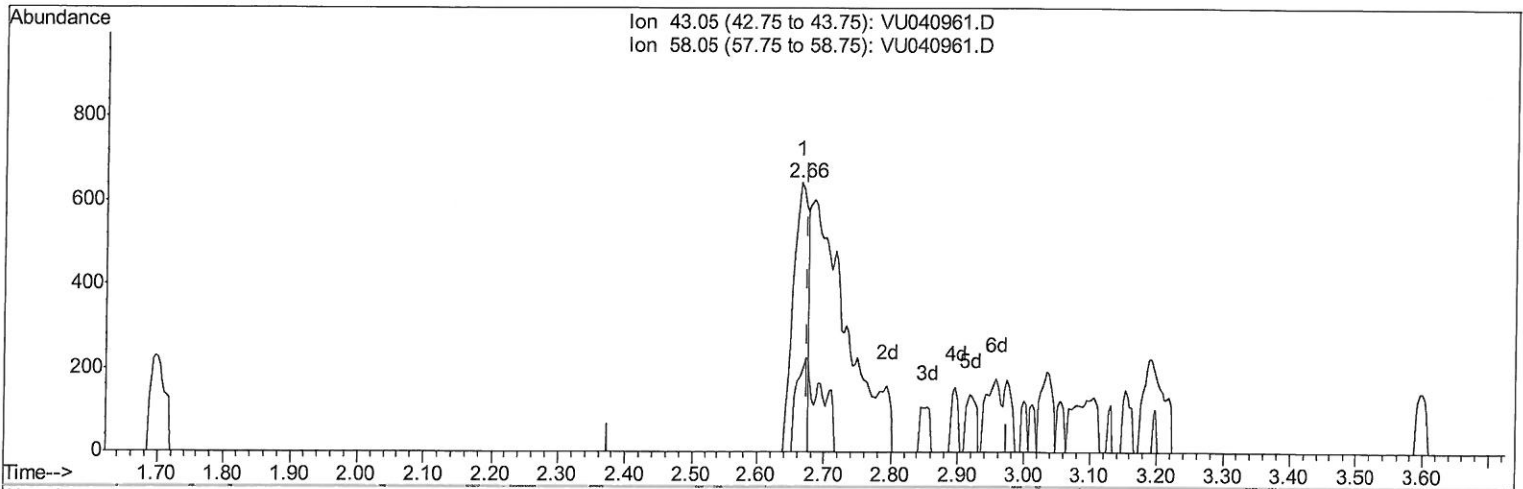

TIC: VU040961.D

(13) Acetone (T)

2.665min (-0.010) 0.85ug/L

response 966

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	34.27#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040961.D
 Acq On : 26 Oct 2020 23:11
 Operator : SY/MD
 Sample : L4492-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP5

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:12:29 PM

Quant Time: Oct 27 05:32:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 05:24:32 2020
 Response via : Initial Calibration

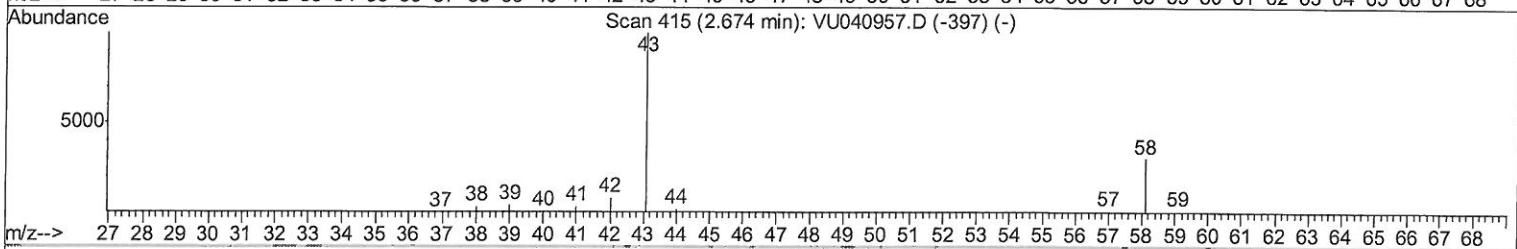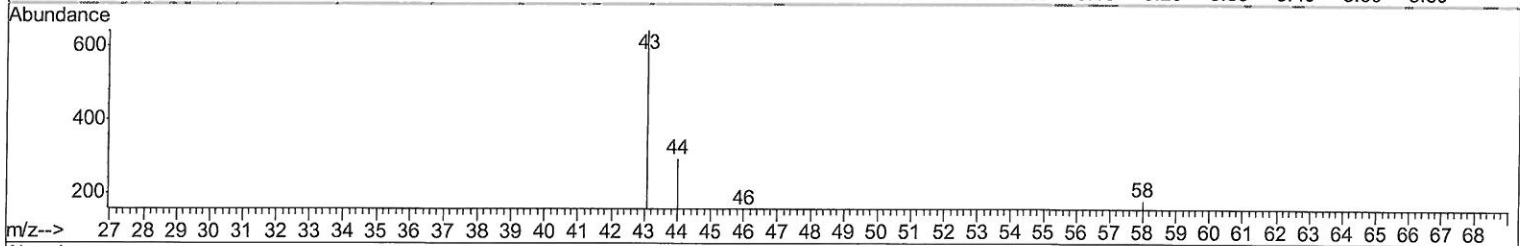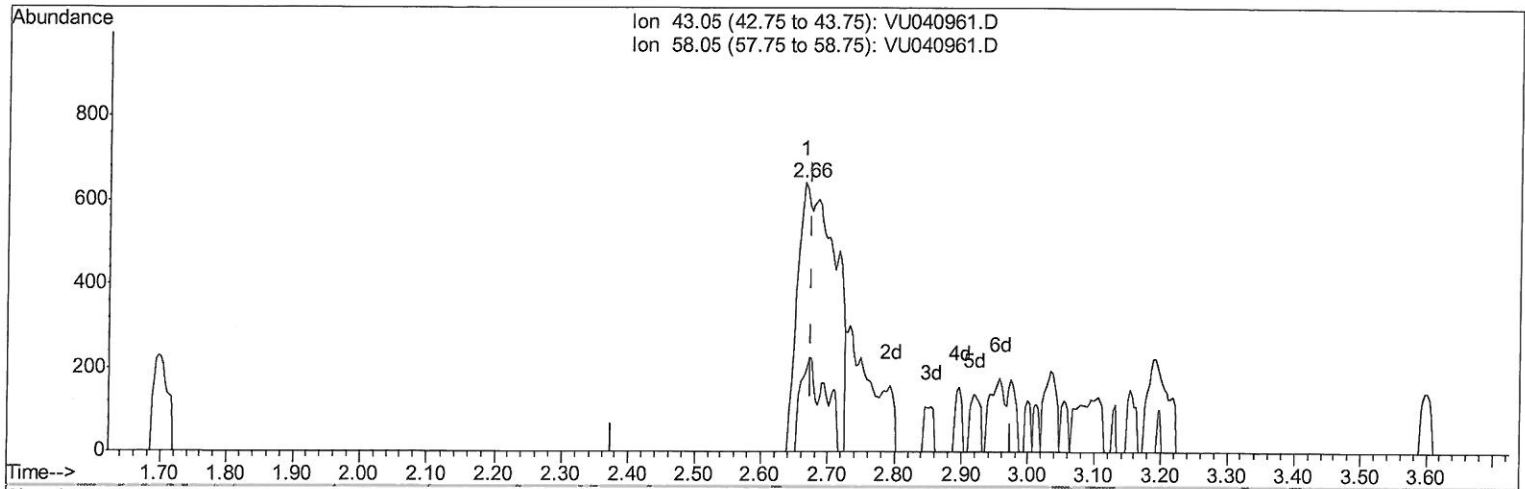

(13) Acetone (T)

2.665min (-0.010) 2.19ug/L m

response 2492

MD
10/27/20

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	13.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102620\
 Data File : VU040961.D
 Acq On : 26 Oct 2020 23:11
 Operator : SY/MD
 Sample : L4492-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP5

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:12:29 PM

Quant Time: Oct 27 05:49:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 27 05:24:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	60257	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	62476	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	24969	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	24224	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.92	69	19524	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.58	63	35945	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	4.67	46	82915	49.74	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.48%
24) Chloroform-d	5.08	84	42798	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.72	65	27230	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.74	84	77953	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.70	67	26548	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.91	98	62615	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	8.19	79	10437	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	8.64	63	65081	51.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.52%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	22872	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	23680	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%

Target Compounds

					Ovalue	
13) Acetone	2.66	43	2492m	2.186	ug/L	98
14) Carbon disulfide	2.81	76	2137	0.150	ug/L	97
34) Trichloroethene	6.56	95	2945	0.620	ug/L	90
47) Tetrachloroethene	8.58	164	7533965	2156.684	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 mD
 10/27/20