


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102620\
Data File : VU040933.D
Acq On : 26 Oct 2020 10:18
Operator : SY/MD
Sample : BFB27
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB27

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 27 05:24:32 2020

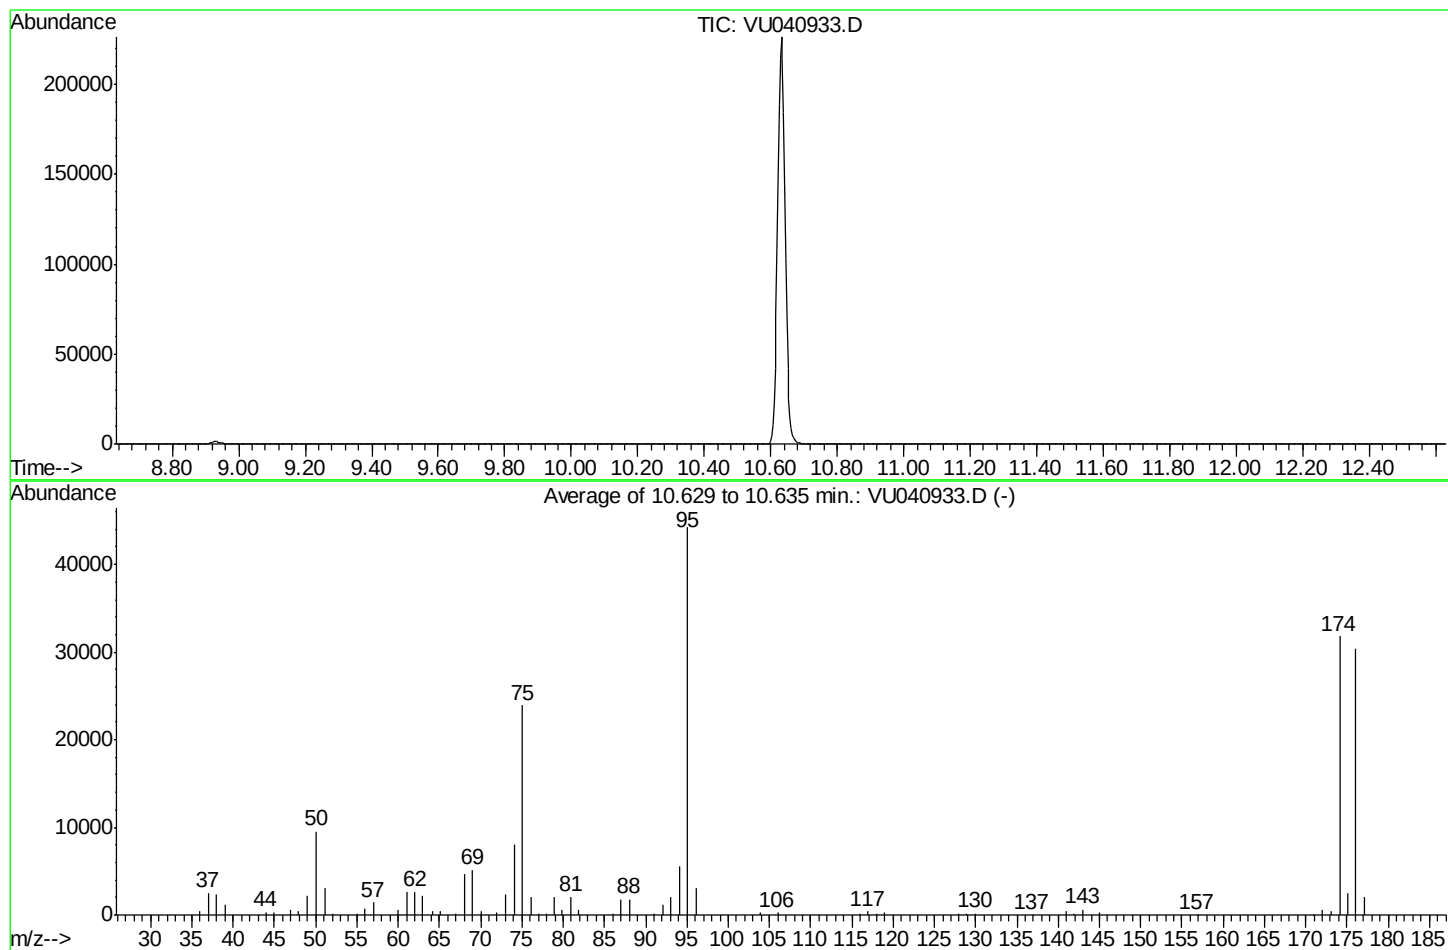

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	9517	PASS
75	95	30	80	54.0	23882	PASS
95	95	100	100	100.0	44229	PASS
96	95	5	9	6.9	3057	PASS
173	174	0.00	2	1.6	500	PASS
174	95	50	120	71.9	31821	PASS
175	174	5	9	7.9	2514	PASS
176	174	95	101	95.3	30338	PASS
177	176	5	9	6.7	2024	PASS

m/z	Abundance
35.00	422.0
37.00	2571.0
38.00	2402.0
39.00	1090.0
44.00	442.0
45.00	339.0
47.00	574.0
47.90	353.0
49.00	2248.0
50.10	9428.0
51.10	3238.0
52.10	137.0
55.00	142.0
56.00	807.0
57.00	1448.0
60.00	562.0
61.00	2671.0
62.10	2674.0
63.00	2161.0
64.10	421.0
65.00	519.0
66.90	156.0
68.00	4704.0
69.00	5173.0
70.00	377.0
72.00	311.0
73.00	2390.0
74.10	8105.0
75.10	23968.0
76.10	2146.0
77.10	212.0
78.00	180.0
78.90	1983.0
79.90	608.0
81.00	2150.0
81.90	547.0
86.10	127.0
87.00	1723.0
88.00	1715.0
91.00	212.0
92.10	1243.0
93.10	2104.0
94.10	5506.0
95.10	43648.0
96.10	3187.0
103.90	188.0
106.00	226.0
116.00	195.0
116.90	457.0
118.00	198.0
119.00	325.0
127.90	150.0
128.90	148.0
130.00	185.0
141.00	501.0
143.00	682.0
145.00	257.0
170.90	111.0
172.10	680.0
173.10	521.0
174.10	30880.0
175.10	2477.0
176.10	29304.0
177.10	1993.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	455.0
37.00	2611.0
38.00	2401.0
39.00	1204.0
44.10	514.0
44.90	333.0
47.00	600.0
48.00	398.0
49.00	2319.0
50.10	9941.0
51.10	3200.0
52.10	140.0
55.00	162.0
56.00	814.0
57.00	1442.0
60.00	561.0
61.00	2769.0
62.10	2778.0
63.00	2324.0
64.10	398.0
65.00	513.0
67.00	164.0
68.00	4872.0
69.10	5311.0
70.00	391.0
72.00	351.0
73.00	2477.0
74.10	8283.0
75.10	24584.0
76.10	2114.0
77.10	206.0
78.00	190.0
78.90	2085.0
79.90	588.0
81.00	2198.0
81.90	565.0
86.10	113.0
87.00	1857.0
88.00	1887.0
91.00	235.0
92.10	1273.0
93.10	2173.0
94.10	5762.0
95.10	45752.0
96.10	3194.0
103.90	249.0
106.00	279.0
116.00	191.0
116.90	444.0
118.00	187.0
118.90	382.0
127.90	168.0
128.80	112.0
130.00	197.0
136.90	101.0
141.00	525.0
141.90	123.0
143.00	658.0
145.00	248.0
156.90	103.0
172.10	641.0
173.10	511.0
174.10	32808.0
175.10	2629.0
176.10	31232.0
177.00	2100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	472.0
37.00	2489.0
38.00	2231.0
39.00	1175.0
44.10	532.0
44.90	342.0
47.00	564.0
48.00	375.0
49.00	2155.0
50.10	9184.0
51.10	2815.0
52.00	126.0
55.00	135.0
56.00	753.0
57.00	1327.0
60.00	503.0
61.00	2535.0
62.00	2579.0
63.00	2243.0
64.10	366.0
65.10	508.0
67.00	162.0
68.10	4594.0
69.10	4997.0
70.00	396.0
72.00	333.0
73.00	2274.0
74.10	7792.0
75.10	23096.0
76.10	1928.0
77.10	199.0
78.00	199.0
78.90	2057.0
79.90	535.0
81.00	2021.0
81.90	531.0
87.00	1771.0
88.10	1782.0
91.00	211.0
92.00	1206.0
93.10	2086.0
94.10	5611.0
95.10	43288.0
96.10	2790.0
103.90	267.0
106.00	298.0
116.00	173.0
117.00	370.0
117.90	154.0
118.90	372.0
127.90	171.0
130.00	176.0
141.00	515.0
141.90	138.0
143.00	573.0
145.00	252.0
172.00	606.0
173.10	470.0
174.10	31776.0
175.10	2437.0
176.10	30480.0
177.00	1981.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
44.00	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27