

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051532.D
 Acq On : 27 Oct 2022 04:13
 Operator : JC/MD
 Sample : N5300-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA80

Quant Time: Oct 27 08:27:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 27 08:11:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	309529	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	306794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	162745	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	119509	4.787	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.800%	
7) Chloroethane-d5	1.909	69	105490	4.917	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.400%	
11) 1,1-Dichloroethene-d2	2.562	65	44732	4.532	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	90.600%	
20) 2-Butanone-d5	4.642	46	317178	57.699	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.400%	
24) Chloroform-d	5.060	84	200720	4.312	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.200%	
26) 1,2-Dichloroethane-d4	5.703	65	104877	4.369	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
32) Benzene-d6	5.729	84	441201	5.228	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.600%	
36) 1,2-Dichloropropane-d6	6.690	67	142291	4.964	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.200%	
41) Toluene-d8	7.899	98	407838	5.401	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.000%	
43) trans-1,3-Dichloroprop...	8.179	79	43040	4.570	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.400%	
46) 2-Hexanone-d5	8.635	63	289720	91.285	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	182.560%#	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	133783	5.843	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	116.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	144737	5.117	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.400%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.600	62	3629	0.104	ug/L #	1
8) Chloroethane	1.932	64	204976	9.243	ug/L	87
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	1221	0.051	ug/L #	24
13) Acetone	2.668	43	25164	6.103	ug/L	86
14) Carbon disulfide	2.787	76	10449	0.151	ug/L #	95
15) Methyl Acetate	3.038	43	18436	1.839	ug/L #	51
17) Methyl tert-butyl Ether	3.362	73	7958	0.154	ug/L #	1
18) trans-1,2-Dichloroethene	3.350	96	32250	1.358	ug/L	93
19) 1,1-Dichloroethane	3.867	63	32778	0.669	ug/L	95
21) 2-Butanone	4.729	43	17107	2.633	ug/L	95
27) 1,2-Dichloroethane	5.777	62	464297	15.143	ug/L #	74
30) Cyclohexane	5.385	56	448335	14.380	ug/L	100
35) Methylcyclohexane	6.761	83	401264	12.448	ug/L	98
37) 1,2-Dichloropropane	6.758	63	5155	0.184	ug/L #	1
38) Bromodichloromethane	7.156	83	25976	0.776	ug/L #	35
40) 4-Methyl-2-pentanone	7.713	43	26810	1.820	ug/L #	45
44) trans-1,3-Dichloropropene	7.980	75	564939	19.362	ug/L #	1
45) 1,1,2-Trichloroethane	8.369	97	14848	0.753	ug/L #	22
48) 2-Hexanone	8.684	43	43986	4.011	ug/L #	56

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051532.D
 Acq On : 27 Oct 2022 04:13
 Operator : JC/MD
 Sample : N5300-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA80

Quant Time: Oct 27 08:27:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 27 08:11:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


53) m,p-Xylene	9.697	106	10829233	285.806	ug/L #	49
54) o-Xylene	10.102	106	6129013	170.957	ug/L	95
55) Styrene	10.102	104	325009	5.266	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.716	83	56124	2.300	ug/L #	28
60) Isopropylbenzene	10.484	105	5541011	53.755	ug/L	98
62) 1,3,5-Trimethylbenzene	11.086	105	644993	23.588	ug/L	98
63) 1,2,4-Trimethylbenzene	11.468	105	8227384	106.390	ug/L	99
64) 1,3-Dichlorobenzene	11.745	146	328267	6.438	ug/L	98
65) 1,4-Dichlorobenzene	11.835	146	2061528	41.020	ug/L	98
67) 1,2-Dichlorobenzene	12.211	146	1040618	20.994	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.970	75	7147	1.818	ug/L #	5
69) 1,3,5-Trichlorobenzene	13.220	180	3550	0.101	ug/L #	79
71) Naphthalene	14.082	128	822825	17.722	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051532.D
Acq On : 27 Oct 2022 04:13
Operator : JC/MD
Sample : N5300-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA80

Quant Time: Oct 27 08:27:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 27 08:11:03 2022
Response via : Initial Calibration




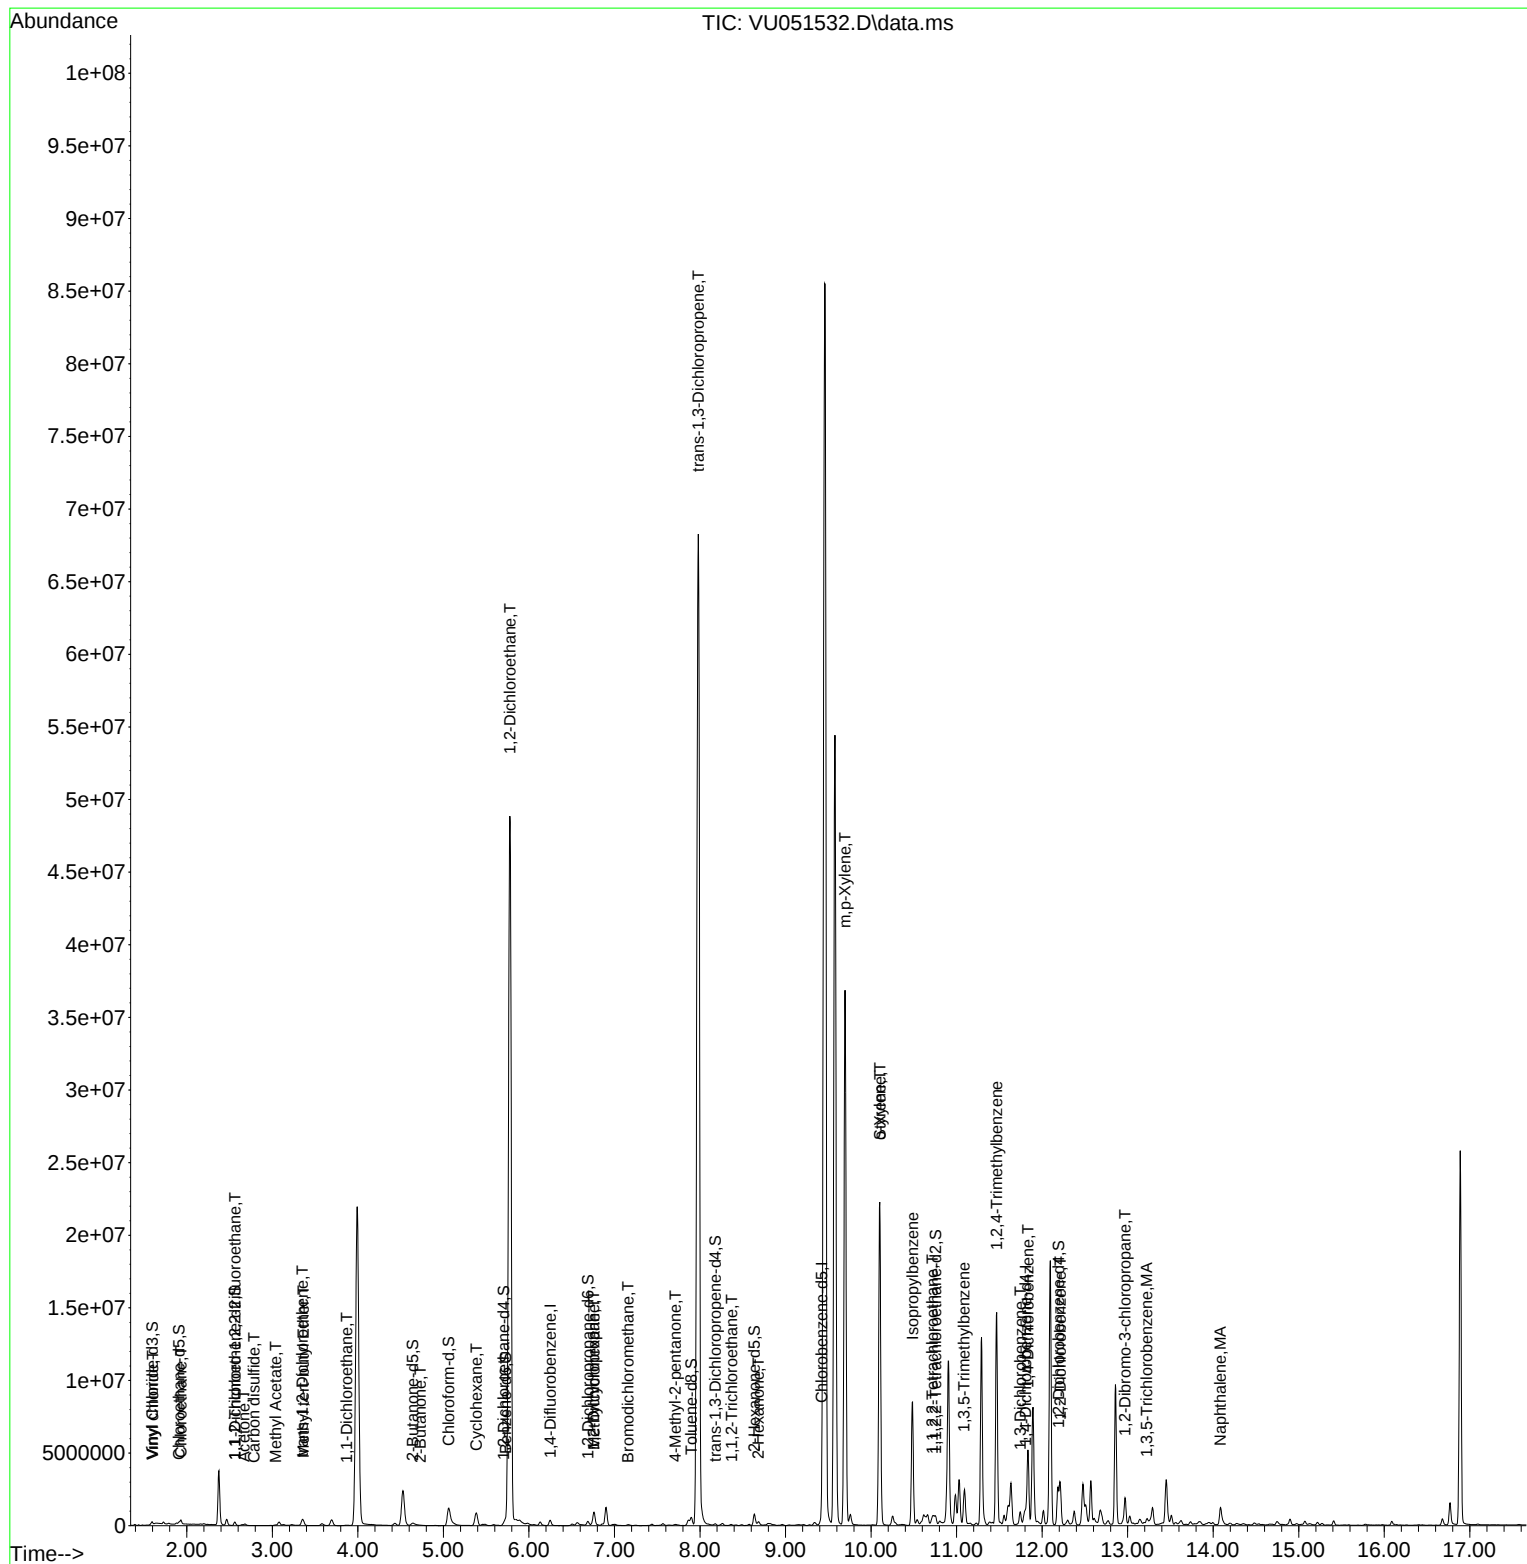




#5
 Vinyl chloride
 Concen: 0.104 ug/L
 RT: 1.600 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU051532.D
 Acq: 27 Oct 2022 04:13




Instrument :
 MSVOA_U
 ClientSampleId :
 BHA80


Tgt Ion: 62 Resp: 3629
 Ion Ratio Lower Upper
 62 100
 64 2356.2 24.0 44.6#

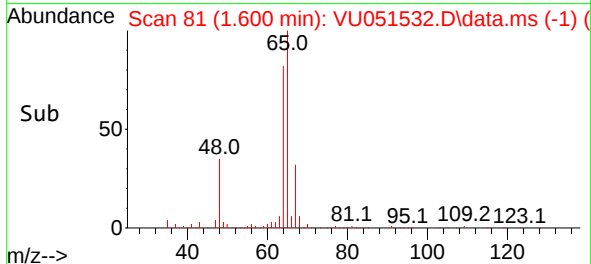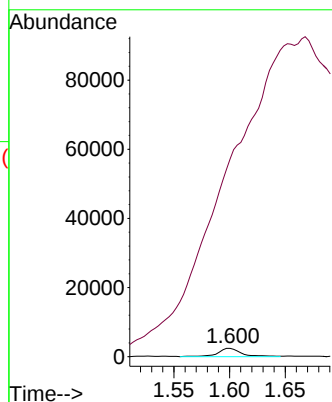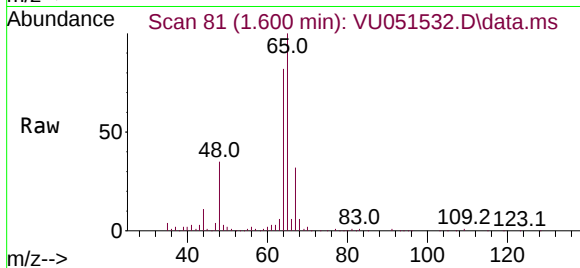

#8
 Chloroethane
 Concen: 9.243 ug/L
 RT: 1.932 min Scan# 184
 Delta R.T. 0.003 min
 Lab File: VU051532.D
 Acq: 27 Oct 2022 04:13

Tgt Ion: 64 Resp: 204976
 Ion Ratio Lower Upper
 64 100
 66 24.5 22.3 41.3


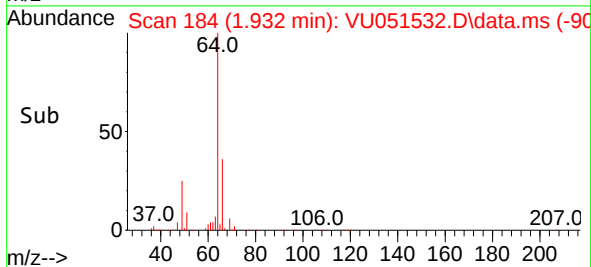
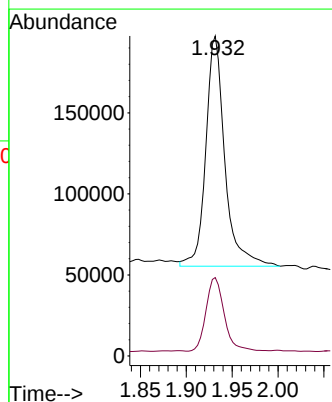
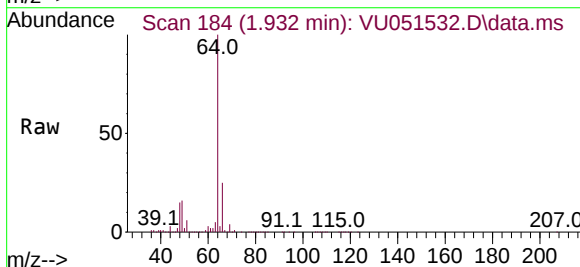




#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.051 ug/L
RT: 2.565 min Scan# 384
Delta R.T. -0.010 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:101 Resp: 1221
Ion Ratio Lower Upper
101 100
85 3.8 34.6 51.8#
151 0.0 56.5 84.7#

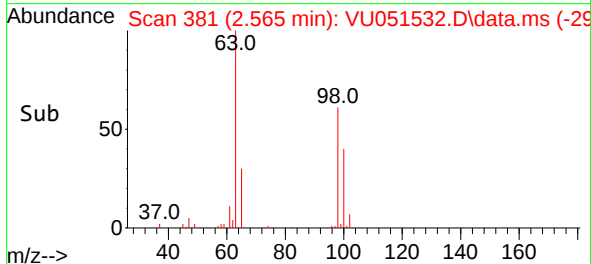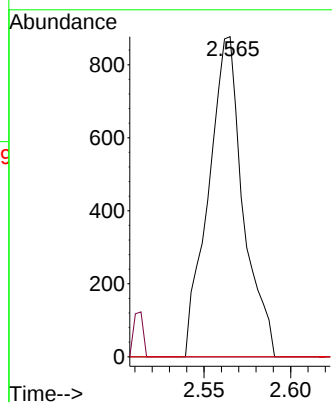

#13
Acetone
Concen: 6.103 ug/L
RT: 2.668 min Scan# 413
Delta R.T. 0.045 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 43 Resp: 25164
Ion Ratio Lower Upper
43 100
58 26.4 0.0 68.8


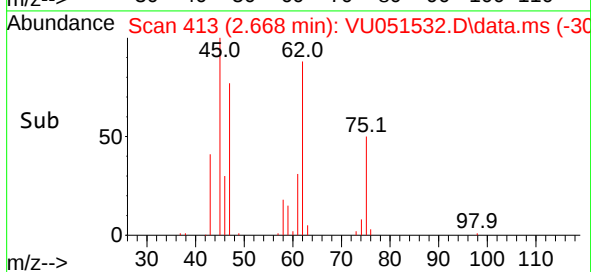
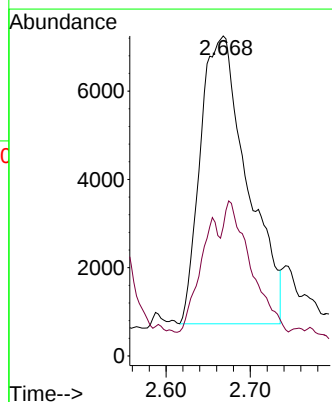





#14
Carbon disulfide
Concen: 0.151 ug/L
RT: 2.787 min Scan# 411
Delta R.T. -0.003 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 76 Resp: 10449
Ion Ratio Lower Upper
76 100
78 10.7 7.0 10.4#

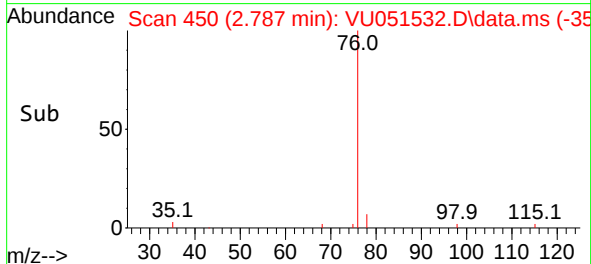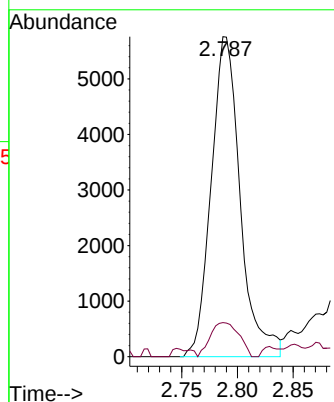

#15
Methyl Acetate
Concen: 1.839 ug/L
RT: 3.038 min Scan# 528
Delta R.T. 0.090 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 43 Resp: 18436
Ion Ratio Lower Upper
43 100
74 0.3 20.0 30.0#

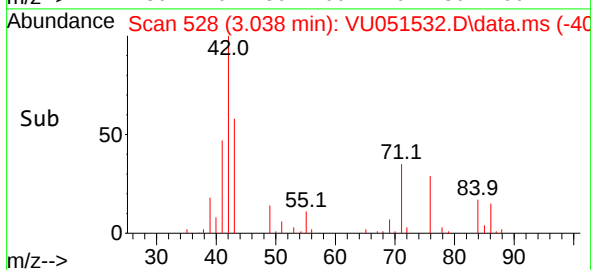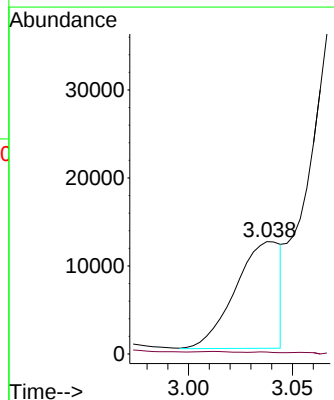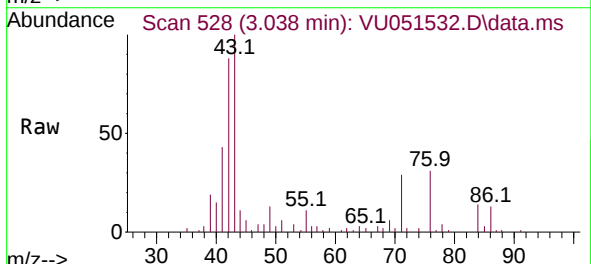



#17

Methyl tert-butyl Ether

Concen: 0.154 ug/L

RT: 3.362 min Scan# 61

Delta R.T. -0.000 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13

Instrument :

MSVOA_U

ClientSampleId :

BHA80





Tgt Ion: 73 Resp: 7958

Ion Ratio Lower Upper

73 100

43 680.8 15.4 23.0#

57 3084.4 18.9 28.3#

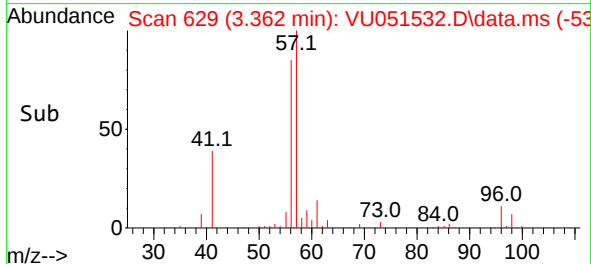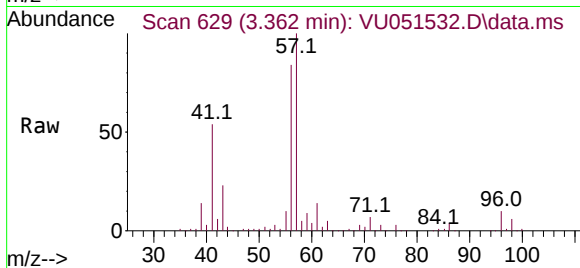

#18

trans-1,2-Dichloroethene

Concen: 1.358 ug/L

RT: 3.350 min Scan# 625

Delta R.T. -0.000 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13




Tgt Ion: 96 Resp: 32250


Ion Ratio Lower Upper

96 100

61 133.9 101.4 188.2

98 61.5 44.9 83.5


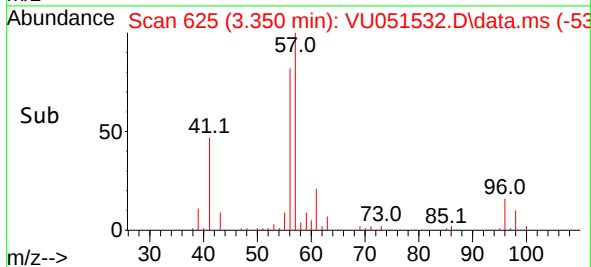

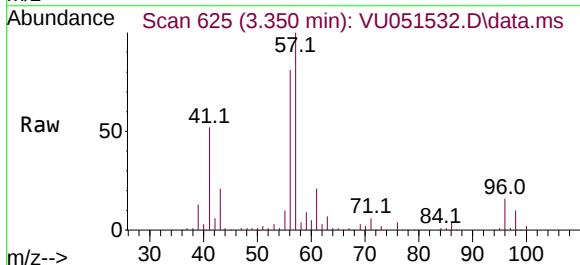




#19
1,1-Dichloroethane
Concen: 0.669 ug/L
RT: 3.867 min Scan# 71
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:	63	Resp:	32778
Ion	Ratio	Lower	Upper
63	100		
65	34.8	22.0	41.0
83	11.8	9.0	16.6

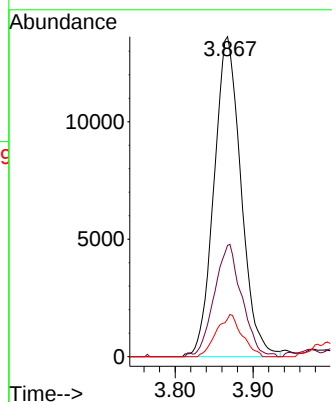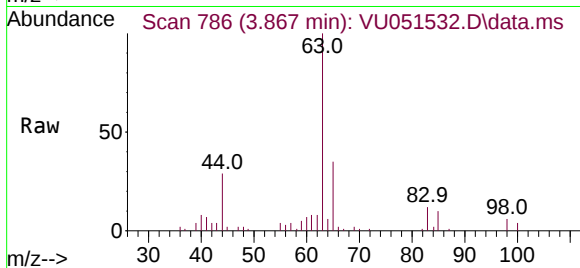

#21
2-Butanone
Concen: 2.633 ug/L
RT: 4.729 min Scan# 1054
Delta R.T. 0.032 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion:	43	Resp:	17107
Ion	Ratio	Lower	Upper
43	100		
72	24.9	13.8	41.4


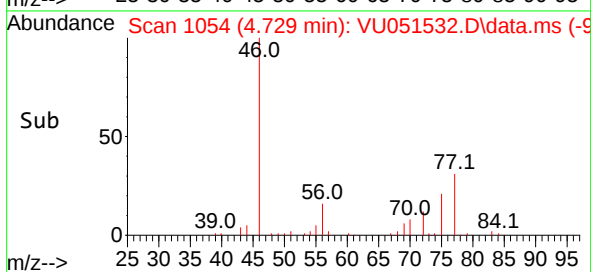
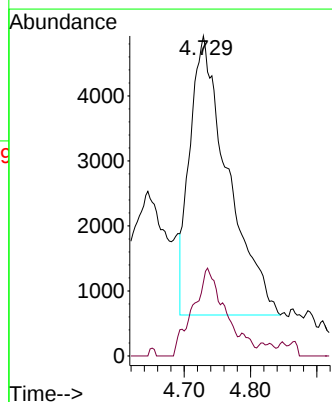
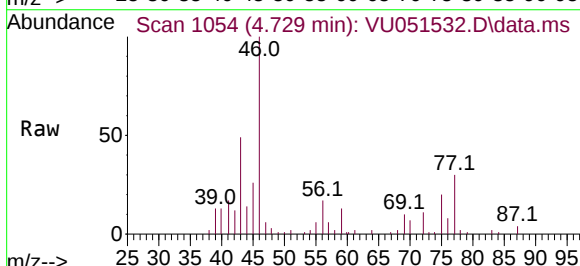


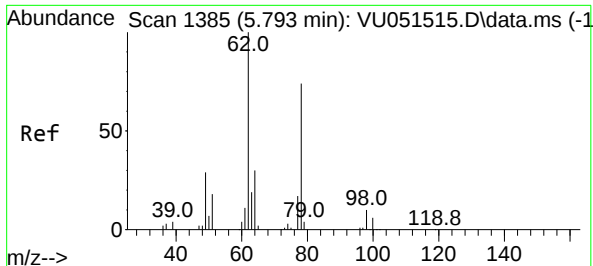

#27
1,2-Dichloroethane
Concen: 15.143 ug/L
RT: 5.777 min Scan# 11
Delta R.T. -0.016 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 62 Resp: 464297
Ion Ratio Lower Upper
62 100
98 0.1 7.7 11.5#

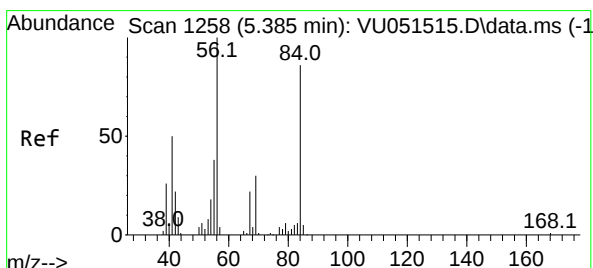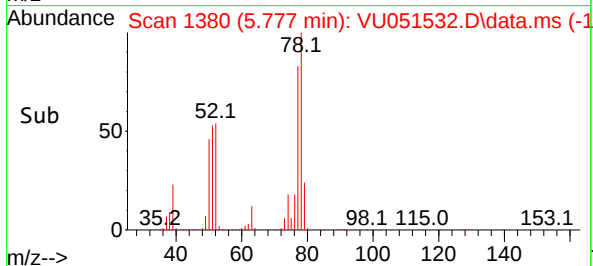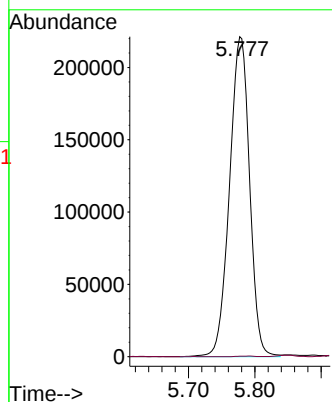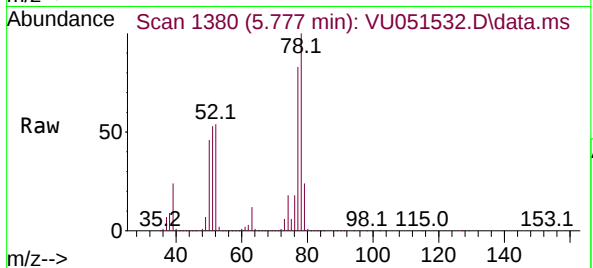

#30
Cyclohexane
Concen: 14.380 ug/L
RT: 5.385 min Scan# 1258
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 56 Resp: 448335
Ion Ratio Lower Upper
56 100
69 31.2 25.1 37.7
84 88.3 70.9 106.3


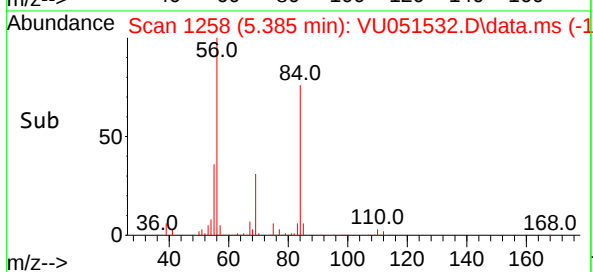
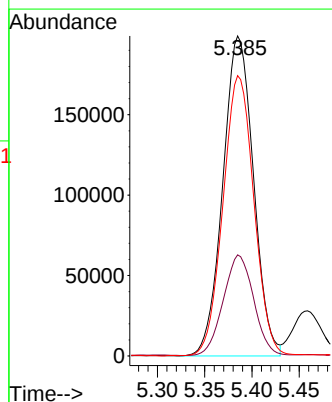
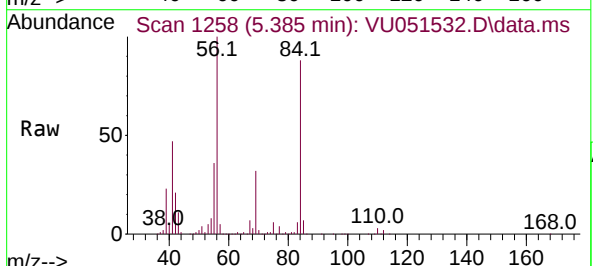


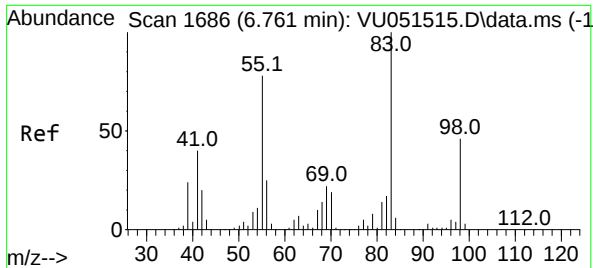

#35
Methylcyclohexane
Concen: 12.448 ug/L
RT: 6.761 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 83 Resp: 401264
Ion Ratio Lower Upper
83 100
55 80.0 65.8 98.6
98 45.5 35.9 53.9

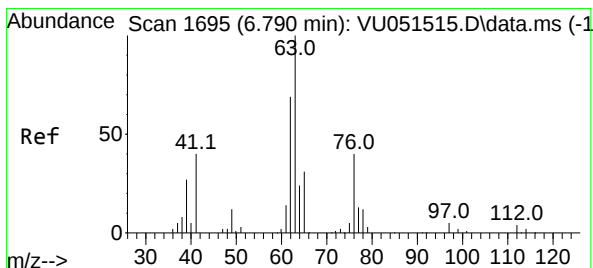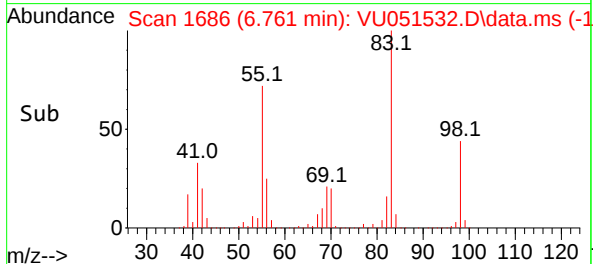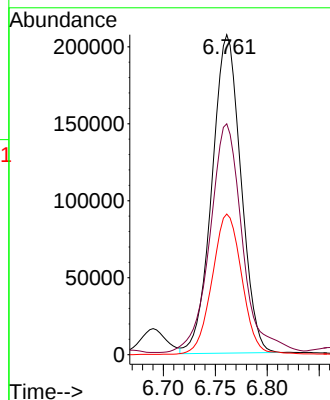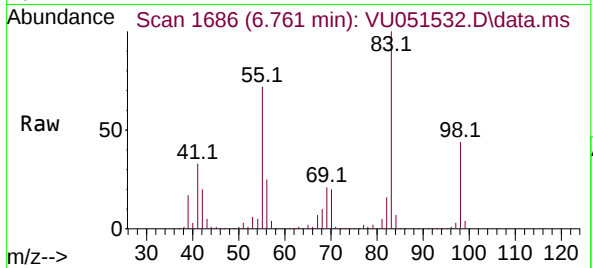

#37
1,2-Dichloropropane
Concen: 0.184 ug/L
RT: 6.758 min Scan# 1685
Delta R.T. -0.032 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 63 Resp: 5155
Ion Ratio Lower Upper
63 100
112 121.7 3.2 4.8#


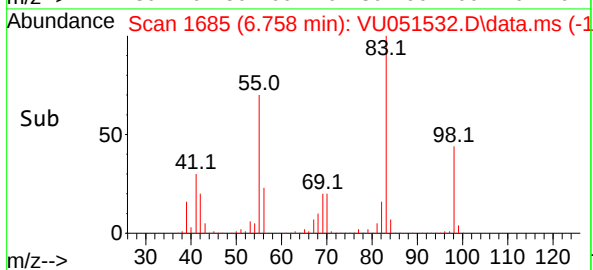
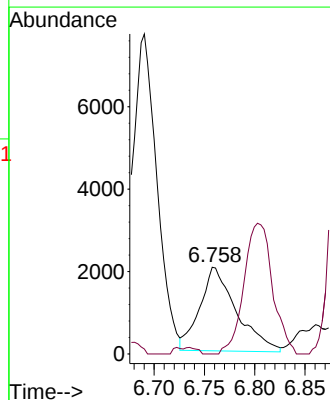
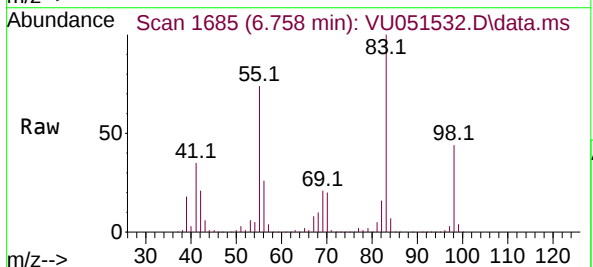


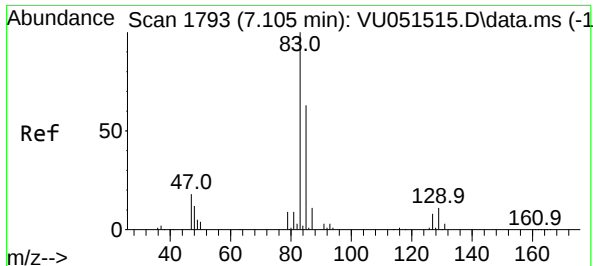

#38
Bromodichloromethane
Concen: 0.776 ug/L
RT: 7.156 min Scan# 11
Delta R.T. 0.051 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 83 Resp: 25976
Ion Ratio Lower Upper
83 100
85 8.4 44.8 83.2#
127 0.0 7.0 10.6#

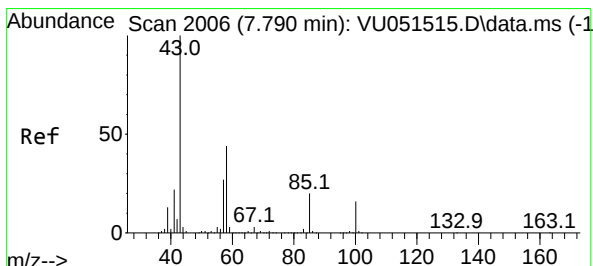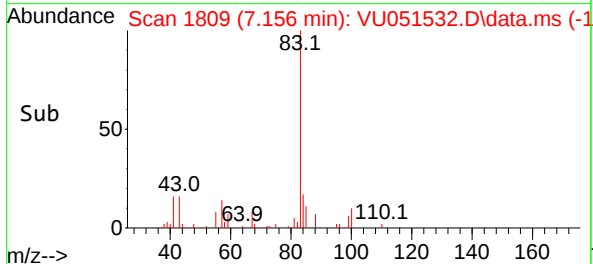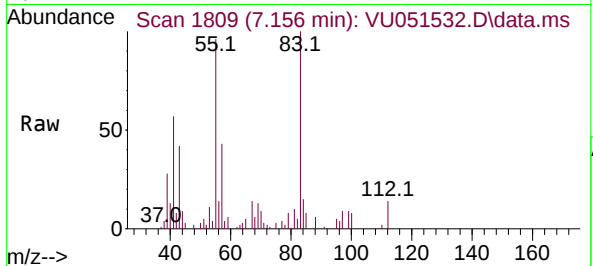

#40
4-Methyl-2-pentanone
Concen: 1.820 ug/L
RT: 7.713 min Scan# 1982
Delta R.T. -0.077 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 43 Resp: 26810
Ion Ratio Lower Upper
43 100
58 2.3 33.0 49.6#
100 0.0 11.8 17.6#


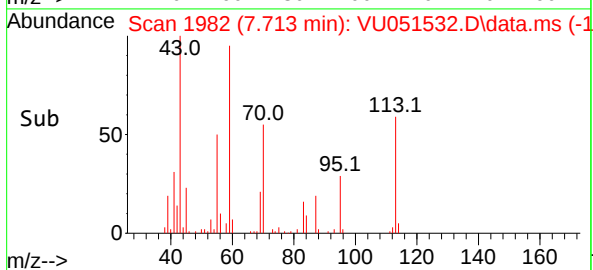

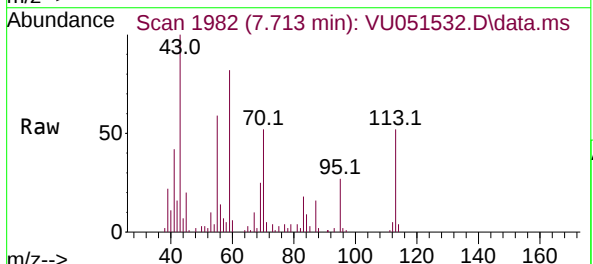




#44
trans-1,3-Dichloropropene
Concen: 19.362 ug/L
RT: 7.980 min Scan# 2065
Delta R.T. -0.228 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 75 Resp: 564939
Ion Ratio Lower Upper
75 100
77 168.3 21.8 40.6#

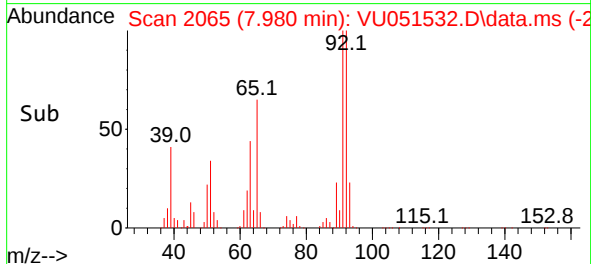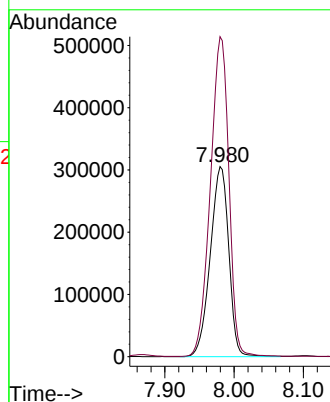

#45
1,1,2-Trichloroethane
Concen: 0.753 ug/L
RT: 8.369 min Scan# 2186
Delta R.T. -0.029 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 97 Resp: 14848
Ion Ratio Lower Upper
97 100
99 1.4 45.3 84.1#
83 12.0 63.1 117.1#
85 8.2 41.8 77.6#


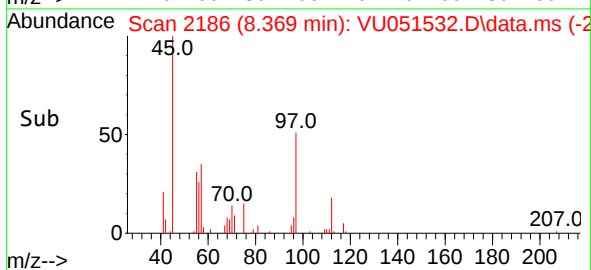
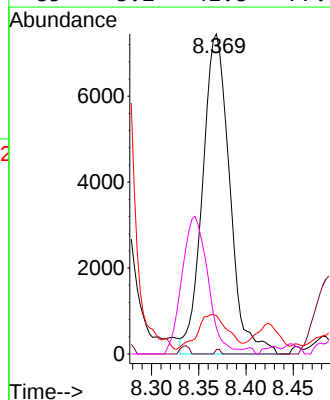
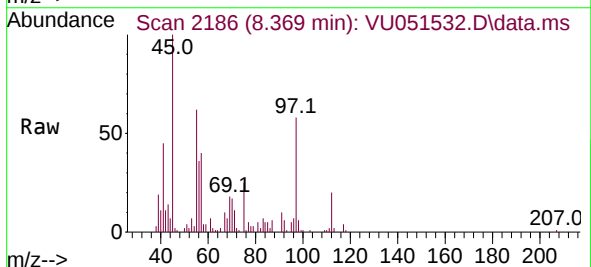




#48
2-Hexanone
Concen: 4.011 ug/L
RT: 8.684 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion: 43 Resp: 43986
Ion Ratio Lower Upper
43 100
58 21.8 48.2 72.2#
57 35.8 15.5 23.3#
100 1.7 9.0 13.4#

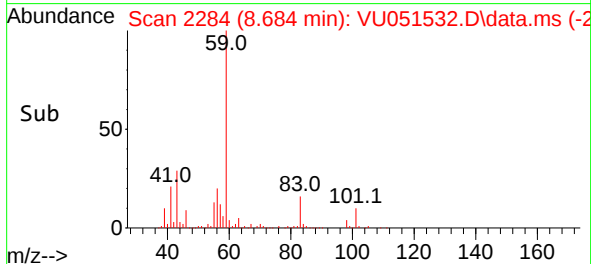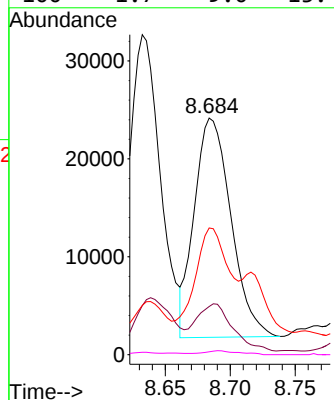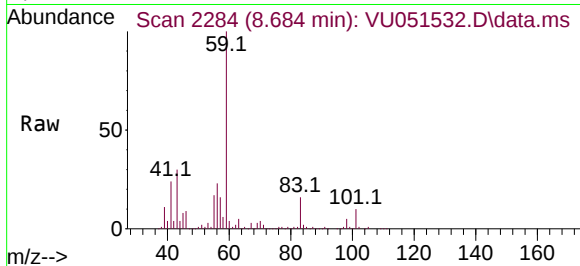

#53
m,p-Xylene
Concen: 285.806 ug/L
RT: 9.697 min Scan# 2599
Delta R.T. 0.006 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion:106 Resp:10829233
Ion Ratio Lower Upper
106 100
91 126.4 143.9 267.3#


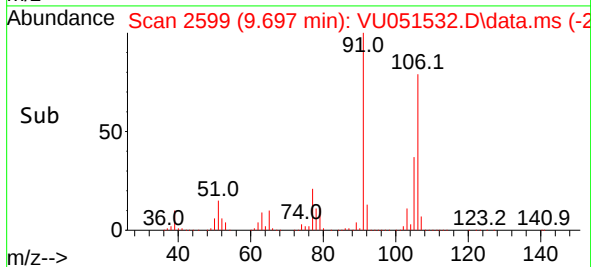
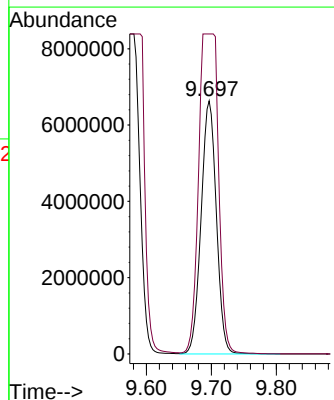
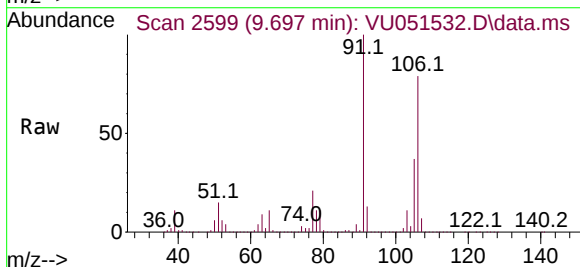




#54
o-Xylene
Concen: 170.957 ug/L
RT: 10.102 min Scan# 2725
Delta R.T. 0.003 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:106 Resp: 6129013
Ion Ratio Lower Upper
106 100
91 212.4 154.4 286.8

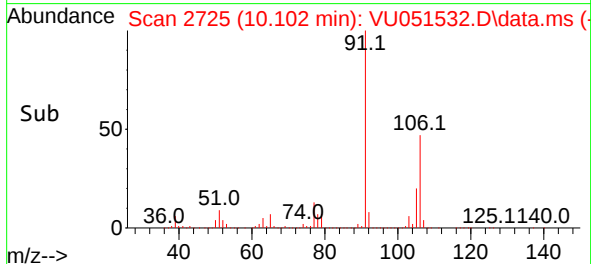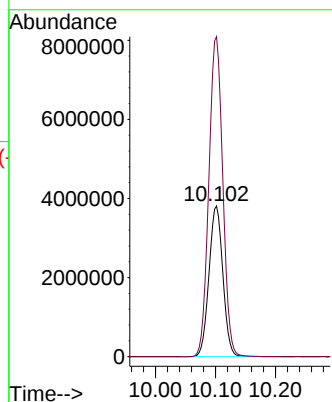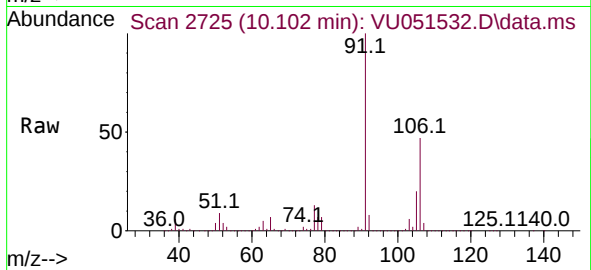

#55
Styrene
Concen: 5.266 ug/L
RT: 10.102 min Scan# 2725
Delta R.T. -0.010 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion:104 Resp: 325009
Ion Ratio Lower Upper
104 100
78 285.8 32.1 59.7#

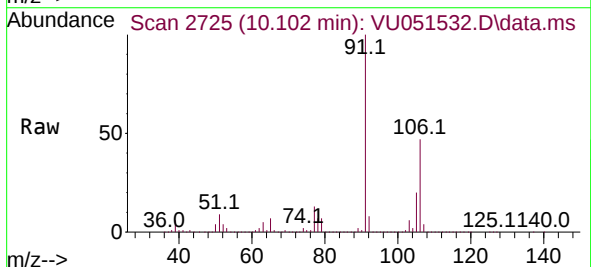



#57

1,1,2,2-Tetrachloroethane

Concen: 2.300 ug/L

RT: 10.716 min Scan# 2936

Delta R.T. -0.064 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13

Instrument :

MSVOA_U

ClientSampleId :

BHA80





Tgt Ion: 83 Resp: 56124

Ion Ratio Lower Upper

83 100

85 3.6 45.9 85.3#

131 0.0 7.4 11.2#

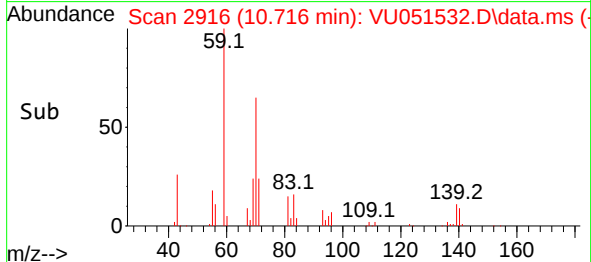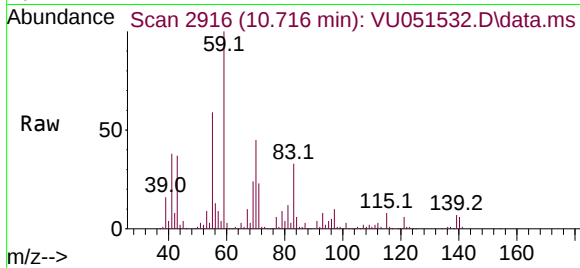

#60

Isopropylbenzene

Concen: 53.755 ug/L

RT: 10.484 min Scan# 2844

Delta R.T. -0.000 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13




Tgt Ion:105 Resp: 5541011


Ion Ratio Lower Upper

105 100

120 26.3 20.6 30.8

77 15.1 13.5 20.3


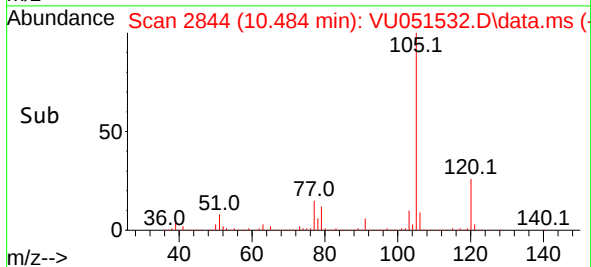

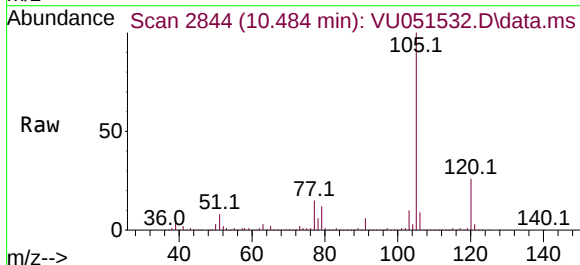


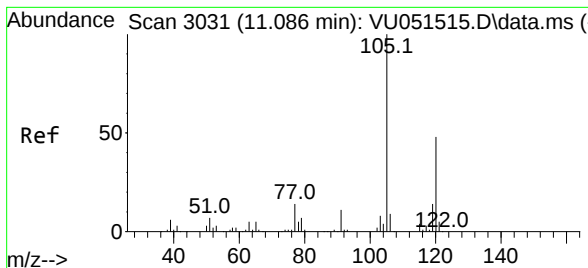

#62
1,3,5-Trimethylbenzene
Concen: 23.588 ug/L
RT: 11.086 min Scan# 3031
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:105 Resp: 644993
Ion Ratio Lower Upper
105 100
120 48.5 37.7 56.5

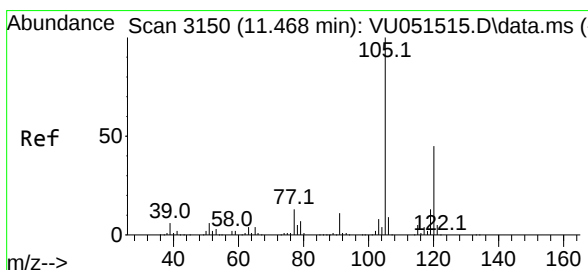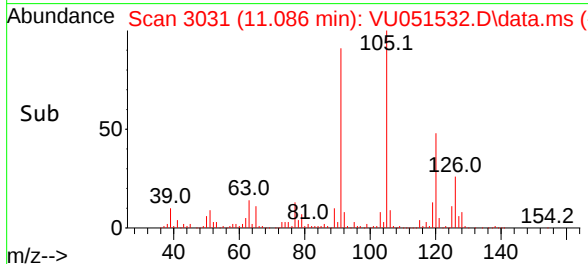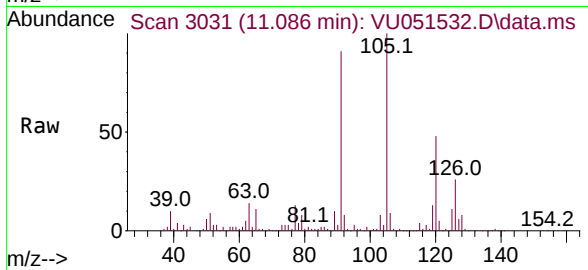

#63
1,2,4-Trimethylbenzene
Concen: 106.390 ug/L
RT: 11.468 min Scan# 3150
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion:105 Resp: 8227384
Ion Ratio Lower Upper
105 100
120 45.1 35.6 53.4


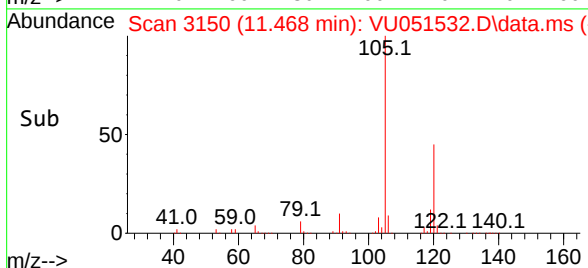

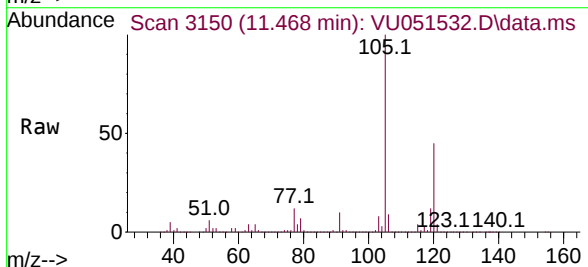




#64
1,3-Dichlorobenzene
Concen: 6.438 ug/L
RT: 11.745 min Scan# 31
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:146 Resp: 328267
Ion Ratio Lower Upper
146 100
111 41.9 28.3 52.7
148 64.5 43.8 81.4

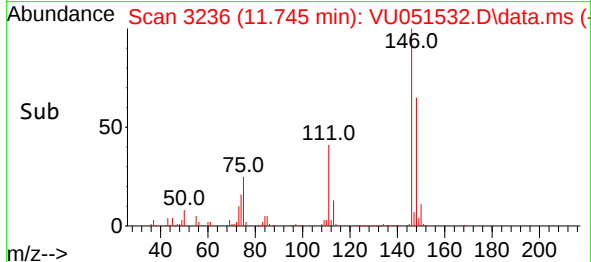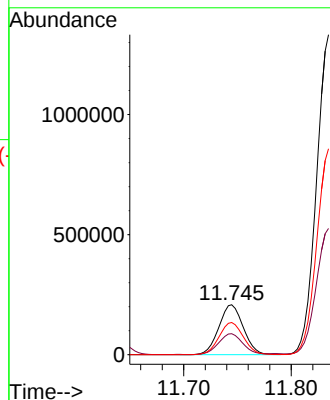

#65
1,4-Dichlorobenzene
Concen: 41.020 ug/L
RT: 11.835 min Scan# 3264
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion:146 Resp: 2061528
Ion Ratio Lower Upper
146 100
111 39.5 29.1 54.1
148 64.4 44.2 82.0


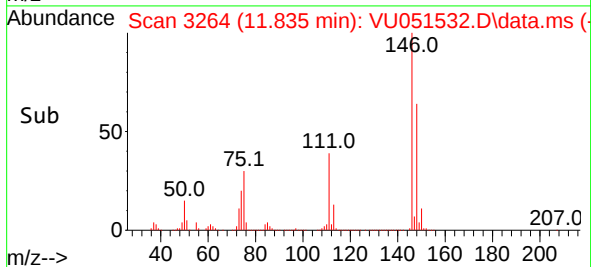
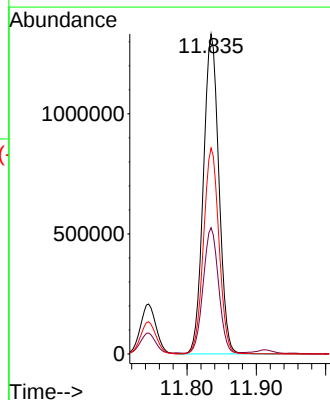
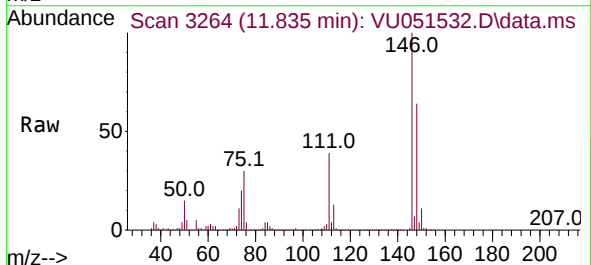




#67
1,2-Dichlorobenzene
Concen: 20.994 ug/L
RT: 12.211 min Scan# 311
Delta R.T. -0.000 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13




Instrument :
MSVOA_U
ClientSampleId :
BHA80


Tgt Ion:146 Resp: 1040618
Ion Ratio Lower Upper
146 100
111 42.4 35.5 53.3
148 64.2 50.9 76.3

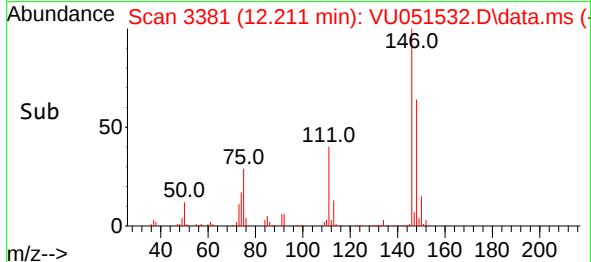

#68
1,2-Dibromo-3-chloropropane
Concen: 1.818 ug/L
RT: 12.970 min Scan# 3617
Delta R.T. -0.026 min
Lab File: VU051532.D
Acq: 27 Oct 2022 04:13

Tgt Ion: 75 Resp: 7147
Ion Ratio Lower Upper
75 100
155 0.0 62.7 94.1#
157 0.0 78.3 117.5#

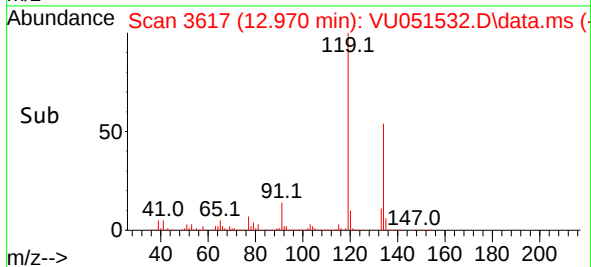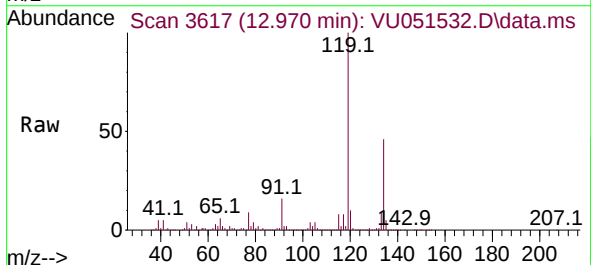

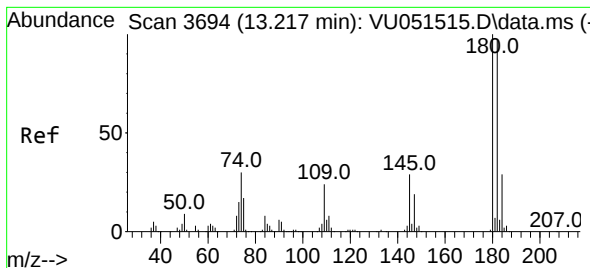

#69

1,3,5-Trichlorobenzene

Concen: 0.101 ug/L

RT: 13.220 min Scan# 3695

Delta R.T. 0.003 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13

Instrument :

MSVOA_U

ClientSampleId :

BHA80

Tgt Ion:180 Resp: 3550





Ion Ratio Lower Upper

180 100

182 105.0 77.7 116.5

184 35.7 23.6 35.4#

145 69.9 23.4 35.2#

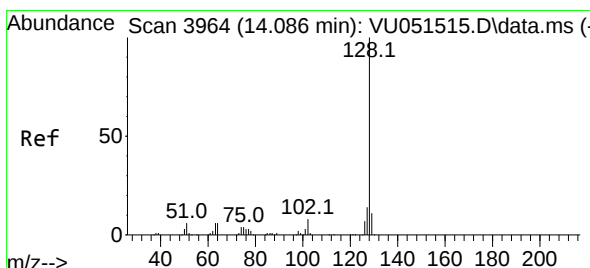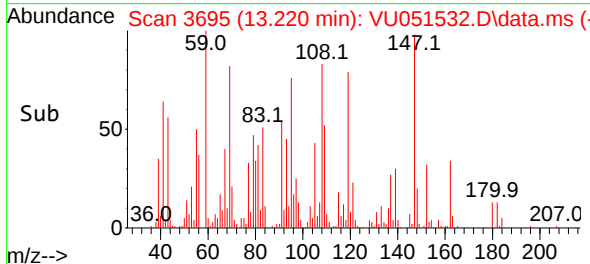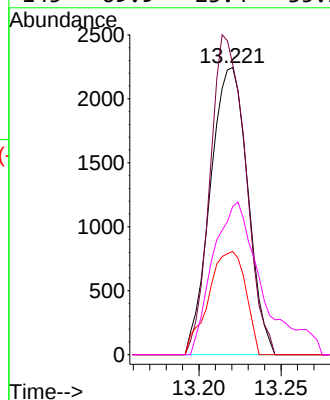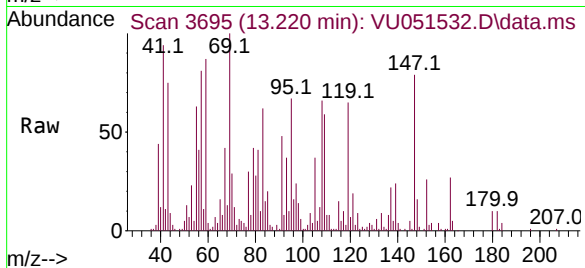

#71

Naphthalene

Concen: 17.722 ug/L

RT: 14.082 min Scan# 3963

Delta R.T. -0.003 min

Lab File: VU051532.D

Acq: 27 Oct 2022 04:13

Tgt Ion:128 Resp: 822825

Ion Ratio Lower Upper

128 100

129 11.0 8.5 12.7

127 12.7 11.1 16.7

