

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051516.D
 Acq On : 26 Oct 2022 21:27
 Operator : JC/MD
 Sample : VU1026WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK119

Quant Time: Oct 27 08:11:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 27 08:11:03 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	233885	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	246382	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	91659	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	100952	5.351	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 107.000%		
7) Chloroethane-d5	1.906	69	90449	5.580	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 111.600%		
11) 1,1-Dichloroethene-d2	2.562	65	37405	5.016	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 100.400%		
20) 2-Butanone-d5	4.616	46	225864	54.376	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 108.760%		
24) Chloroform-d	5.060	84	163146	4.638	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 92.800%		
26) 1,2-Dichloroethane-d4	5.700	65	92004	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 101.400%		
32) Benzene-d6	5.726	84	332715	4.909	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 98.200%		
36) 1,2-Dichloropropane-d6	6.690	67	111068	4.825	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 96.600%		
41) Toluene-d8	7.896	98	254475	4.196	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 84.000%		
43) trans-1,3-Dichloroprop...	8.179	79	30630	4.050	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 81.000%		
46) 2-Hexanone-d5	8.629	63	150144	58.907	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 117.820%		
56) 1,1,2,2-Tetrachloroeth...	10.754	84	93087	5.062	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 101.200%		
66) 1,2-Dichlorobenzene-d4	12.192	152	82427	5.174	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 103.400%		
Target Compounds						Qvalue
16) Methylene chloride	3.038	84	7928	0.315	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051516.D
Acq On : 26 Oct 2022 21:27
Operator : JC/MD
Sample : VU1026WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK119

Quant Time: Oct 27 08:11:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 27 08:11:03 2022
Response via : Initial Calibration

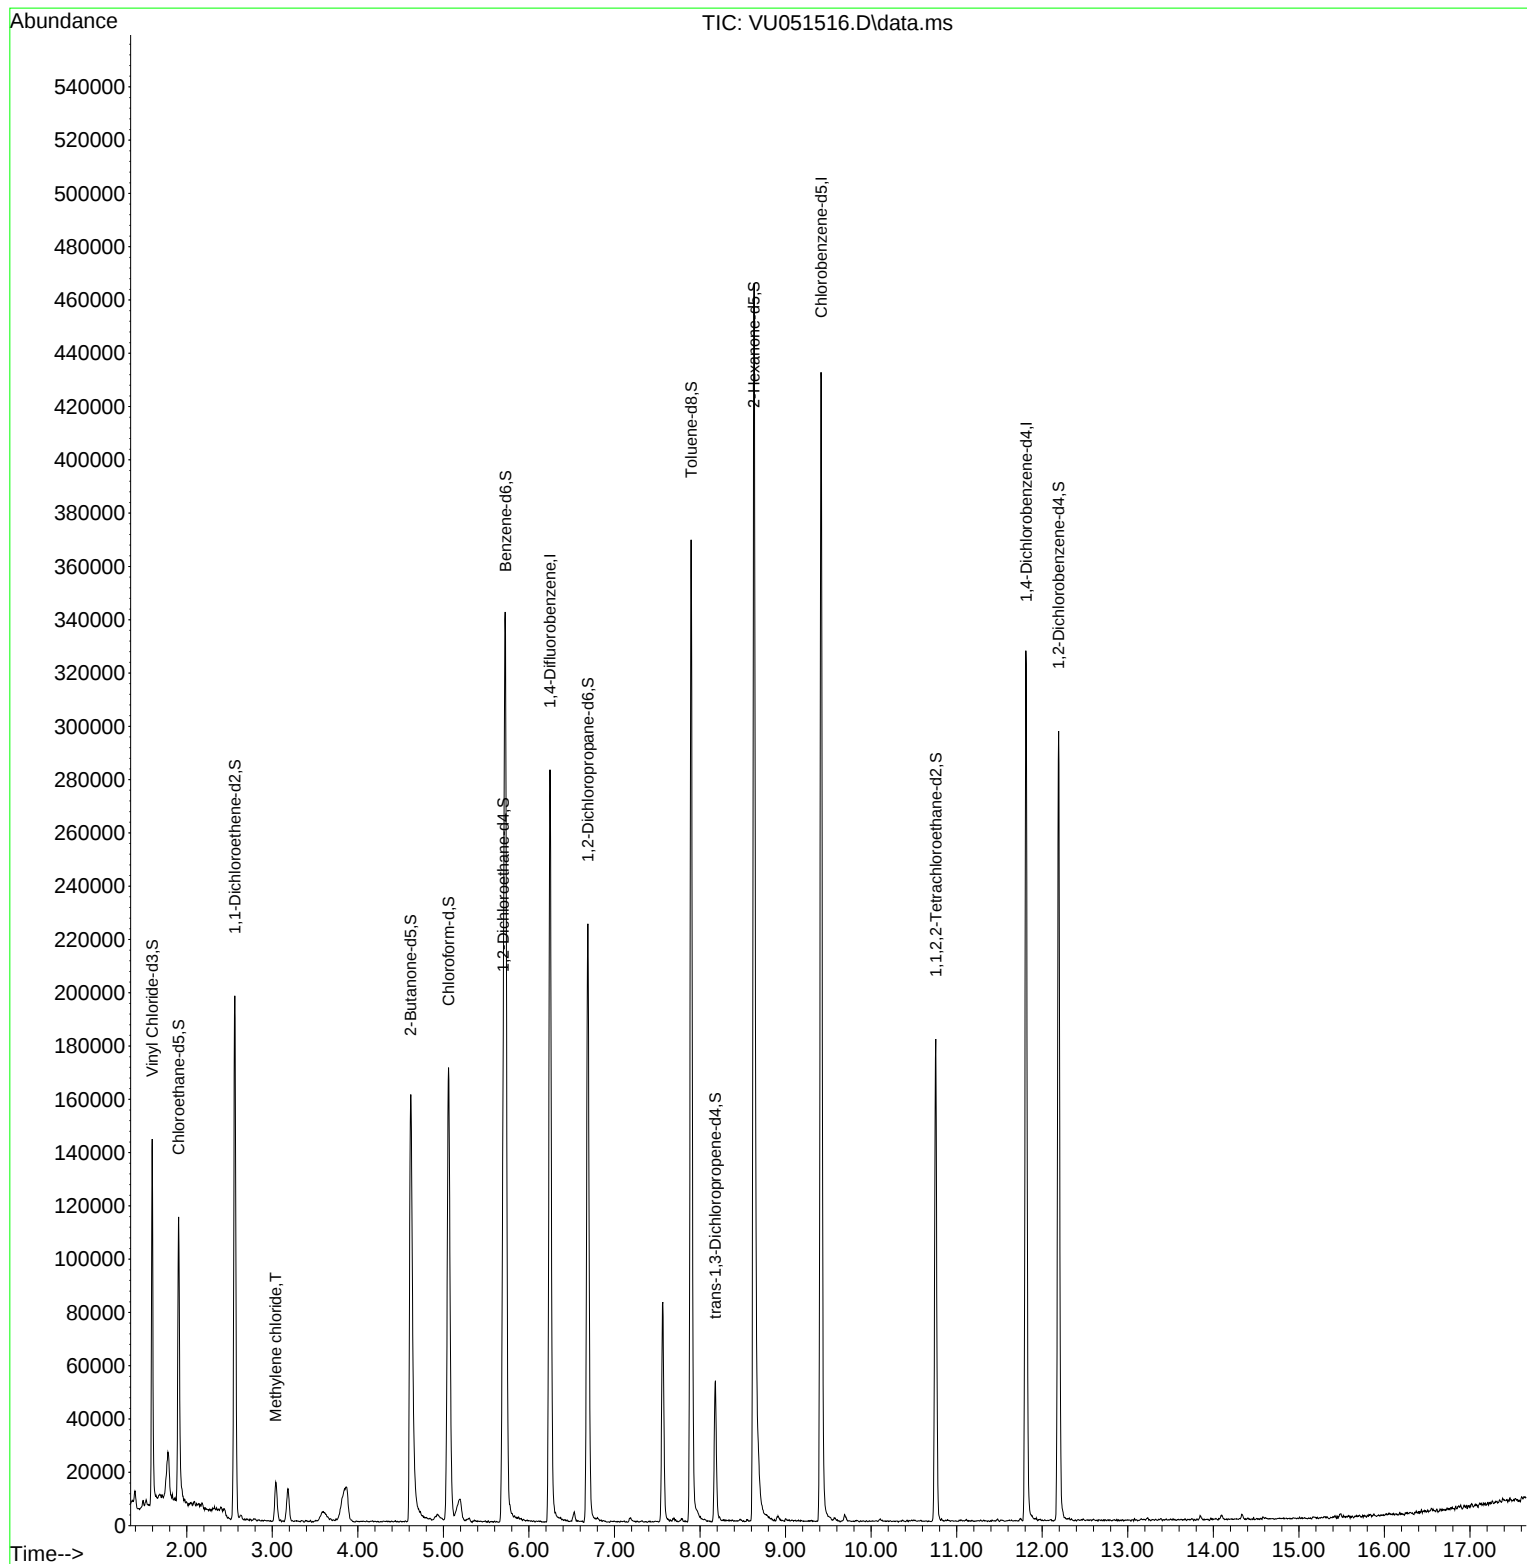

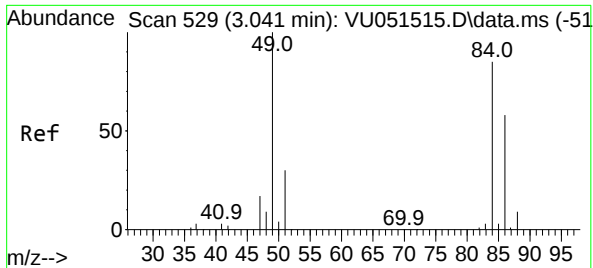

#16
Methylene chloride
Concen: 0.315 ug/L
RT: 3.038 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU051516.D
Acq: 26 Oct 2022 21:27

Instrument :
MSVOA_U
ClientSampleId :
VBLK119

Tgt Ion:	84	Resp:	7928
Ion	Ratio	Lower	Upper
84	100		
86	68.5	46.5	86.3
49	101.4	81.3	151.1

