

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051506.D
 Acq On : 26 Oct 2022 16:52
 Operator : JC/MD
 Sample : N5270-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	90	rBV	142493	185952	17.81%	2.194%
2	1.909	169	177	192	rVB	114963	153507	14.70%	1.811%
3	2.562	366	380	394	rBV	203407	329151	31.53%	3.883%
4	2.758	430	441	457	rBV	25224	47593	4.56%	0.561%
5	3.183	561	573	586	rBV	7368	15669	1.50%	0.185%
6	3.363	614	629	643	rBV	19256	44435	4.26%	0.524%
7	3.858	755	783	785	rBV	13493	41089	3.94%	0.485%
8	3.990	810	824	842	rBV5	5547	15394	1.47%	0.182%
9	4.620	1006	1020	1056	rBV	179257	459348	44.00%	5.419%
10	5.064	1139	1158	1183	rBV3	213085	625455	59.90%	7.379%
11	5.723	1341	1363	1377	rBV2	380664	1017749	97.48%	12.007%
12	6.247	1513	1526	1546	rBV	305145	582586	55.80%	6.873%
13	6.539	1606	1617	1628	rBV10	6226	12857	1.23%	0.152%
14	6.690	1647	1664	1682	rBV	243298	478424	45.82%	5.644%
15	7.565	1921	1936	1951	rBV2	94124	172317	16.50%	2.033%
16	7.896	2024	2039	2054	rBV	403085	715038	68.48%	8.435%
17	7.967	2055	2061	2073	rVB2	14931	28790	2.76%	0.340%
18	8.179	2116	2127	2145	rBV	58918	103062	9.87%	1.216%
19	8.552	2233	2243	2253	rVB4	9212	14897	1.43%	0.176%
20	8.633	2253	2268	2302	rBV2	528117	1044091	100.00%	12.317%
21	9.417	2495	2512	2539	rBV	448264	774649	74.19%	9.139%
22	9.571	2551	2560	2575	rVB	11603	18191	1.74%	0.215%
23	9.690	2584	2597	2610	rBV2	34537	59673	5.72%	0.704%
24	10.755	2916	2928	2942	rBV	200436	320132	30.66%	3.777%
25	11.812	3244	3257	3276	rBV	370347	605921	58.03%	7.148%
26	12.192	3362	3375	3396	rBV	348451	581750	55.72%	6.863%
27	15.484	4391	4399	4412	rVB2	19136	28818	2.76%	0.340%




Sum of corrected areas: 8476538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051506.D
Acq On : 26 Oct 2022 16:52
Operator : JC/MD
Sample : N5270-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

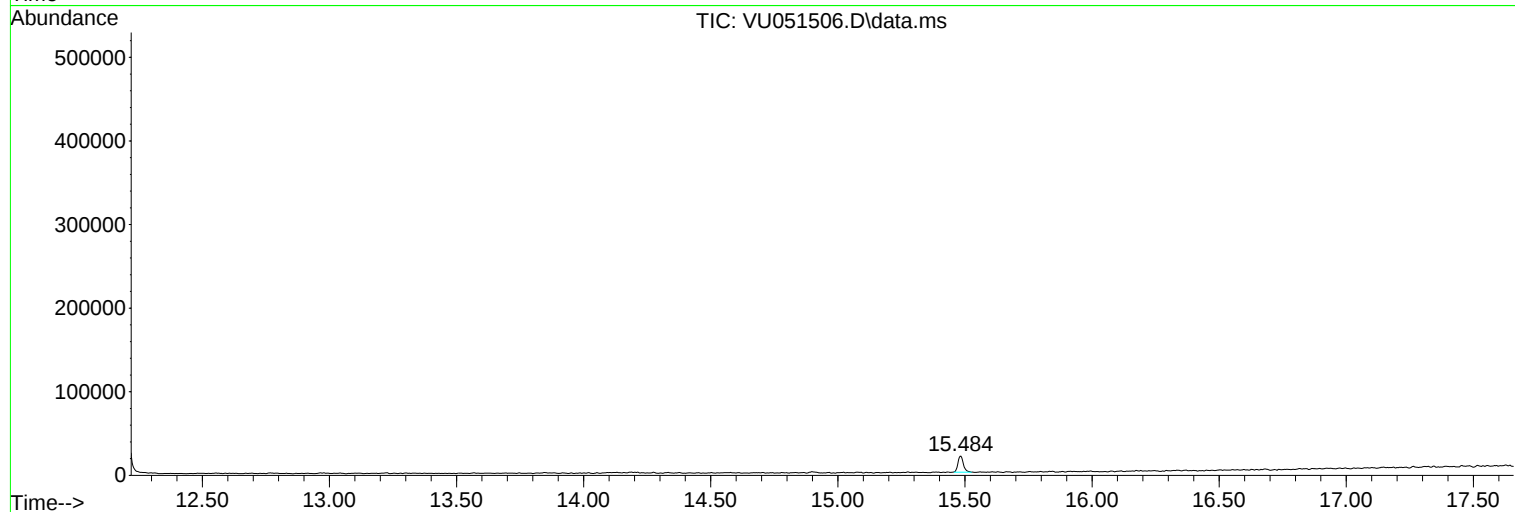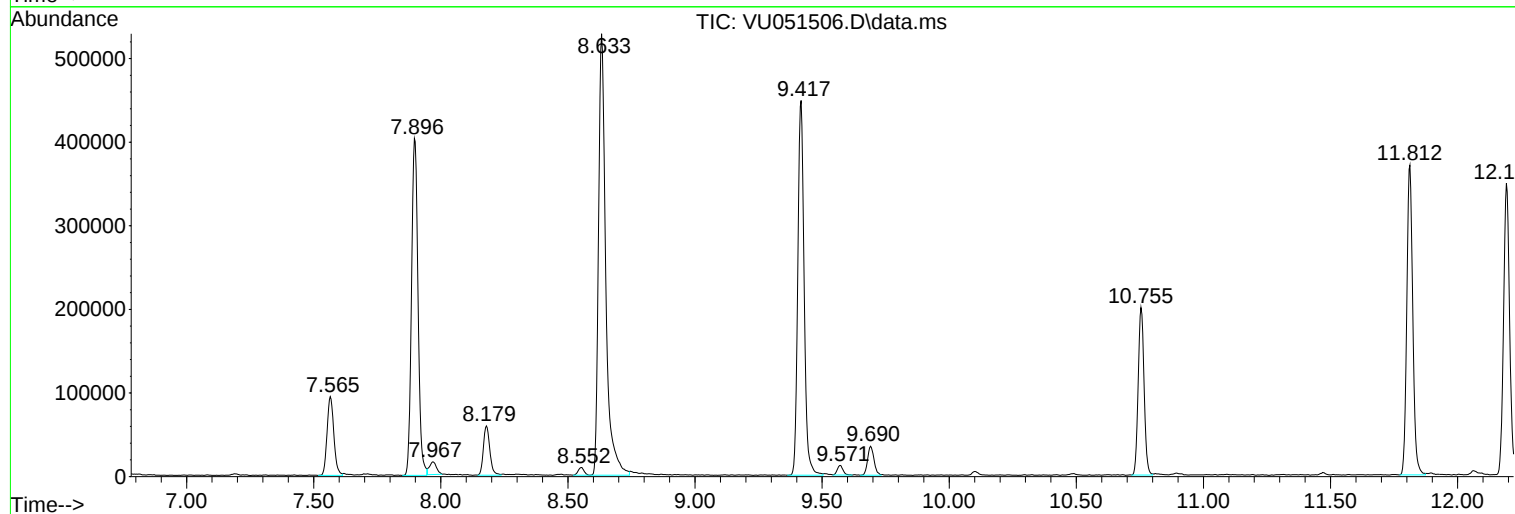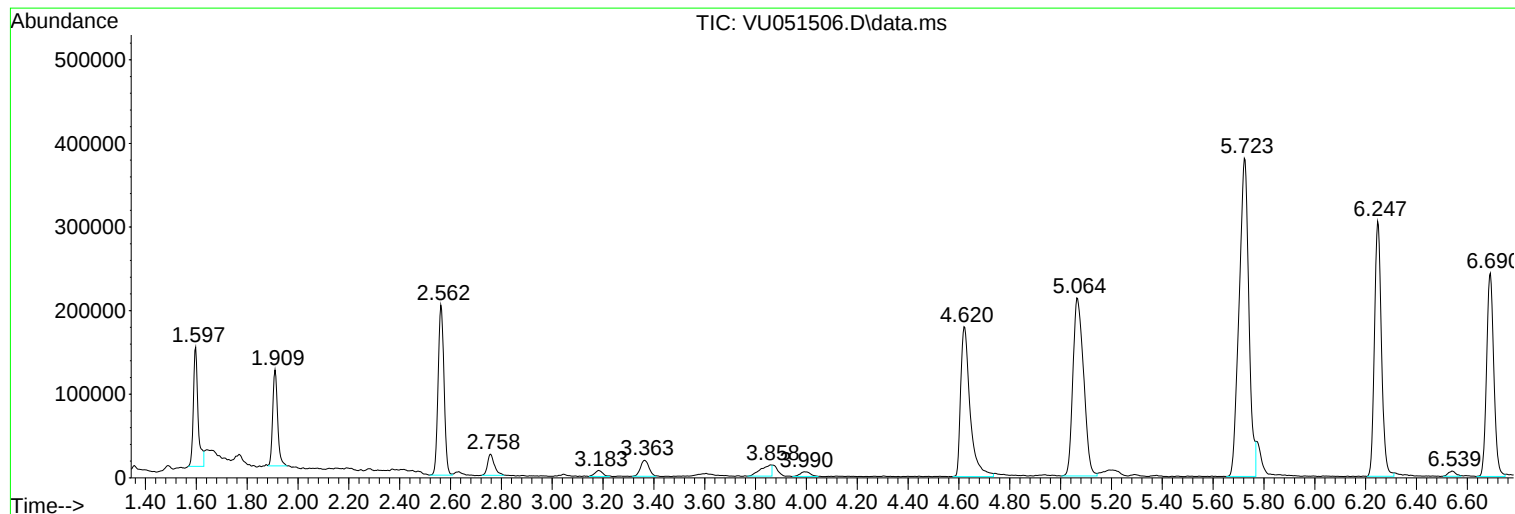

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051506.D
Acq On : 26 Oct 2022 16:52
Operator : JC/MD
Sample : N5270-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051506.D
Acq On : 26 Oct 2022 16:52
Operator : JC/MD
Sample : N5270-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc