

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051512.D
 Acq On : 26 Oct 2022 19:26
 Operator : JC/MD
 Sample : N5270-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	85542	104538	11.07%	1.485%
2	1.909	169	177	198	rVB	78647	110783	11.73%	1.574%
3	2.562	369	380	392	rBV	137497	224865	23.81%	3.195%
4	2.623	392	399	413	rVB2	14764	26745	2.83%	0.380%
5	2.758	431	441	463	rVB3	7910	16702	1.77%	0.237%
6	3.182	557	573	590	rVB2	10260	23805	2.52%	0.338%
7	3.861	753	784	787	rBV	13793	43614	4.62%	0.620%
8	4.620	1006	1020	1066	rBV	153830	407383	43.14%	5.788%
9	5.070	1142	1160	1180	rBV3	183767	569652	60.33%	8.093%
10	5.186	1185	1196	1215	rVB	9010	32142	3.40%	0.457%
11	5.722	1340	1363	1396	rBV2	285969	780185	82.63%	11.084%
12	6.247	1513	1526	1549	rBV	261388	512137	54.24%	7.276%
13	6.690	1648	1664	1692	rBV	198087	392780	41.60%	5.580%
14	7.166	1802	1812	1825	rVB4	6816	13930	1.48%	0.198%
15	7.565	1923	1936	1960	rBV2	75642	135787	14.38%	1.929%
16	7.710	1972	1981	1993	rVB5	7012	12142	1.29%	0.172%
17	7.896	2023	2039	2054	rBV	299701	522456	55.33%	7.422%
18	7.970	2055	2062	2079	rVB3	18225	35728	3.78%	0.508%
19	8.179	2113	2127	2145	rBV2	47379	81436	8.62%	1.157%
20	8.632	2256	2268	2300	rBV2	465638	944222	100.00%	13.414%
21	8.787	2308	2316	2330	rVB7	13872	25125	2.66%	0.357%
22	9.417	2499	2512	2533	rBV	402501	680622	72.08%	9.669%
23	9.690	2585	2597	2609	rBV3	12295	21594	2.29%	0.307%
24	10.098	2715	2724	2741	rVB7	4772	9534	1.01%	0.135%
25	10.754	2916	2928	2942	rBV	179347	287286	30.43%	4.081%
26	11.812	3242	3257	3278	rBV	318198	523600	55.45%	7.439%
27	12.063	3326	3335	3350	rBV5	11387	21954	2.33%	0.312%
28	12.192	3359	3375	3393	rBV	278043	460372	48.76%	6.540%
29	12.893	3583	3593	3605	rBV5	10703	17834	1.89%	0.253%




Sum of corrected areas: 7038953

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051512.D
Acq On : 26 Oct 2022 19:26
Operator : JC/MD
Sample : N5270-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

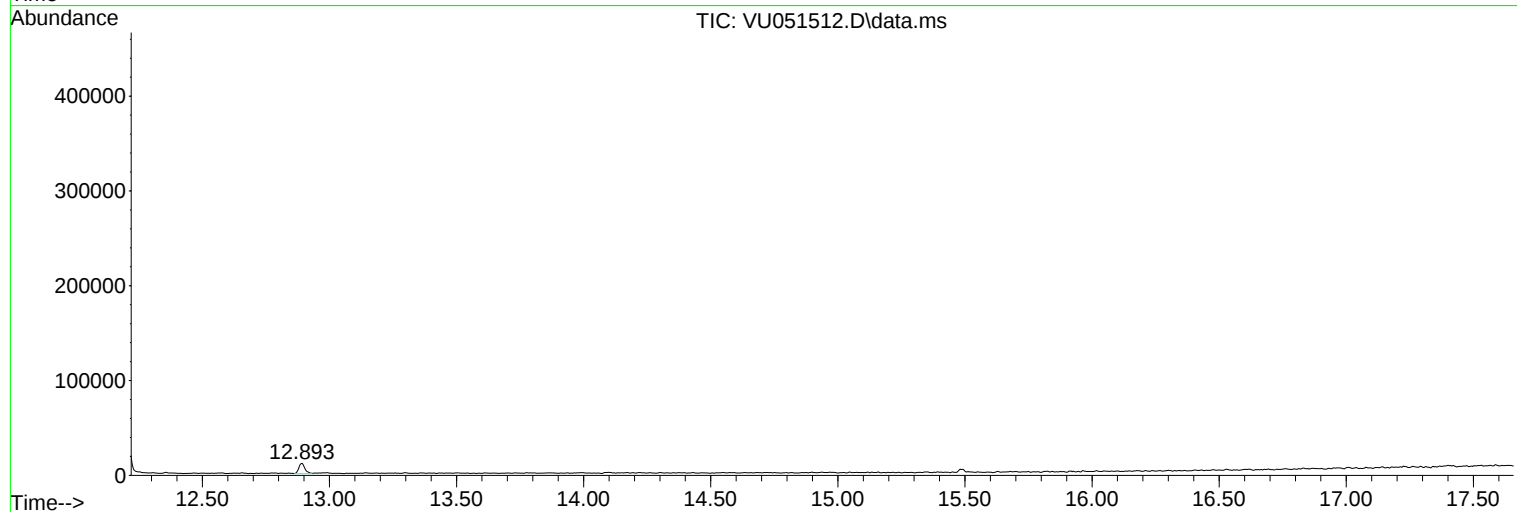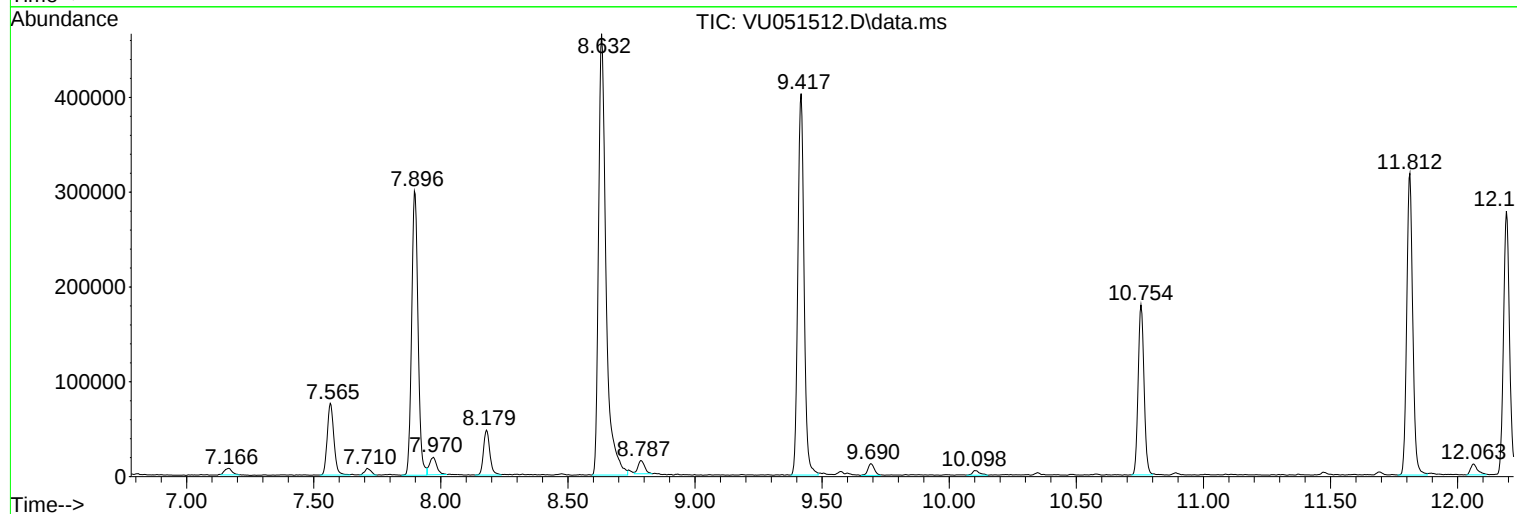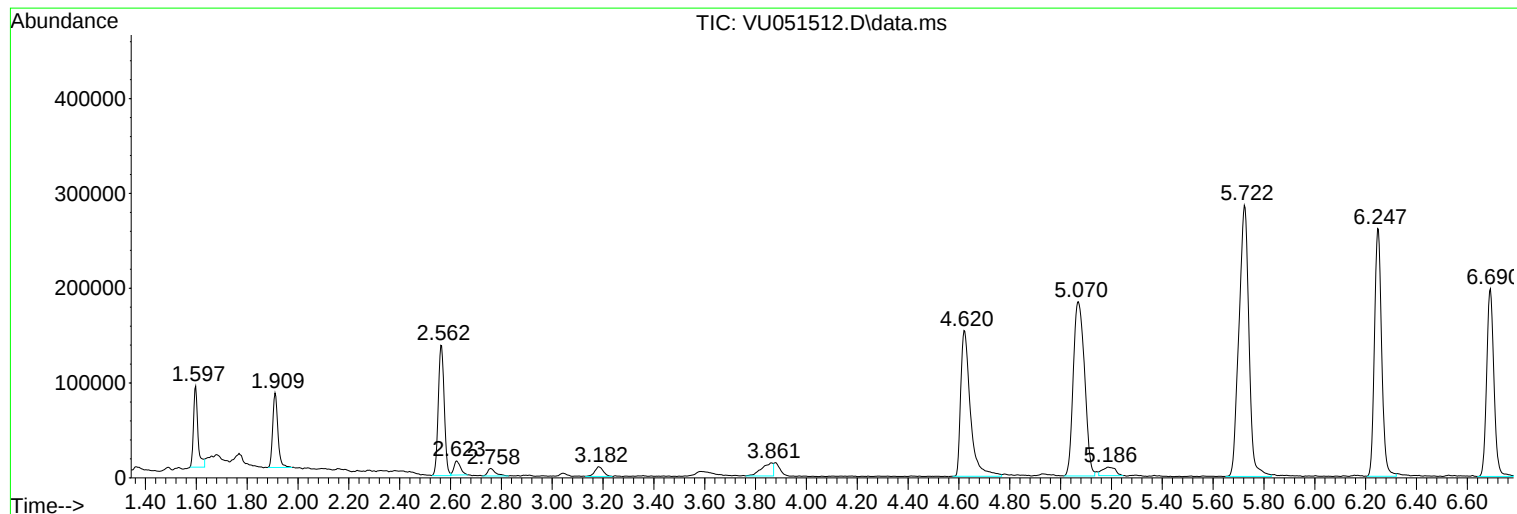

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051512.D
Acq On : 26 Oct 2022 19:26
Operator : JC/MD
Sample : N5270-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051512.D
Acq On : 26 Oct 2022 19:26
Operator : JC/MD
Sample : N5270-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc