

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
 Data File : VU051516.D
 Acq On : 26 Oct 2022 21:27
 Operator : JC/MD
 Sample : VU1026WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK119

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	93	rBV	137471	160713	17.55%	2.183%
2	1.781	126	137	150	rVB5	17340	39508	4.31%	0.537%
3	1.906	167	176	195	rVB	106535	156072	17.05%	2.120%
4	2.562	365	380	395	rBV	196556	320315	34.98%	4.351%
5	3.041	518	529	543	rBV2	14732	29740	3.25%	0.404%
6	3.182	559	573	588	rBV2	12395	27031	2.95%	0.367%
7	3.848	751	780	781	rBV3	11738	33791	3.69%	0.459%
8	4.620	1004	1020	1052	rBV	160433	408634	44.63%	5.550%
9	5.060	1141	1157	1177	rBV	169698	387009	42.27%	5.256%
10	5.195	1179	1199	1216	rVB	8026	30422	3.32%	0.413%
11	5.723	1337	1363	1387	rBV2	341709	910281	99.41%	12.364%
12	6.247	1512	1526	1544	rBV	282397	545967	59.63%	7.416%
13	6.690	1648	1664	1689	rBV	224670	442194	48.29%	6.006%
14	7.565	1920	1936	1952	rBV2	82581	147691	16.13%	2.006%
15	7.896	2026	2039	2070	rBV	368548	649252	70.91%	8.818%
16	8.179	2115	2127	2140	rBV	52980	90671	9.90%	1.232%
17	8.632	2255	2268	2308	rBV2	464486	915646	100.00%	12.437%
18	9.414	2498	2511	2538	rBV	431275	729606	79.68%	9.910%
19	10.754	2912	2928	2946	rBV	181128	294910	32.21%	4.006%
20	11.809	3244	3256	3276	rBV	326636	540473	59.03%	7.341%
21	12.192	3356	3375	3396	rBV	296537	502582	54.89%	6.826%




Sum of corrected areas: 7362508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051516.D
Acq On : 26 Oct 2022 21:27
Operator : JC/MD
Sample : VU1026WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

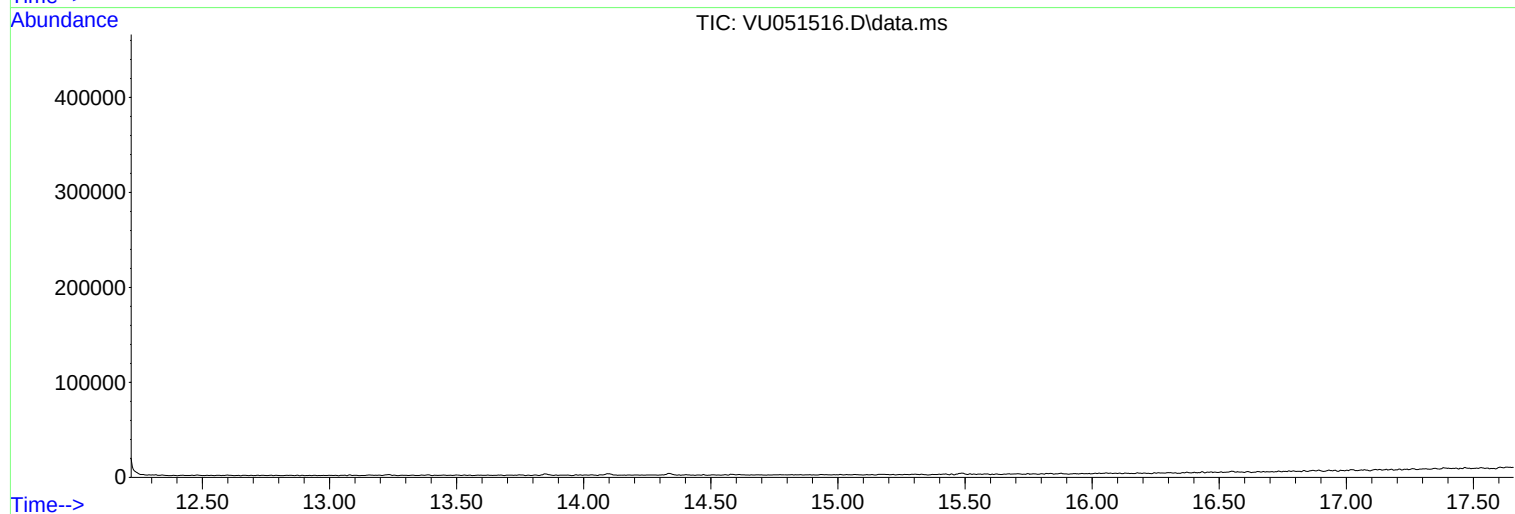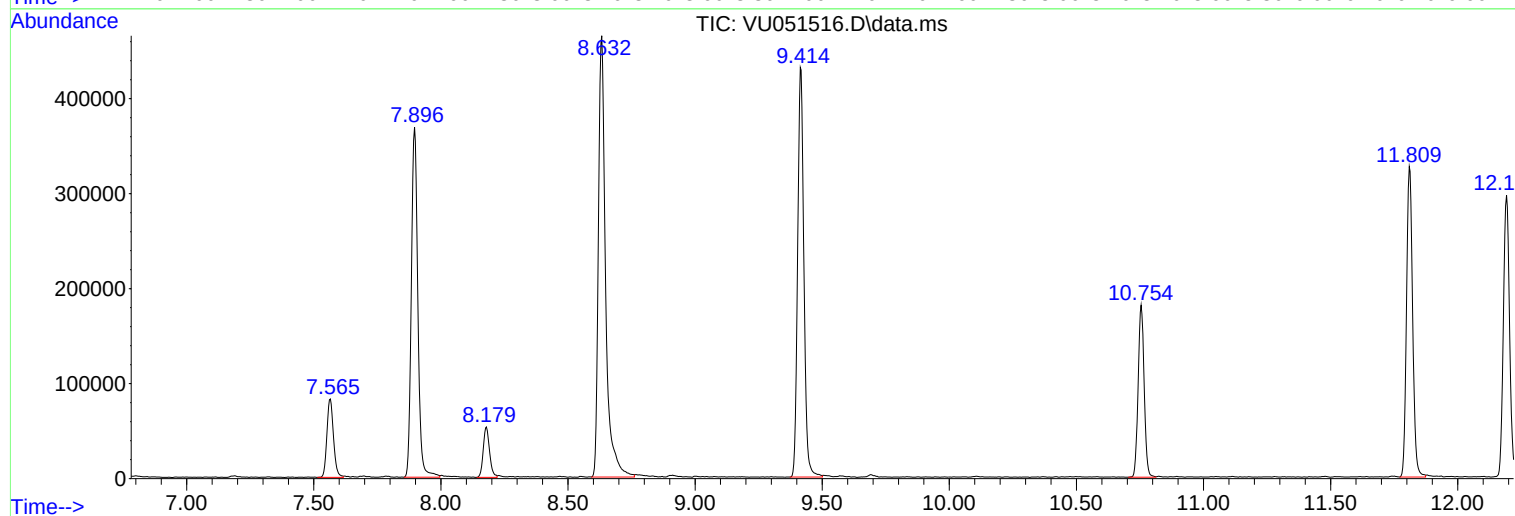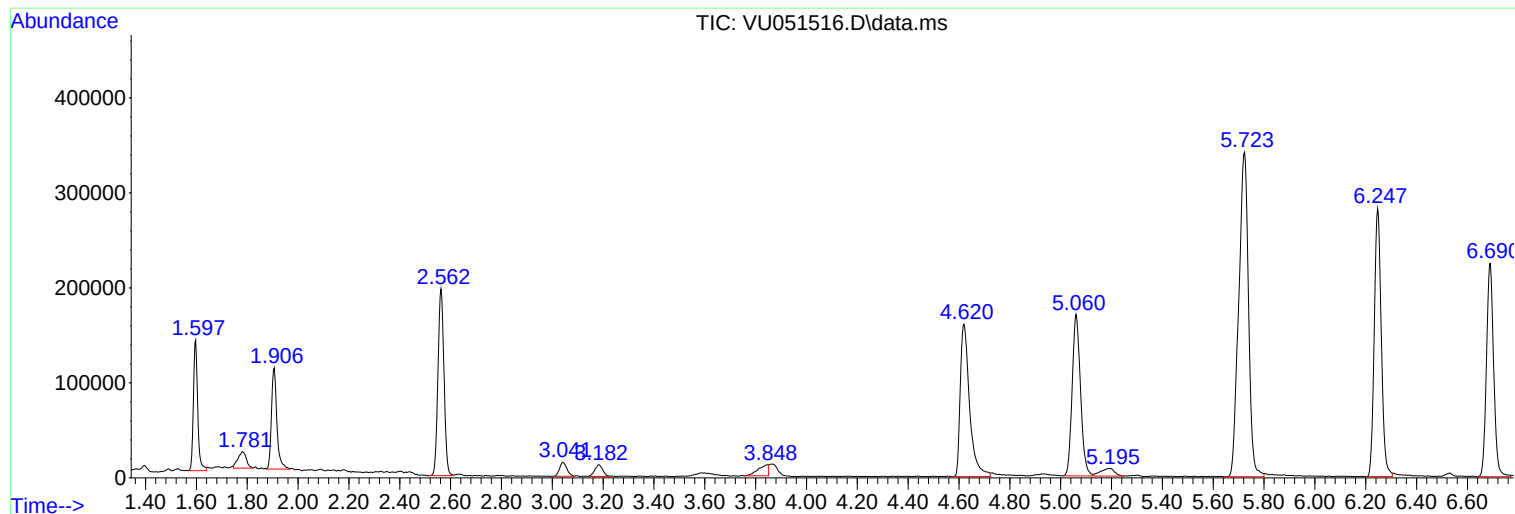

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051516.D
Acq On : 26 Oct 2022 21:27
Operator : JC/MD
Sample : VU1026WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051516.D
Acq On : 26 Oct 2022 21:27
Operator : JC/MD
Sample : VU1026WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc