
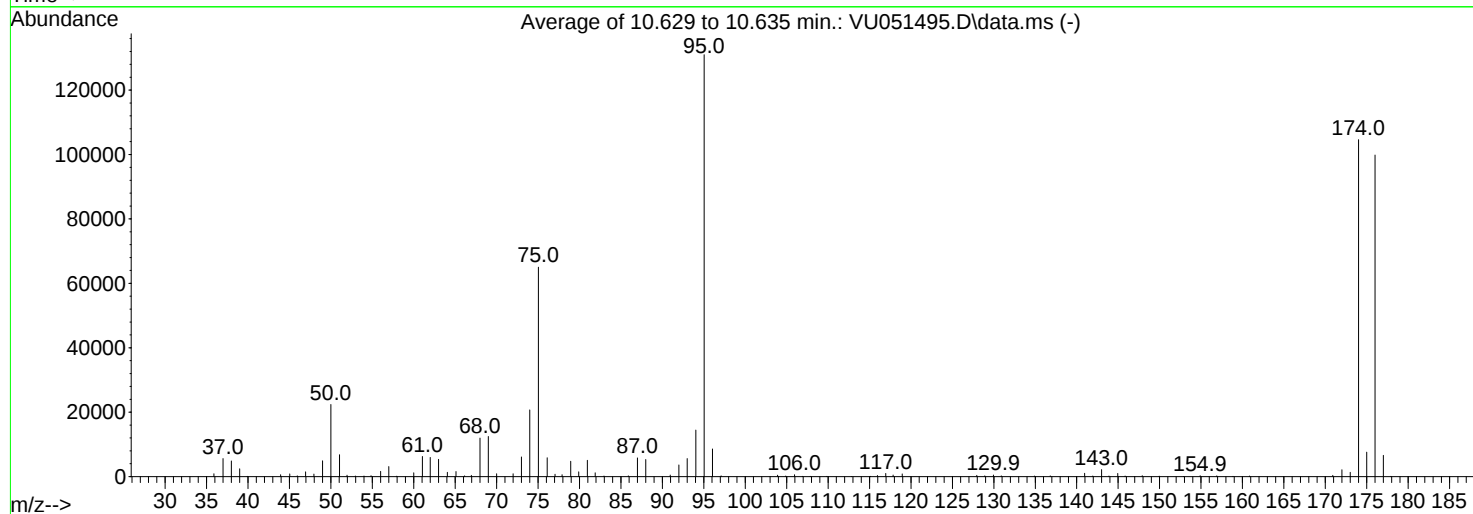


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102622\
Data File : VU051495.D
Acq On : 26 Oct 2022 09:17
Operator : JC/MD
Sample : BFB157
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB157

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 28 00:08:00 2022

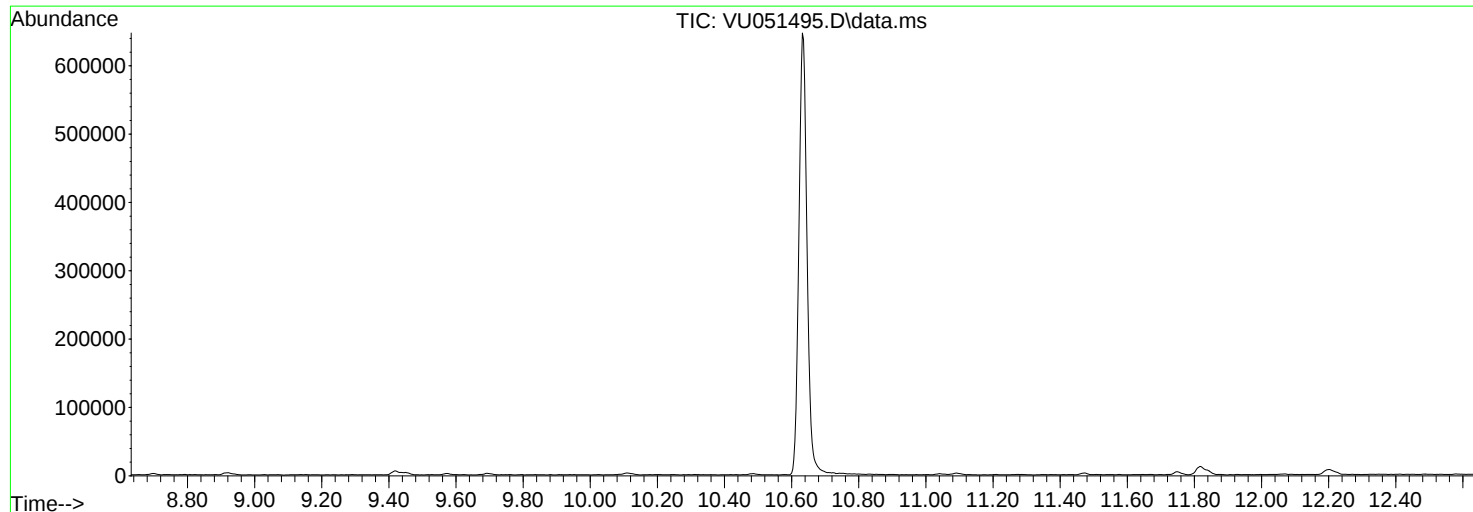

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	22379	PASS
75	95	30	80	49.6	65035	PASS
95	95	100	100	100.0	130987	PASS
96	95	5	9	6.5	8562	PASS
173	174	0.00	2	1.3	1312	PASS
174	95	50	120	79.9	104637	PASS
175	174	5	9	7.2	7563	PASS
176	174	95	101	95.4	99835	PASS
177	176	5	9	6.6	6587	PASS

Scan 2876 (10.587 min): VU051495.D\data.ms
BFB157

m/z	Abundance
39.90	934.0
43.90	656.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	833.0
37.00	5475.0
38.00	4544.0
39.00	2336.0
39.90	1040.0
44.00	1274.0
45.00	827.0
46.00	241.0
46.90	1468.0
47.90	704.0
49.00	4924.0
50.00	21528.0
51.10	6531.0
52.00	412.0
52.90	194.0
54.00	177.0
54.80	339.0
56.00	1579.0
57.00	3006.0
57.90	107.0
60.00	1115.0
61.00	6019.0
62.00	5890.0
63.00	5260.0
64.10	1225.0
65.10	1397.0
66.10	239.0
67.00	361.0
68.00	11599.0
69.00	11915.0
70.00	921.0
72.00	759.0
73.00	5558.0
74.00	20144.0
75.10	62480.0
76.10	6102.0
77.10	662.0
77.90	692.0
78.90	4591.0
79.90	1264.0
80.90	4592.0
81.90	1114.0
82.90	153.0
85.90	232.0
87.00	5830.0
88.00	4857.0
91.00	458.0
92.00	3596.0
93.00	5246.0
94.10	14114.0
95.00	125632.0
96.00	8580.0
97.10	250.0
103.90	416.0
104.90	179.0
106.00	600.0
107.90	122.0
115.10	140.0
116.00	310.0
117.00	906.0
117.80	497.0
119.00	797.0
128.00	387.0
128.90	240.0
129.90	499.0
130.90	195.0
134.90	196.0
136.80	218.0
140.90	978.0
142.00	140.0
143.00	1945.0
143.90	190.0
144.90	1029.0
145.80	182.0
147.90	232.0
150.00	119.0
154.90	275.0
156.90	211.0
158.90	117.0
160.90	187.0
170.90	355.0
172.00	1965.0
173.00	1176.0
174.00	97408.0
175.00	7043.0
176.00	93296.0
177.00	6231.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	891.0
37.00	5846.0
38.00	5023.0
39.00	2496.0
40.00	1024.0
44.00	1257.0
45.10	830.0
45.90	259.0
47.00	1491.0
47.90	796.0
49.00	5060.0
50.00	23200.0
51.00	6957.0
52.00	434.0
52.90	212.0
54.00	185.0
54.80	290.0
56.00	1666.0
57.00	3207.0
57.90	108.0
60.00	1195.0
61.10	6508.0
62.00	6035.0
63.00	5570.0
64.00	1371.0
65.10	1555.0
66.20	253.0
66.90	412.0
68.00	12376.0
69.00	12815.0
70.00	870.0
72.00	906.0
73.00	6235.0
74.00	21200.0
75.10	66976.0
76.10	6074.0
77.10	725.0
77.90	596.0
79.00	4839.0
79.90	1494.0
81.00	5204.0
81.90	1195.0
82.90	176.0
85.90	259.0
87.00	5922.0
88.00	5478.0
90.90	467.0
92.00	3726.0
93.00	5749.0
94.10	14931.0
95.00	135040.0
96.00	8695.0
97.10	215.0
103.90	452.0
104.90	173.0
106.00	618.0
106.90	118.0
107.80	123.0
109.90	111.0
115.10	128.0
116.00	297.0
117.00	988.0
117.90	501.0
119.00	810.0
128.00	406.0
128.90	246.0
129.90	498.0
130.90	223.0
134.90	209.0
136.80	232.0
141.00	1087.0
141.90	165.0
143.00	2286.0
143.90	193.0
145.00	960.0
145.90	158.0
147.90	298.0
150.00	138.0
154.90	322.0
156.90	207.0
160.80	195.0
170.90	414.0
172.00	2148.0
173.00	1369.0
174.00	107800.0
175.00	7867.0
176.00	103008.0
177.00	6845.0
177.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	907.0
37.00	5442.0
38.00	4939.0
39.00	2397.0
40.00	1001.0
44.00	1172.0
45.10	778.0
45.90	203.0
47.00	1488.0
48.00	779.0
49.00	4779.0
50.00	22408.0
51.00	6817.0
51.90	456.0
53.00	199.0
54.00	143.0
54.90	243.0
56.00	1587.0
57.00	3148.0
58.00	116.0
60.00	1172.0
61.10	6244.0
62.00	5876.0
63.00	5147.0
64.00	1382.0
65.10	1728.0
66.10	221.0
66.90	417.0
68.00	11851.0
69.00	12645.0
70.00	821.0
72.00	887.0
73.00	6444.0
74.00	20680.0
75.00	65648.0
76.10	5311.0
77.00	770.0
77.90	406.0
79.00	4766.0
79.90	1628.0
81.00	5360.0
81.90	1235.0
83.00	152.0
85.90	216.0
87.00	5684.0
88.00	5595.0
90.90	521.0
92.00	3526.0
93.00	5744.0
94.00	14286.0
95.10	132288.0
96.10	8411.0
97.10	196.0
103.90	485.0
104.90	176.0
105.90	539.0
106.90	103.0
109.80	107.0
112.80	120.0
115.80	311.0
116.90	971.0
117.90	450.0
118.90	821.0
127.90	399.0
128.90	165.0
130.00	413.0
130.90	210.0
134.90	176.0
136.80	226.0
141.00	1049.0
141.90	154.0
143.00	2323.0
143.90	120.0
145.00	893.0
145.90	137.0
147.00	102.0
147.90	265.0
149.90	128.0
152.90	107.0
154.90	305.0
156.90	217.0
158.80	119.0
160.80	173.0
170.90	385.0
172.00	2198.0
173.00	1392.0
174.00	108704.0
175.00	7778.0
176.00	103200.0
177.00	6685.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157