

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055901.D
 Acq On : 26 Oct 2023 13:06
 Operator : MD/SY
 Sample : 04952-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 27 02:51:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 27 02:48:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	558175	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	562115	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	292203	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	225253	44.991	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.980%
7) Chloroethane-d5	1.895	69	185365	45.294	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.580%
11) 1,1-Dichloroethene-d2	2.560	63	305822	34.258	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.520%
21) 2-Butanone-d5	4.615	46	270815	73.000	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	73.000%
24) Chloroform-d	5.058	84	404501	42.144	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.280%
26) 1,2-Dichloroethane-d4	5.695	65	260479	44.091	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.180%
32) Benzene-d6	5.721	84	862653	47.965	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.920%
36) 1,2-Dichloropropane-d6	6.685	67	273155	47.975	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.940%
41) Toluene-d8	7.894	98	765384	47.130	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.260%
43) trans-1,3-Dichloroprop...	8.177	79	122233	44.691	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.380%
47) 2-Hexanone-d5	8.631	63	240348	107.377	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.380%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	417059	47.588	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.180%
66) 1,2-Dichlorobenzene-d4	12.190	152	313417	54.050	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.100%
Target Compounds						
					Qvalue	
8) Chloroethane	1.837	64	20522	6.465	ug/L #	53
25) Chloroform	5.081	83	8749	1.009	ug/L	91
51) Chlorobenzene	9.444	112	67620	5.574	ug/L	92
63) 1,2,4-Trimethylbenzene	11.467	105	18276	1.254	ug/L	99
67) 1,2-Dichlorobenzene	12.209	146	9126	1.021	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055901.D
Acq On : 26 Oct 2023 13:06
Operator : MD/SY
Sample : 04952-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Oct 27 02:51:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 27 02:48:43 2023
Response via : Initial Calibration




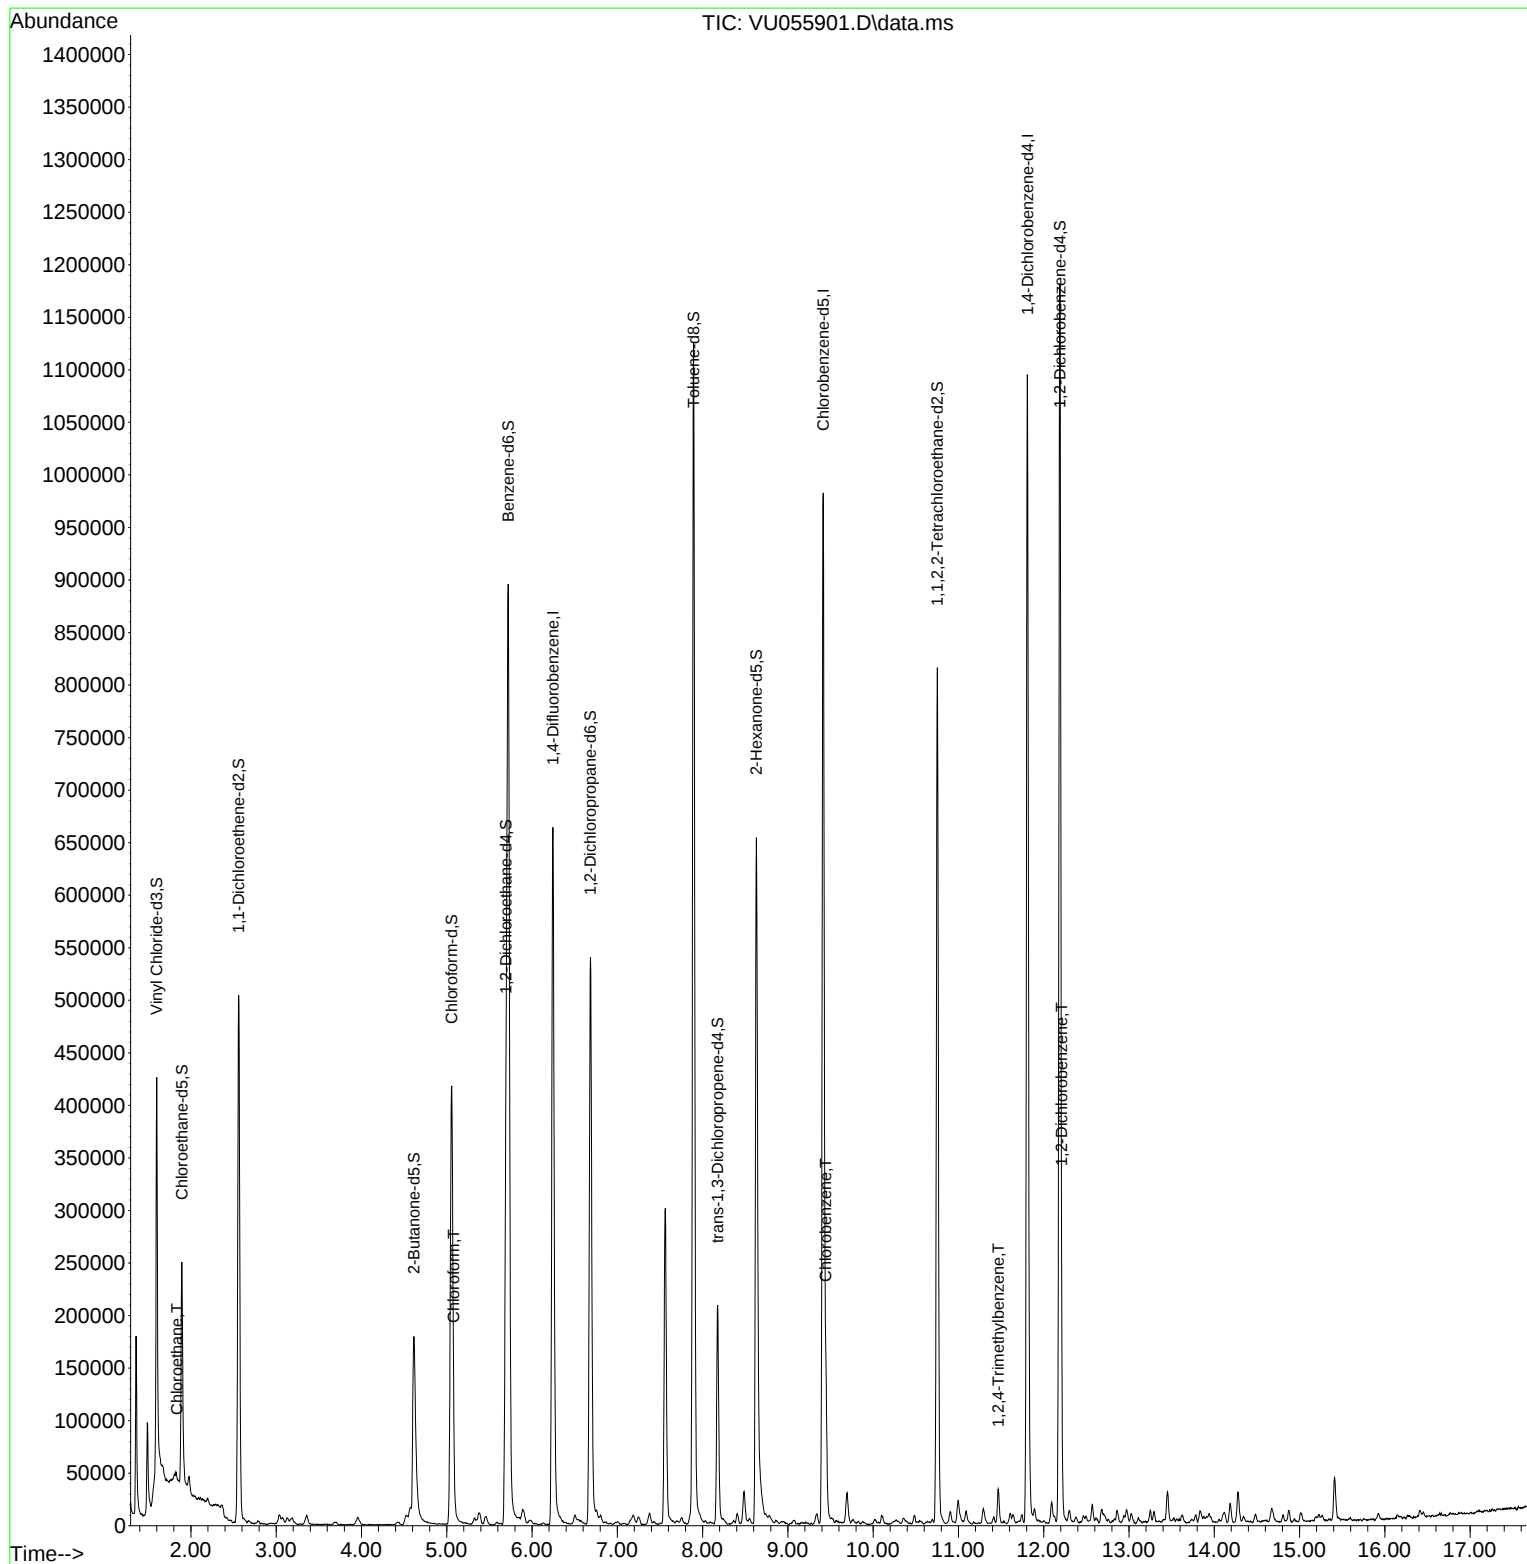


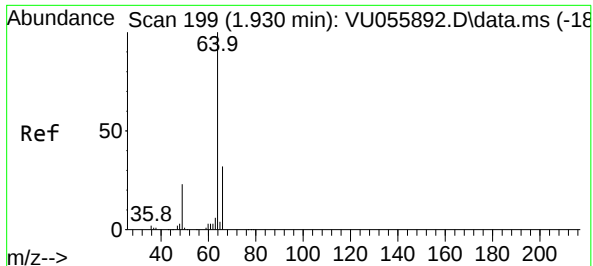

#8
Chloroethane
Concen: 6.465 ug/L
RT: 1.837 min Scan# 1179
Delta R.T. -0.093 min
Lab File: VU055901.D
Acq: 26 Oct 2023 13:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 64 Resp: 20522
Ion Ratio Lower Upper
64 100
66 6.3 22.9 42.5#

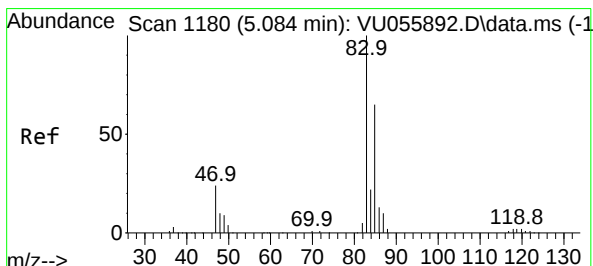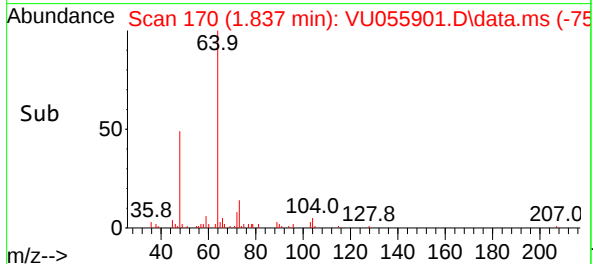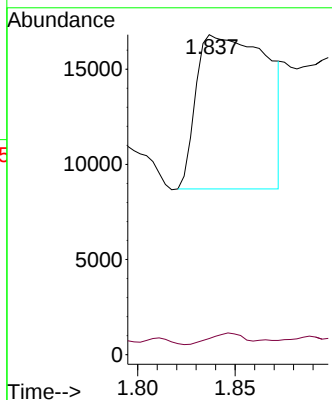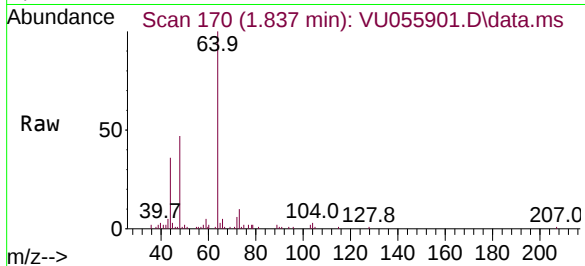

#25
Chloroform
Concen: 1.009 ug/L
RT: 5.081 min Scan# 1179
Delta R.T. -0.003 min
Lab File: VU055901.D
Acq: 26 Oct 2023 13:06

Tgt Ion: 83 Resp: 8749
Ion Ratio Lower Upper
83 100
85 73.4 46.3 86.1


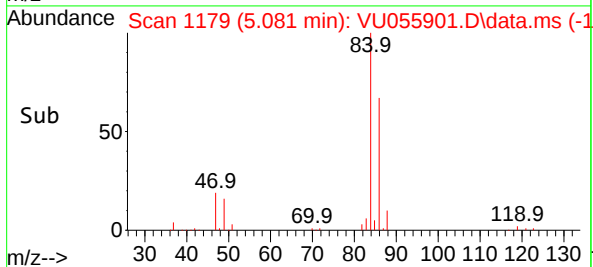
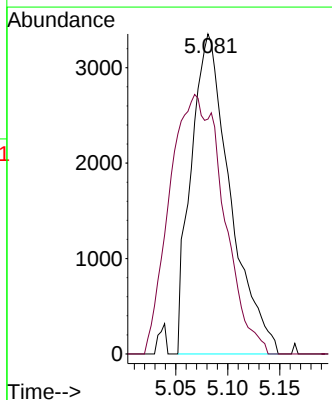
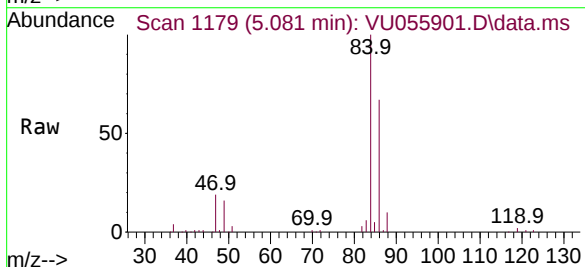


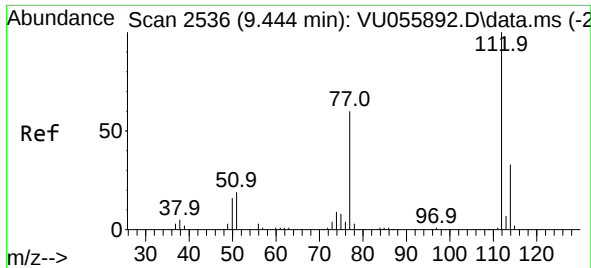

#51
Chlorobenzene
Concen: 5.574 ug/L
RT: 9.444 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU055901.D
Acq: 26 Oct 2023 13:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:112 Resp: 67620
Ion Ratio Lower Upper
112 100
114 39.1 22.0 40.8
77 65.5 49.0 73.6

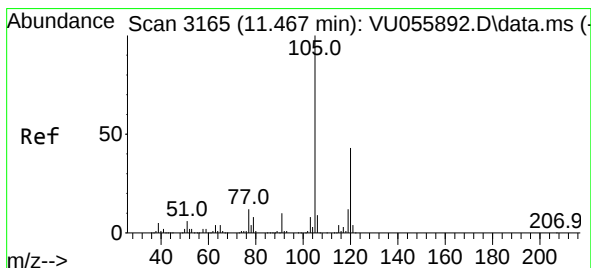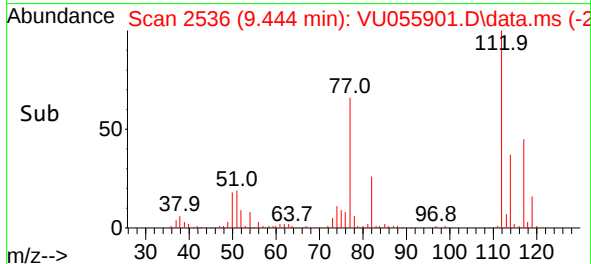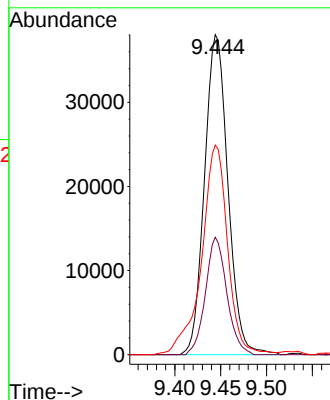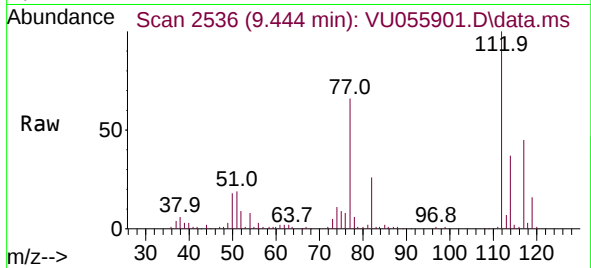

#63
1,2,4-Trimethylbenzene
Concen: 1.254 ug/L
RT: 11.467 min Scan# 3165
Delta R.T. -0.000 min
Lab File: VU055901.D
Acq: 26 Oct 2023 13:06

Tgt Ion:105 Resp: 18276
Ion Ratio Lower Upper
105 100
120 42.8 35.0 52.4

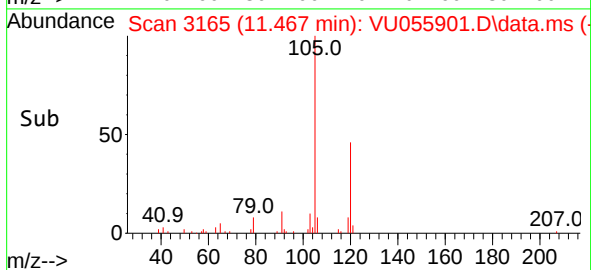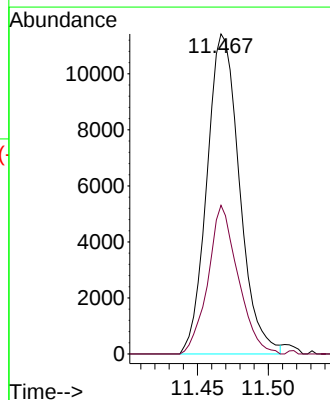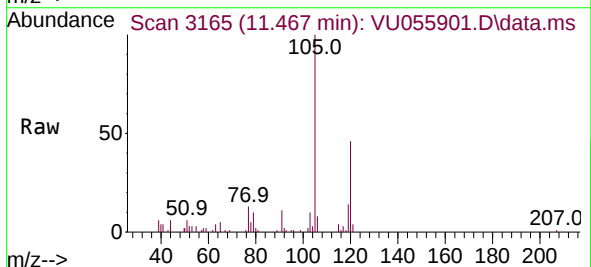

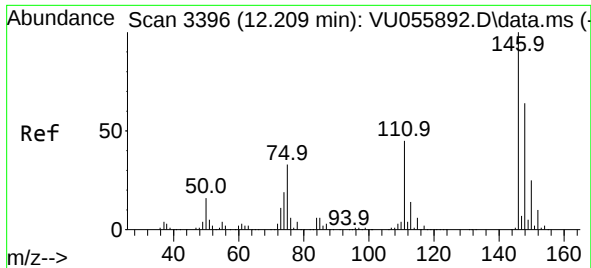

#67

1,2-Dichlorobenzene

Concen: 1.021 ug/L

RT: 12.209 min Scan# 31

Delta R.T. -0.000 min


Lab File: VU055901.D

Acq: 26 Oct 2023 13:06

Instrument :

MSVOA_U

ClientSampleId :

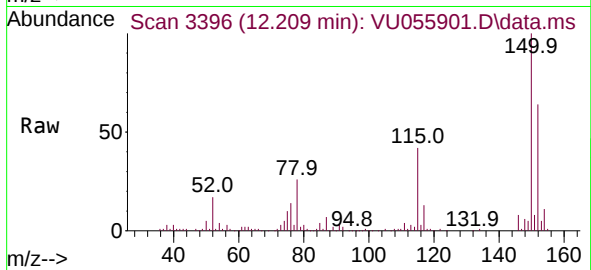

Tgt Ion:146 Resp: 9126

Ion Ratio Lower Upper

146 100

111 52.9 35.2 52.8#

148 74.0 52.3 78.5

