

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055908.D
 Acq On : 26 Oct 2023 16:25
 Operator : MD/SY
 Sample : 04952-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	53	60	67	rBV2	14524	28103	1.17%	0.150%
2	1.599	88	96	113	rBV	288864	338174	14.11%	1.810%
3	1.878	177	183	206	rVB	207606	323532	13.49%	1.732%
4	2.557	381	394	412	rBV	485563	793786	33.11%	4.249%
5	2.791	456	467	473	rBV4	2165	3785	0.16%	0.020%
6	2.955	514	518	522	rVV4	772	699	0.03%	0.004%
7	3.039	530	544	553	rBV6	4949	9651	0.40%	0.052%
8	3.177	575	587	596	rBV2	4091	8998	0.38%	0.048%
9	3.238	603	606	611	rVB3	534	430	0.02%	0.002%
10	3.296	621	624	628	rBV2	423	333	0.01%	0.002%
11	3.345	634	639	643	rBV3	682	577	0.02%	0.003%
12	3.525	692	695	701	rVV2	330	330	0.01%	0.002%
13	3.557	702	705	710	rVV2	342	369	0.02%	0.002%
14	3.656	732	736	739	rBV2	483	445	0.02%	0.002%
15	3.679	739	743	744	rVV2	511	317	0.01%	0.002%
16	3.689	744	746	750	rVB3	519	393	0.02%	0.002%
17	3.814	780	785	786	rBV	559	408	0.02%	0.002%
18	4.226	909	913	916	rBV2	373	346	0.01%	0.002%
19	4.261	921	924	927	rVB3	468	315	0.01%	0.002%
20	4.280	927	930	935	rBV2	428	443	0.02%	0.002%
21	4.325	935	944	948	rVB3	506	682	0.03%	0.004%
22	4.357	948	954	958	rBV3	444	464	0.02%	0.002%
23	4.383	958	962	964	rBV3	463	279	0.01%	0.001%
24	4.460	983	986	989	rBV2	408	300	0.01%	0.002%
25	4.615	1023	1034	1063	rBV	187938	479919	20.02%	2.569%
26	5.055	1153	1171	1199	rBV	405563	936681	39.07%	5.014%
27	5.222	1221	1223	1235	rVB5	1437	1873	0.08%	0.010%
28	5.274	1235	1239	1243	rVV2	660	615	0.03%	0.003%
29	5.332	1243	1257	1272	rVB6	4344	11544	0.48%	0.062%
30	5.717	1354	1377	1399	rBV2	890149	2397508	100.00%	12.835%
31	5.971	1452	1456	1460	rBV2	1120	1065	0.04%	0.006%
32	6.245	1527	1541	1579	rBV	665528	1304554	54.41%	6.984%
33	6.528	1619	1629	1640	rBV9	4421	8909	0.37%	0.048%
34	6.592	1645	1649	1651	rBV4	971	866	0.04%	0.005%
35	6.685	1662	1678	1702	rBV	532828	1057316	44.10%	5.660%
36	6.946	1754	1759	1762	rBV3	422	392	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055908.D
 Acq On : 26 Oct 2023 16:25
 Operator : MD/SY
 Sample : 04952-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.100	1802	1807	1815	rBV3	665	972	0.04%	0.005%
38	7.190	1820	1835	1840	rBV5	6241	11625	0.48%	0.062%
39	7.241	1849	1851	1859	rVB6	955	850	0.04%	0.005%
40	7.286	1861	1865	1869	rBV	423	387	0.02%	0.002%
41	7.306	1869	1871	1876	rVB2	382	351	0.01%	0.002%
42	7.489	1920	1928	1932	rBV	480	529	0.02%	0.003%
43	7.560	1938	1950	1967	rBV	285955	515284	21.49%	2.758%
44	7.695	1986	1992	2009	rVB7	3058	6896	0.29%	0.037%
45	7.759	2009	2012	2014	rBV	512	285	0.01%	0.002%
46	7.807	2025	2027	2035	rVB5	514	478	0.02%	0.003%
47	7.894	2035	2054	2078	rBV	1104328	1908748	79.61%	10.218%
48	8.177	2130	2142	2158	rBV	205469	355839	14.84%	1.905%
49	8.357	2191	2198	2204	rBV4	777	989	0.04%	0.005%
50	8.447	2223	2226	2227	rBV3	847	543	0.02%	0.003%
51	8.466	2230	2232	2236	rVB3	979	532	0.02%	0.003%
52	8.505	2240	2244	2245	rBV3	530	403	0.02%	0.002%
53	8.550	2249	2258	2271	rVB2	19124	35206	1.47%	0.188%
54	8.634	2271	2284	2313	rBV	718888	1369618	57.13%	7.332%
55	9.065	2416	2418	2421	rVB	698	316	0.01%	0.002%
56	9.155	2442	2446	2448	rBV2	519	368	0.02%	0.002%
57	9.164	2448	2449	2452	rVV	600	278	0.01%	0.001%
58	9.196	2458	2459	2464	rVB	519	298	0.01%	0.002%
59	9.338	2496	2503	2509	rBV3	699	869	0.04%	0.005%
60	9.415	2514	2527	2554	rBV	977595	1660465	69.26%	8.889%
61	9.605	2583	2586	2592	rVB4	621	411	0.02%	0.002%
62	9.663	2600	2604	2608	rVB3	672	405	0.02%	0.002%
63	9.698	2608	2615	2618	rBV4	1169	1347	0.06%	0.007%
64	9.749	2629	2631	2635	rVV3	648	422	0.02%	0.002%
65	9.772	2635	2638	2642	rVB	593	472	0.02%	0.003%
66	10.029	2716	2718	2723	rVB2	574	451	0.02%	0.002%
67	10.061	2724	2728	2733	rVB3	523	345	0.01%	0.002%
68	10.097	2734	2739	2741	rBV3	344	305	0.01%	0.002%
69	10.116	2741	2745	2748	rBV3	562	334	0.01%	0.002%
70	10.190	2764	2768	2770	rBV3	631	506	0.02%	0.003%
71	10.228	2777	2780	2784	rBV2	500	374	0.02%	0.002%
72	10.309	2803	2805	2809	rVB	485	338	0.01%	0.002%
73	10.360	2819	2821	2824	rVV	499	303	0.01%	0.002%
74	10.412	2830	2837	2839	rBV	331	360	0.02%	0.002%
75	10.566	2882	2885	2890	rVV2	451	370	0.02%	0.002%
76	10.646	2906	2910	2912	rVB2	651	399	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055908.D
 Acq On : 26 Oct 2023 16:25
 Operator : MD/SY
 Sample : 04952-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	10.685	2917	2922	2925	rBV2	374	314	0.01%	0.002%
78	10.753	2930	2943	2967	rBV	839041	1390742	58.01%	7.445%
79	10.897	2981	2988	2995	rBV5	1201	1820	0.08%	0.010%
80	11.119	3054	3057	3059	rVB2	601	304	0.01%	0.002%
81	11.174	3069	3074	3078	rBV2	570	674	0.03%	0.004%
82	11.415	3146	3149	3151	rBV2	1018	744	0.03%	0.004%
83	11.666	3224	3227	3231	rVV2	574	359	0.01%	0.002%
84	11.730	3240	3247	3248	rBV2	1104	1319	0.06%	0.007%
85	11.810	3258	3272	3298	rBV	1087553	1776492	74.10%	9.510%
86	12.100	3360	3362	3365	rVB2	686	352	0.01%	0.002%
87	12.190	3377	3390	3412	rBV	1153936	1902705	79.36%	10.186%
88	12.405	3455	3457	3460	rBV2	600	302	0.01%	0.002%
89	12.508	3487	3489	3493	rVB2	792	537	0.02%	0.003%
90	12.621	3520	3524	3526	rBV2	551	383	0.02%	0.002%
91	12.936	3620	3622	3624	rBV2	575	319	0.01%	0.002%
92	13.058	3658	3660	3663	rBV2	509	290	0.01%	0.002%
93	13.344	3746	3749	3752	rBV2	723	513	0.02%	0.003%
94	13.437	3772	3778	3783	rBV6	832	1265	0.05%	0.007%
95	13.585	3821	3824	3829	rBV4	790	741	0.03%	0.004%
96	13.640	3836	3841	3843	rBV2	641	623	0.03%	0.003%
97	14.068	3971	3974	3978	rVB4	804	516	0.02%	0.003%
98	14.122	3987	3991	3993	rBV3	1142	940	0.04%	0.005%
99	14.450	4089	4093	4101	rVB7	3379	3382	0.14%	0.018%
100	14.971	4253	4255	4258	rBV2	1038	568	0.02%	0.003%




Sum of corrected areas: 18679876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055908.D
Acq On : 26 Oct 2023 16:25
Operator : MD/SY
Sample : 04952-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

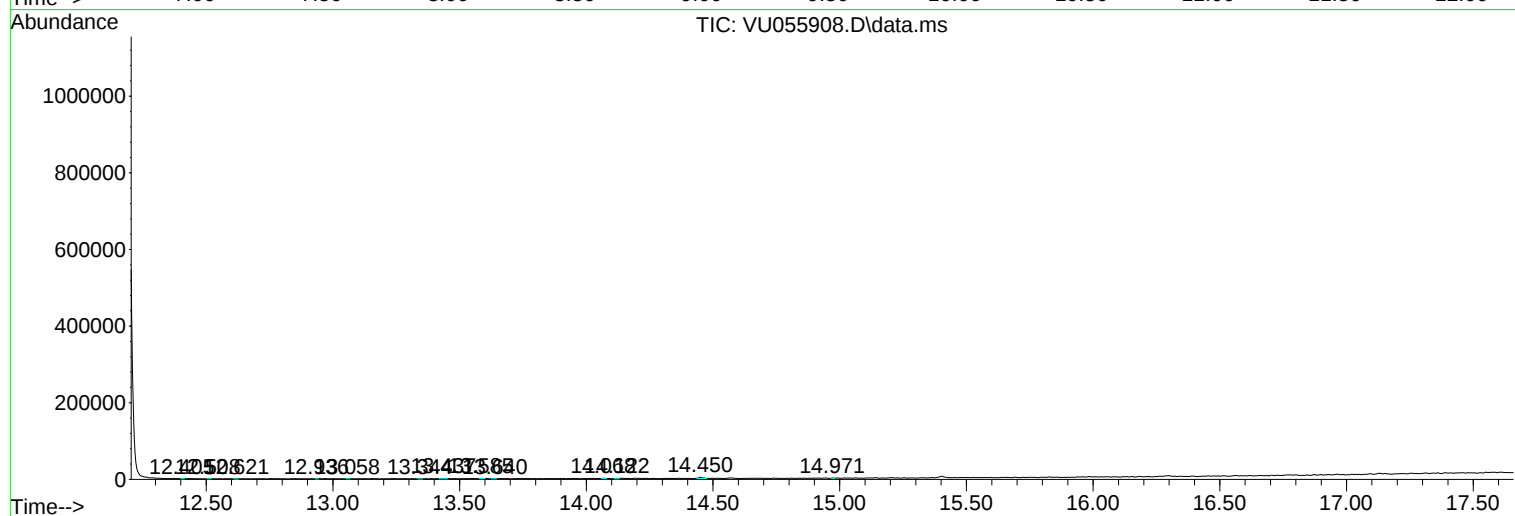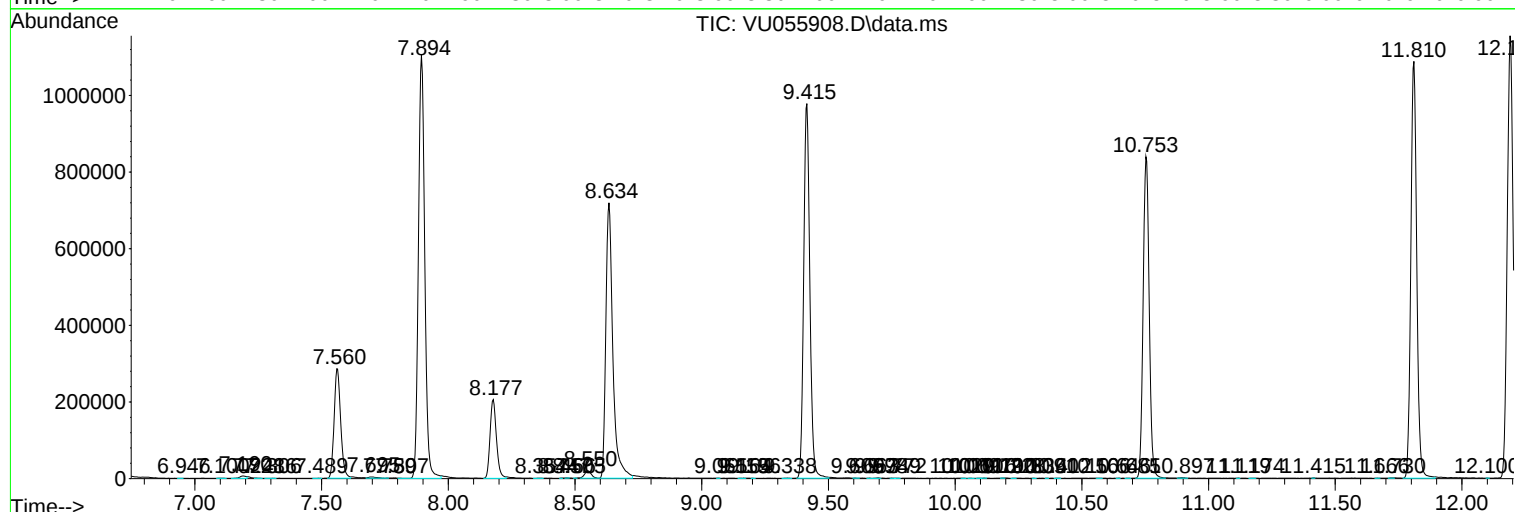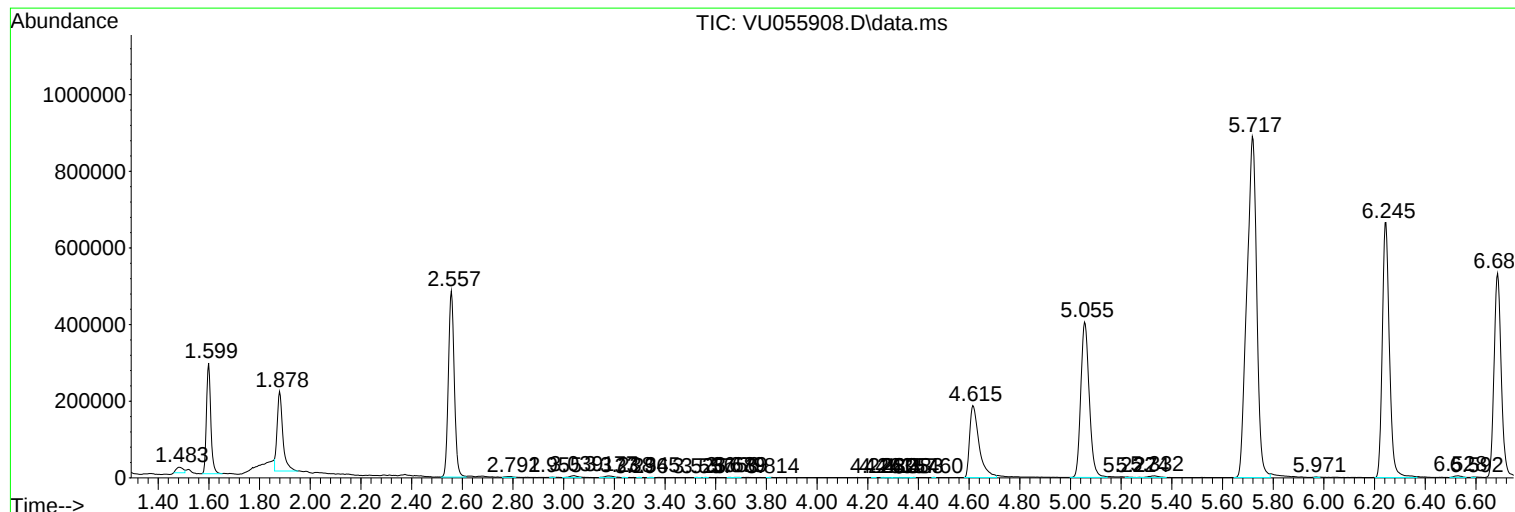

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055908.D
Acq On : 26 Oct 2023 16:25
Operator : MD/SY
Sample : 04952-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055908.D
Acq On : 26 Oct 2023 16:25
Operator : MD/SY
Sample : 04952-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------