

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055910.D
 Acq On : 26 Oct 2023 17:11
 Operator : MD/SY
 Sample : VIBLK037
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	111	rVB	271799	311299	13.55%	1.745%
2	1.888	180	186	204	rVB	191171	279099	12.15%	1.565%
3	2.557	383	394	413	rBV	459335	753081	32.77%	4.223%
4	2.833	478	480	483	rBV	444	262	0.01%	0.001%
5	2.917	503	506	509	rBV3	410	228	0.01%	0.001%
6	3.039	533	544	559	rVB4	6825	14948	0.65%	0.084%
7	3.319	628	631	634	rBV2	438	363	0.02%	0.002%
8	3.348	638	640	646	rVB3	690	601	0.03%	0.003%
9	3.447	669	671	673	rVB	206	54	0.00%	0.000%
10	3.467	673	677	681	rBV2	532	539	0.02%	0.003%
11	3.547	698	702	706	rBV3	542	454	0.02%	0.003%
12	3.563	706	707	708	rBV	377	106	0.00%	0.001%
13	3.595	715	717	718	rBV2	227	109	0.00%	0.001%
14	3.653	731	735	736	rBV2	431	278	0.01%	0.002%
15	3.737	759	761	764	rBV2	184	105	0.00%	0.001%
16	3.772	771	772	774	rBV	393	92	0.00%	0.001%
17	3.795	774	779	782	rVV2	405	374	0.02%	0.002%
18	3.817	782	786	788	rVV	440	333	0.01%	0.002%
19	3.833	788	791	797	rVB2	421	406	0.02%	0.002%
20	3.862	797	800	802	rBV	158	86	0.00%	0.000%
21	3.907	810	814	819	rBV2	299	289	0.01%	0.002%
22	3.962	828	831	832	rBV	353	156	0.01%	0.001%
23	4.001	839	843	847	rBV	287	274	0.01%	0.002%
24	4.036	851	854	855	rBV	366	173	0.01%	0.001%
25	4.065	861	863	866	rVB2	349	156	0.01%	0.001%
26	4.116	878	879	880	rBV2	208	57	0.00%	0.000%
27	4.181	894	899	900	rBV2	502	351	0.02%	0.002%
28	4.226	909	913	914	rBV	338	230	0.01%	0.001%
29	4.267	923	926	927	rBV	244	134	0.01%	0.001%
30	4.277	927	929	932	rVB2	511	219	0.01%	0.001%
31	4.319	938	942	946	rBV	364	298	0.01%	0.002%
32	4.367	955	957	958	rBV	274	98	0.00%	0.001%
33	4.409	967	970	976	rBV3	245	262	0.01%	0.001%
34	4.435	976	978	980	rVB	398	154	0.01%	0.001%
35	4.451	980	983	985	rBV	659	238	0.01%	0.001%
36	4.489	991	995	998	rBV	351	284	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055910.D
 Acq On : 26 Oct 2023 17:11
 Operator : MD/SY
 Sample : VIBLK037
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	4.505	998	1000	1003	rVB	439	205	0.01%	0.001%
38	4.528	1004	1007	1008	rBV	315	175	0.01%	0.001%
39	4.576	1021	1022	1023	rBV	97	36	0.00%	0.000%
40	4.615	1023	1034	1072	rBV	193259	500794	21.79%	2.808%
41	5.055	1156	1171	1197	rBV	394301	899927	39.16%	5.046%
42	5.287	1240	1243	1244	rBV2	771	438	0.02%	0.002%
43	5.460	1293	1297	1299	rBV2	360	258	0.01%	0.001%
44	5.486	1302	1305	1307	rVV3	293	177	0.01%	0.001%
45	5.496	1307	1308	1310	rVB	198	52	0.00%	0.000%
46	5.541	1319	1322	1324	rBV	306	203	0.01%	0.001%
47	5.557	1324	1327	1330	rVV2	336	235	0.01%	0.001%
48	5.602	1336	1341	1343	rBV2	378	336	0.01%	0.002%
49	5.644	1351	1354	1356	rBV2	258	181	0.01%	0.001%
50	5.717	1356	1377	1405	rBV2	833486	2297786	100.00%	12.884%
51	6.090	1491	1493	1494	rVB2	214	47	0.00%	0.000%
52	6.103	1494	1497	1500	rBV2	837	613	0.03%	0.003%
53	6.148	1507	1511	1515	rBV3	320	333	0.01%	0.002%
54	6.245	1528	1541	1565	rBV	639955	1241043	54.01%	6.959%
55	6.528	1619	1629	1639	rVB9	4159	8670	0.38%	0.049%
56	6.592	1646	1649	1652	rBV3	1131	849	0.04%	0.005%
57	6.685	1664	1678	1701	rBV	516282	1022952	44.52%	5.736%
58	6.946	1756	1759	1760	rBV	262	114	0.00%	0.001%
59	6.962	1762	1764	1767	rBV	275	210	0.01%	0.001%
60	7.004	1774	1777	1780	rVB2	604	330	0.01%	0.002%
61	7.068	1794	1797	1800	rVB	300	149	0.01%	0.001%
62	7.084	1800	1802	1804	rBV2	151	75	0.00%	0.000%
63	7.139	1817	1819	1821	rBV	200	83	0.00%	0.000%
64	7.190	1821	1835	1847	rBV5	5315	12878	0.56%	0.072%
65	7.270	1855	1860	1864	rBV3	610	538	0.02%	0.003%
66	7.354	1885	1886	1887	rBV	412	137	0.01%	0.001%
67	7.489	1923	1928	1932	rBV2	729	694	0.03%	0.004%
68	7.563	1938	1951	1972	rBV	276230	502745	21.88%	2.819%
69	7.894	2041	2054	2081	rBV	1029422	1834089	79.82%	10.284%
70	8.177	2131	2142	2175	rVB	195703	342848	14.92%	1.922%
71	8.299	2175	2180	2183	rBV4	866	863	0.04%	0.005%
72	8.415	2213	2216	2217	rBV2	359	204	0.01%	0.001%
73	8.467	2225	2232	2237	rBV5	1156	1474	0.06%	0.008%
74	8.550	2251	2258	2270	rVB8	4910	9308	0.41%	0.052%
75	8.631	2272	2283	2326	rBV	715418	1359312	59.16%	7.622%
76	9.087	2422	2425	2427	rBV	417	287	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
 Data File : VU055910.D
 Acq On : 26 Oct 2023 17:11
 Operator : MD/SY
 Sample : VIBLK037
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	9.119	2432	2435	2439	rBV2	512	468	0.02%	0.003%
78	9.177	2450	2453	2455	rBV	565	407	0.02%	0.002%
79	9.299	2489	2491	2492	rVB2	489	135	0.01%	0.001%
80	9.315	2492	2496	2501	rVB2	643	507	0.02%	0.003%
81	9.341	2501	2504	2508	rBV2	1153	719	0.03%	0.004%
82	9.367	2510	2512	2513	rBV	456	178	0.01%	0.001%
83	9.415	2514	2527	2560	rBV	917520	1583911	68.93%	8.881%
84	9.762	2633	2635	2638	rBV	380	180	0.01%	0.001%
85	9.791	2642	2644	2648	rVB2	715	429	0.02%	0.002%
86	9.913	2680	2682	2686	rVB2	533	292	0.01%	0.002%
87	9.987	2703	2705	2707	rBV	427	178	0.01%	0.001%
88	10.142	2751	2753	2754	rBV	307	117	0.01%	0.001%
89	10.155	2756	2757	2762	rVB2	578	376	0.02%	0.002%
90	10.286	2795	2798	2802	rBV2	385	355	0.02%	0.002%
91	10.328	2809	2811	2813	rBV	299	196	0.01%	0.001%
92	10.753	2930	2943	2970	rBV	834590	1358105	59.10%	7.615%
93	11.264	3099	3102	3103	rBV	359	201	0.01%	0.001%
94	11.807	3258	3271	3293	rBV	1022641	1674988	72.90%	9.392%
95	12.190	3376	3390	3418	rBV	1090296	1804628	78.54%	10.119%
96	12.656	3534	3535	3537	rVB	919	192	0.01%	0.001%




Sum of corrected areas: 17834400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055910.D
Acq On : 26 Oct 2023 17:11
Operator : MD/SY
Sample : VIBLK037
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

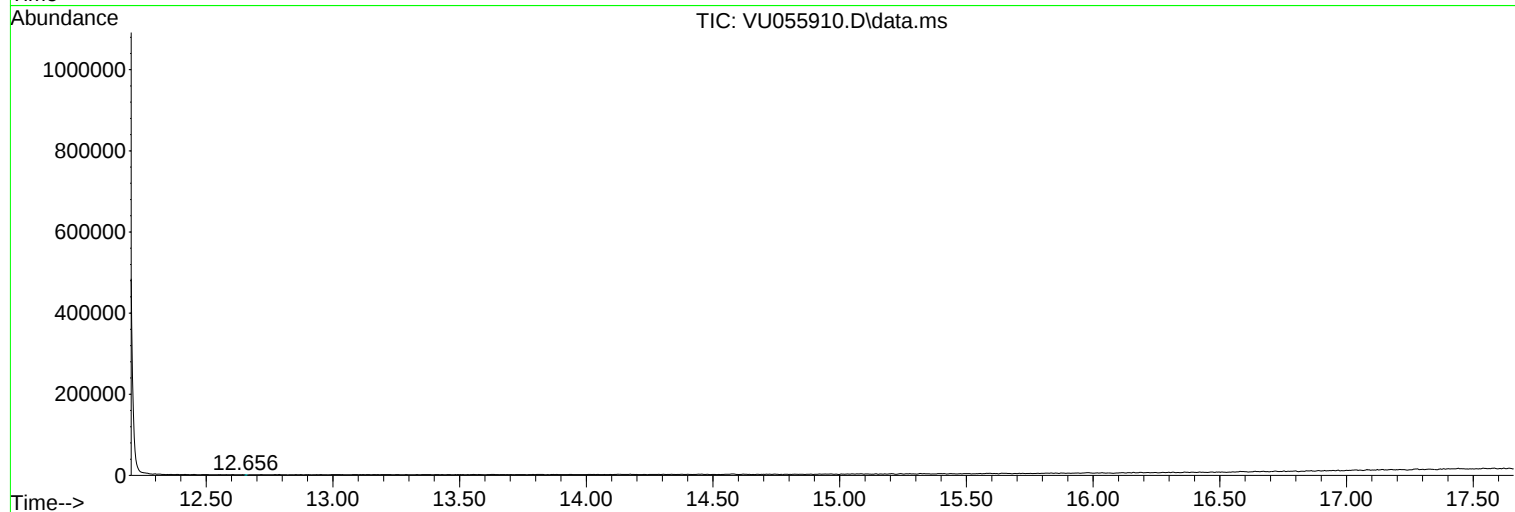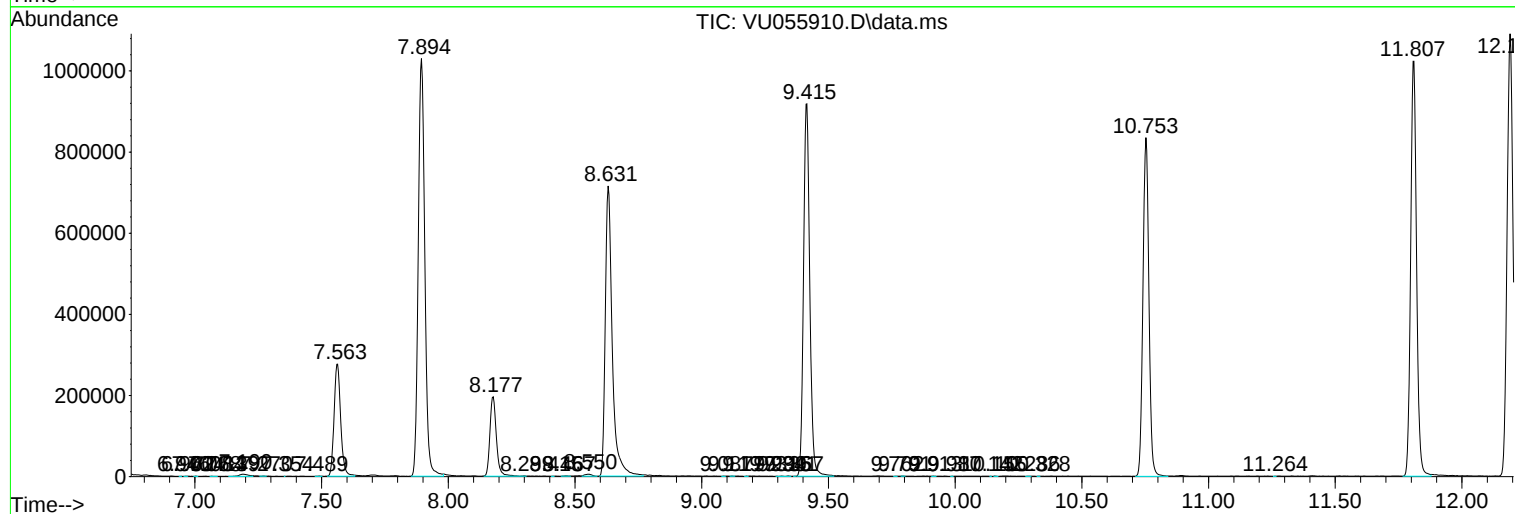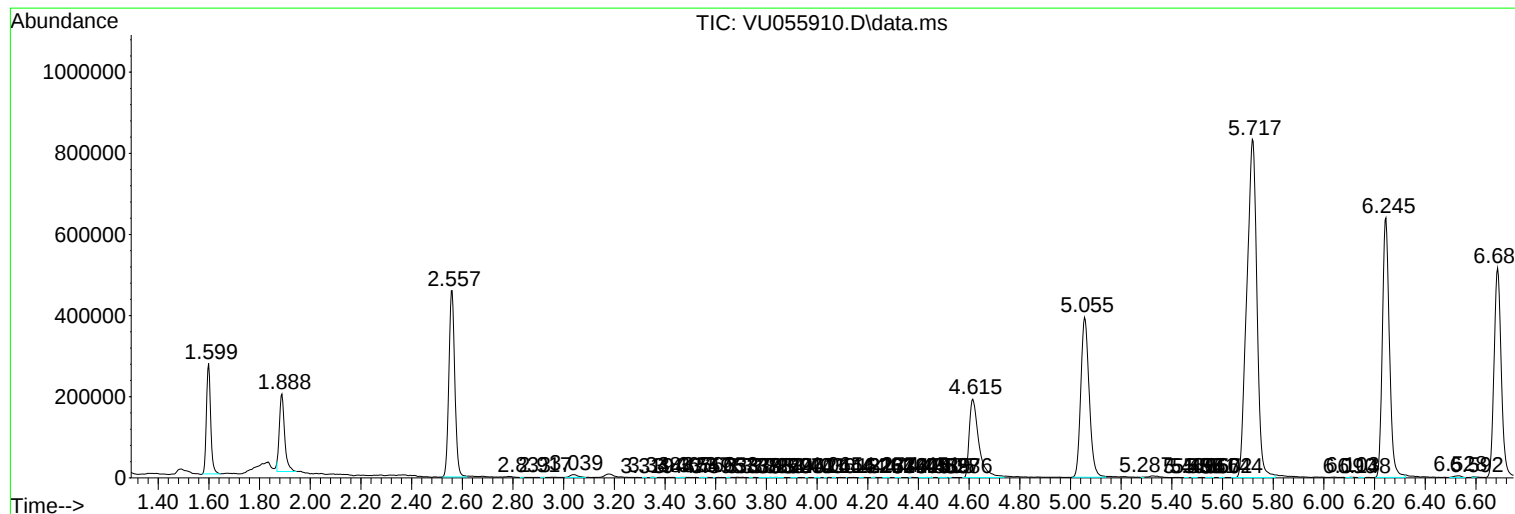

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055910.D
Acq On : 26 Oct 2023 17:11
Operator : MD/SY
Sample : VIBLK037
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055910.D
Acq On : 26 Oct 2023 17:11
Operator : MD/SY
Sample : VIBLK037
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------