
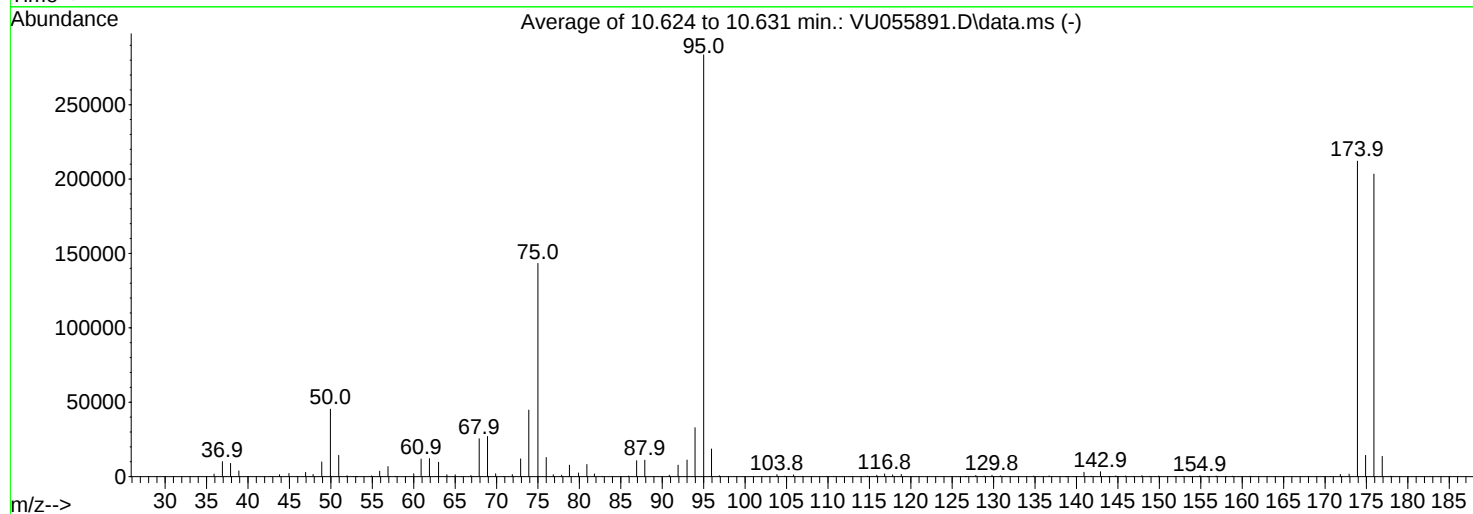


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102623\
Data File : VU055891.D
Acq On : 26 Oct 2023 08:37
Operator : MD/SY
Sample : BFB028
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB028

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Fri Oct 27 02:48:43 2023

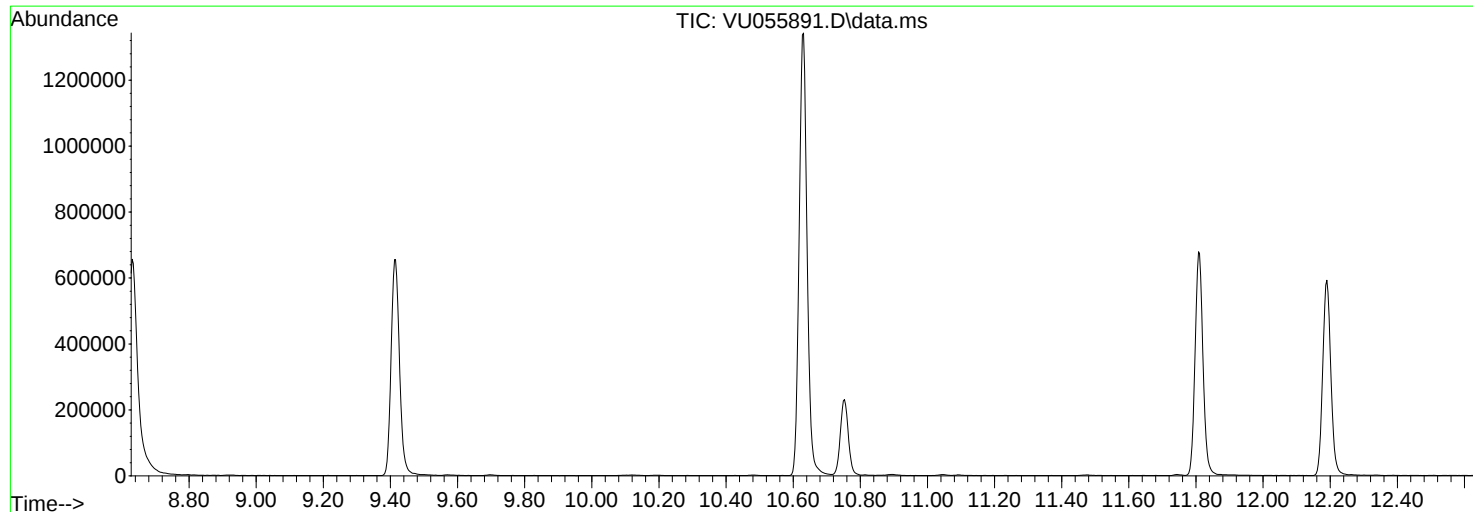

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	45365	PASS
75	95	30	80	50.6	143339	PASS
95	95	100	100	100.0	283520	PASS
96	95	5	9	6.5	18565	PASS
173	174	0.00	2	0.8	1737	PASS
174	95	50	120	74.8	212075	PASS
175	174	5	9	6.8	14339	PASS
176	174	95	101	95.9	203413	PASS
177	176	5	9	6.7	13692	PASS

m/z	Abundance
39.90	476.0
43.80	651.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1634.0
36.90	9613.0
37.90	8586.0
38.90	3647.0
40.00	352.0
42.70	181.0
43.90	1979.0
44.90	1919.0
45.90	285.0
46.90	2642.0
47.90	1262.0
48.90	9101.0
49.90	43072.0
51.00	13553.0
51.90	739.0
52.70	175.0
54.90	568.0
55.90	3235.0
56.90	6670.0
57.80	211.0
60.00	1852.0
60.90	11536.0
61.90	11174.0
63.00	9407.0
64.00	1306.0
65.00	1240.0
65.80	116.0
66.90	734.0
67.90	23616.0
68.90	25592.0
69.90	1739.0
70.80	118.0
71.90	1370.0
72.90	11085.0
73.90	42120.0
75.00	136064.0
76.00	12289.0
76.90	1248.0
78.00	938.0
78.80	7631.0
79.90	2449.0
80.90	8003.0
81.80	1625.0
82.70	194.0
86.00	586.0
86.90	9979.0
87.90	10797.0
90.90	941.0
91.90	7609.0
93.00	10714.0
93.90	30680.0
95.00	265536.0
95.90	18280.0
96.90	480.0
103.90	1285.0
104.90	324.0
105.90	1166.0
106.90	189.0
109.80	242.0
110.70	202.0
111.70	233.0
112.90	256.0
114.70	358.0
115.90	979.0
116.80	1520.0
117.80	1191.0
118.90	1483.0
127.80	799.0
128.80	426.0
129.80	936.0
130.80	542.0
134.80	370.0
136.70	471.0
139.90	152.0
140.90	2700.0
141.70	287.0
142.90	3114.0
143.80	153.0
144.80	514.0
145.90	390.0
146.90	203.0
147.90	633.0
148.90	202.0
149.90	363.0
151.90	190.0
152.90	179.0
153.80	207.0
154.90	691.0
156.90	358.0
158.80	262.0
161.00	296.0
170.70	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

171.90	1425.0
172.90	1656.0
173.90	193984.0
174.90	13554.0
175.90	185408.0
176.90	12749.0
178.00	387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1770.0
36.90	10351.0
37.90	9129.0
38.90	4070.0
40.00	396.0
42.80	190.0
43.90	1947.0
44.90	2248.0
45.90	259.0
47.00	2971.0
47.80	1475.0
48.90	10333.0
50.00	46528.0
51.00	14818.0
52.00	702.0
52.70	159.0
54.90	623.0
55.90	3725.0
56.90	6921.0
57.80	280.0
60.00	2054.0
60.90	12295.0
61.90	12492.0
63.00	9954.0
64.00	1379.0
65.00	1253.0
65.80	185.0
66.90	841.0
67.90	26072.0
68.90	27992.0
69.90	2009.0
70.90	120.0
71.90	1491.0
72.90	12294.0
73.90	46096.0
75.00	147840.0
76.00	13395.0
76.80	1402.0
77.80	1022.0
78.80	7960.0
79.90	2600.0
80.90	8410.0
81.80	1835.0
82.80	191.0
85.90	503.0
86.90	11081.0
87.90	11516.0
90.80	1052.0
91.90	8108.0
93.00	11804.0
94.00	34152.0
95.00	292608.0
96.00	19072.0
96.90	640.0
103.80	1421.0
104.80	313.0
105.80	1209.0
106.90	211.0
109.80	263.0
110.70	277.0
111.70	202.0
112.60	223.0
112.90	238.0
114.80	357.0
115.90	1004.0
116.90	1871.0
117.80	1306.0
118.90	1541.0
127.80	900.0
128.80	409.0
129.80	1020.0
130.80	556.0
134.80	399.0
136.70	616.0
138.70	115.0
139.60	176.0
140.90	2958.0
141.80	320.0
142.90	3391.0
143.80	126.0
144.70	565.0
145.90	433.0
146.90	297.0
147.90	659.0
148.80	218.0
149.90	424.0
151.90	170.0
152.90	186.0
153.70	159.0
154.90	757.0
156.80	427.0
158.80	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

160.90	297.0
170.60	134.0
171.80	1484.0
172.90	1747.0
173.90	218048.0
174.90	14689.0
175.90	209408.0
176.90	14174.0
177.90	312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1727.0
36.90	10278.0
37.90	9075.0
38.90	3976.0
40.00	387.0
42.80	145.0
43.80	1876.0
45.00	2355.0
46.00	242.0
47.00	3020.0
47.80	1718.0
48.90	10286.0
49.90	46496.0
50.90	14483.0
52.00	652.0
53.10	144.0
54.90	608.0
55.90	3920.0
56.90	6636.0
57.80	338.0
60.00	1981.0
60.90	11753.0
61.90	12793.0
63.00	9670.0
64.00	1340.0
65.00	1264.0
65.80	225.0
66.90	816.0
67.90	26672.0
68.90	27488.0
69.90	2042.0
70.90	111.0
71.90	1480.0
72.90	12295.0
73.90	46104.0
75.00	146112.0
76.00	13115.0
76.90	1417.0
77.80	922.0
78.80	7791.0
79.90	2535.0
80.90	8148.0
81.80	1934.0
82.80	153.0
85.90	393.0
86.90	11309.0
87.90	10965.0
90.80	1025.0
91.90	7658.0
93.00	11182.0
94.00	34008.0
95.00	292416.0
96.00	18344.0
96.90	715.0
103.80	1405.0
104.70	342.0
105.80	1108.0
107.00	232.0
109.90	222.0
110.70	268.0
111.70	123.0
112.70	241.0
114.80	306.0
115.90	1003.0
116.90	2032.0
117.80	1210.0
118.80	1421.0
126.60	111.0
127.90	1015.0
128.90	447.0
129.80	1018.0
130.80	456.0
134.90	458.0
136.70	600.0
139.60	163.0
140.90	3031.0
141.80	343.0
142.90	3423.0
143.90	126.0
144.70	498.0
145.90	414.0
146.90	353.0
147.90	558.0
148.80	182.0
149.90	388.0
151.80	116.0
152.90	170.0
153.70	128.0
154.90	672.0
155.80	128.0
156.80	480.0
158.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

158.80	309.0
160.90	335.0
170.60	109.0
171.80	1573.0
172.90	1809.0
173.90	224192.0
174.90	14774.0
175.90	215424.0
176.90	14152.0
177.90	274.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028