

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102720\
 Data File : VU040984.D
 Acq On : 27 Oct 2020 15:31
 Operator : SY/MD
 Sample : L4493-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ1

Quant Time: Oct 28 03:14:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 28 02:17:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	55869	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	57607	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	23418	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	23325	4.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.40%
7) Chloroethane-d5	1.92	69	18489	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.60%
11) 1,1-Dichloroethene-d2	2.58	63	34900	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	4.66	46	78502	50.79	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.58%
24) Chloroform-d	5.08	84	42253	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
26) 1,2-Dichloroethane-d4	5.72	65	26846	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
32) Benzene-d6	5.74	84	76470	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.70	67	26249	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	7.91	98	59081	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	8.19	79	9878	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.64	63	54766	46.78	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.56%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	22341	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	22835	5.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.20%


Target Compounds					Ovalue
47) Tetrachloroethene	8.56	164	1984	0.616 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102720\
Data File : VU040984.D
Acq On : 27 Oct 2020 15:31
Operator : SY/MD
Sample : L4493-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ1

Quant Time: Oct 28 03:14:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 28 02:17:39 2020
Response via : Initial Calibration

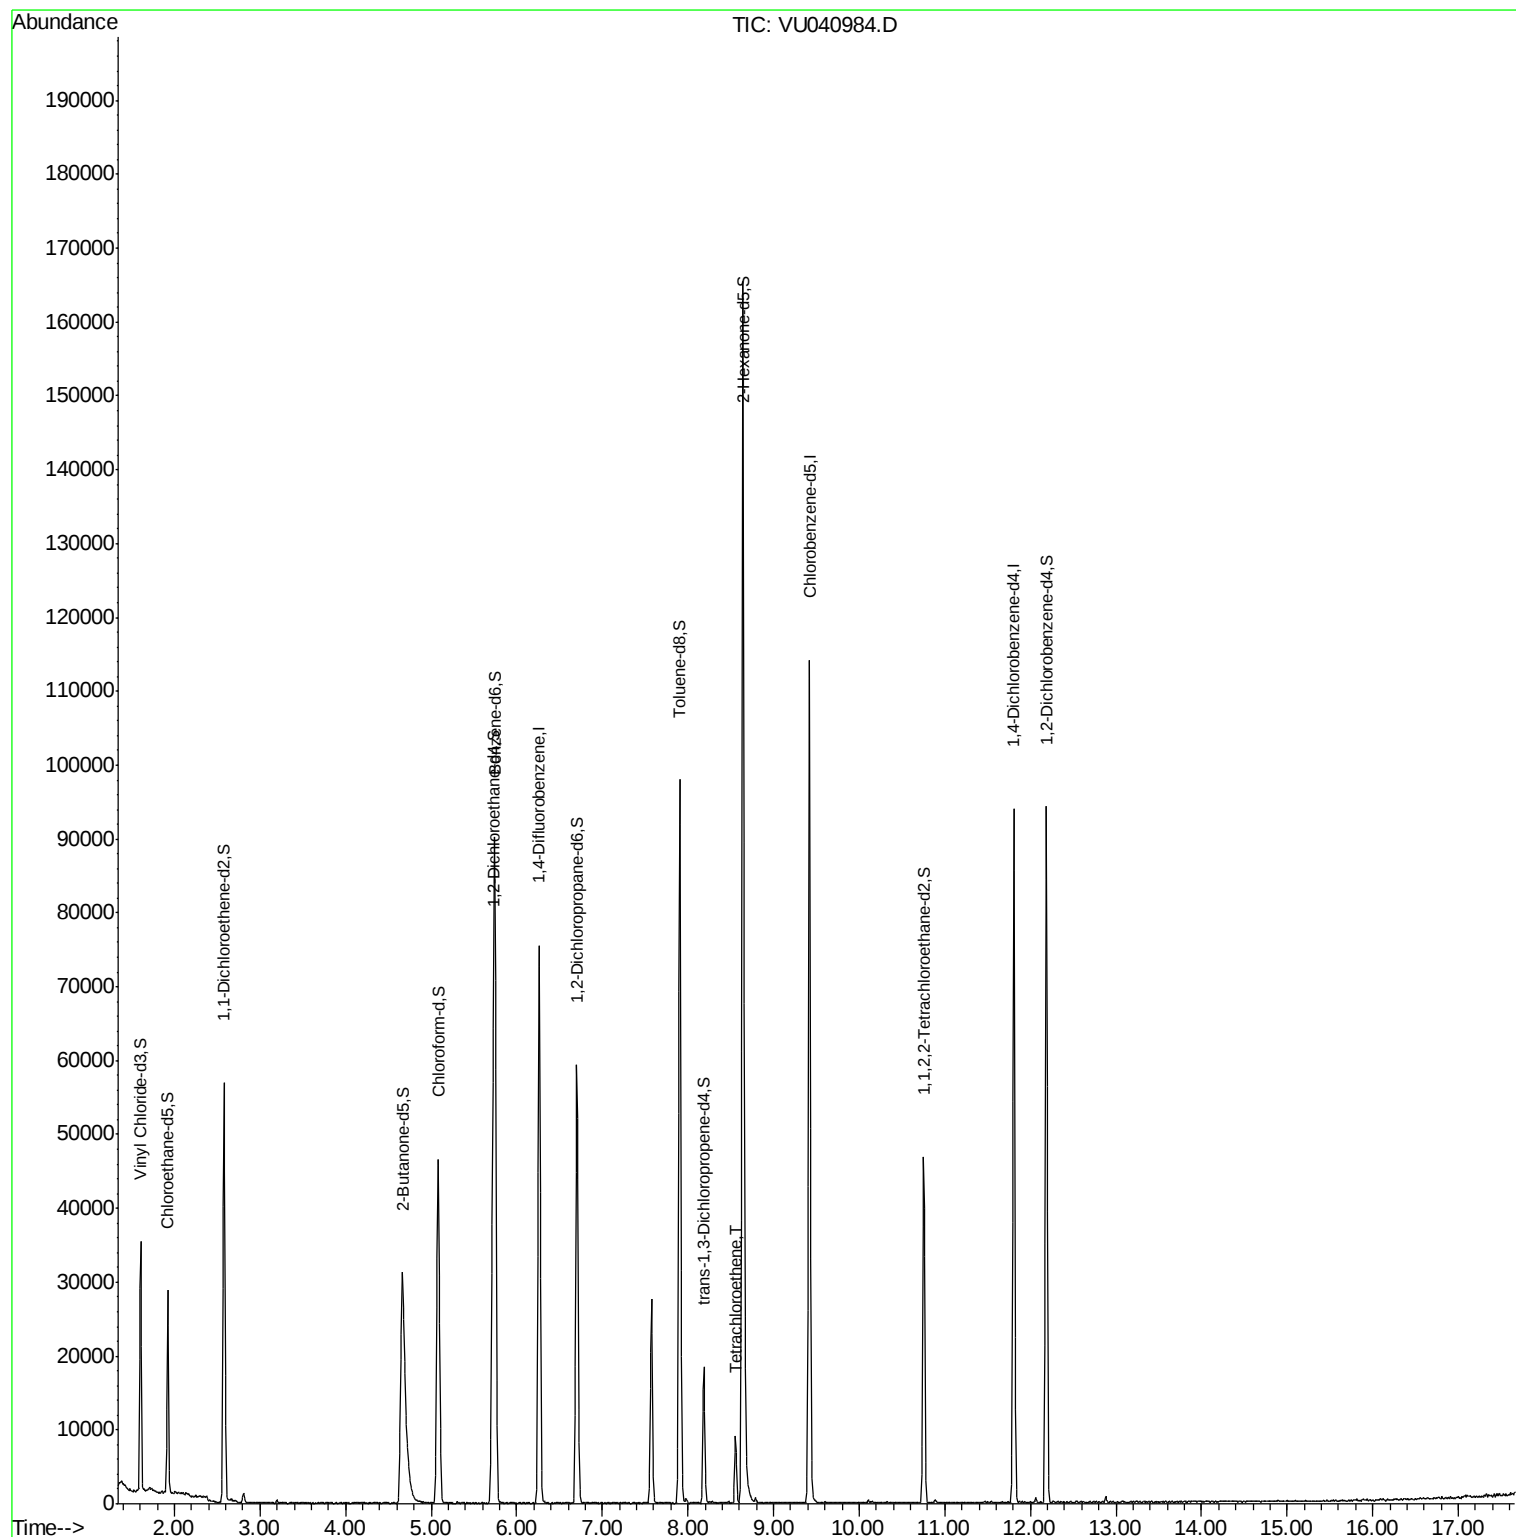

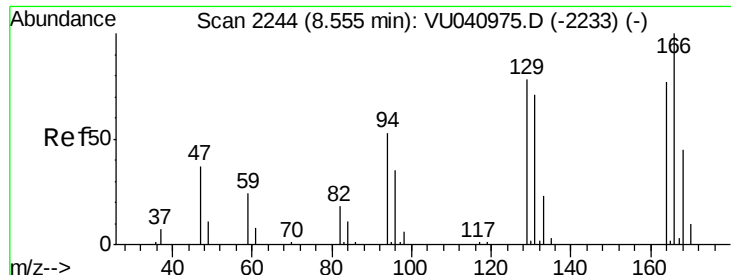

#47

Tetrachloroethene

Concen: 0.616 ug/L

RT: 8.56 min Scan# 2245

Delta R.T. 0.00 min

Lab File: VU040984.D


Acq: 27 Oct 2020 15:31

Instrument :

MSVOA_U

ClientSampleId :

C0AQ1

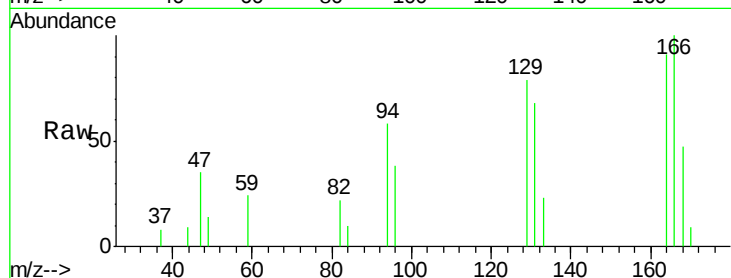

Tot Ion:164 Resp: 1984

Ion Ratio Lower Upper

164 100

129 86.6 70.3 130.7

131 74.3 70.8 131.4

166 109.7 92.0 170.8

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

