


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102720\
 Data File : VU040974.D
 Acq On : 27 Oct 2020 10:49
 Operator : SY/MD
 Sample : BFB28
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB28

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 28 02:17:39 2020

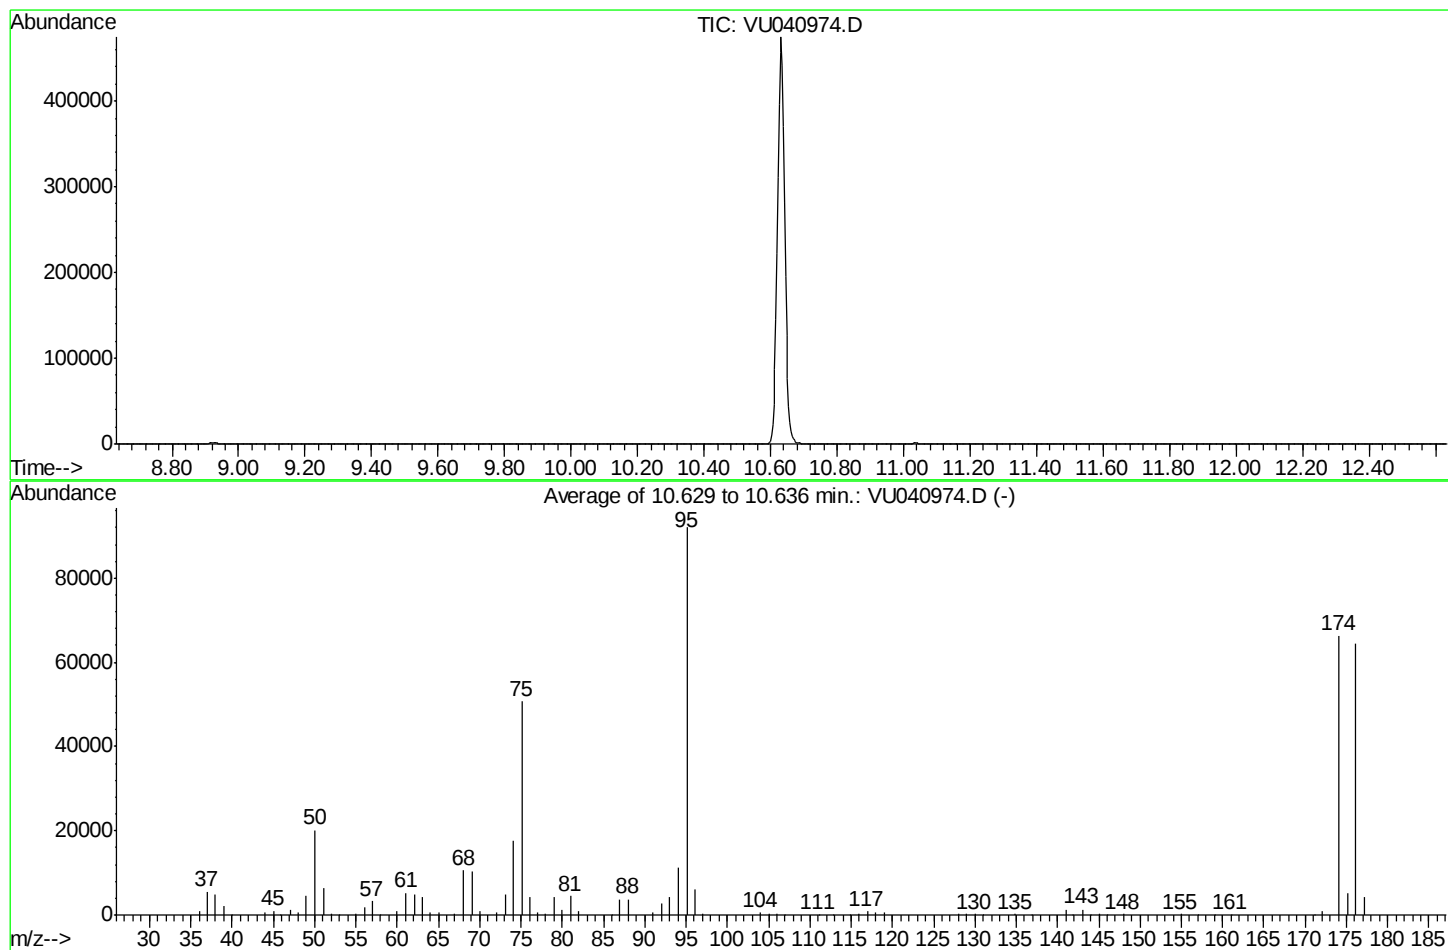

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	20066	PASS
75	95	30	80	55.1	50712	PASS
95	95	100	100	100.0	92056	PASS
96	95	5	9	6.6	6050	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	66360	PASS
175	174	5	9	7.6	5047	PASS
176	174	95	101	96.9	64298	PASS
177	176	5	9	6.5	4149	PASS

m/z	Abundance
36.00	951.0
37.00	5710.0
38.00	4960.0
39.00	2168.0
39.90	132.0
44.00	889.0
45.00	1052.0
45.90	100.0
47.10	1233.0
48.00	691.0
49.00	4562.0
50.10	20352.0
51.10	6387.0
52.00	261.0
53.00	114.0
55.00	292.0
56.00	1860.0
57.00	3470.0
58.10	117.0
60.00	1038.0
61.10	5304.0
62.10	4994.0
63.10	4398.0
64.10	729.0
65.10	807.0
67.00	375.0
68.00	10562.0
69.10	10165.0
70.10	762.0
72.00	667.0
73.10	4955.0
74.10	17632.0
75.10	51080.0
76.10	4282.0
77.00	523.0
78.00	387.0
79.00	4287.0
80.00	1219.0
81.00	4508.0
82.00	980.0
86.10	117.0
87.00	3816.0
88.00	3720.0
91.00	499.0
92.10	2788.0
93.00	4322.0
94.10	11379.0
95.10	92432.0
96.10	6080.0
97.00	189.0
104.00	482.0
105.10	229.0
106.00	499.0
106.90	106.0
111.10	117.0
112.90	125.0
116.00	407.0
117.00	831.0
118.00	487.0
118.90	546.0
128.00	308.0
129.00	169.0
130.00	294.0
131.00	136.0
134.90	161.0
136.90	164.0
141.00	1063.0
141.80	105.0
143.00	1247.0
144.00	103.0
145.00	443.0
146.00	112.0
148.00	249.0
155.00	212.0
157.00	137.0
171.10	122.0
172.10	1002.0
174.10	64552.0
175.10	5046.0
176.10	62600.0
177.10	4117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	974.0
37.00	5752.0
38.00	5075.0
39.00	2153.0
39.90	130.0
44.00	872.0
45.00	1092.0
45.90	113.0
47.10	1243.0
47.90	643.0
49.00	4858.0
50.10	20832.0
51.10	6512.0
52.00	260.0
53.00	138.0
55.00	285.0
56.00	1810.0
57.00	3451.0
58.00	119.0
60.00	1058.0
61.10	5425.0
62.10	5151.0
63.10	4494.0
64.00	668.0
65.10	748.0
67.00	404.0
68.10	10871.0
69.10	10550.0
70.10	825.0
72.00	655.0
73.10	5000.0
74.10	18208.0
75.10	52576.0
76.10	4460.0
77.00	565.0
78.00	394.0
79.00	4355.0
80.00	1287.0
81.00	4580.0
82.00	1075.0
86.00	118.0
87.00	3891.0
88.00	3843.0
90.90	486.0
92.10	2855.0
93.00	4462.0
94.10	11796.0
95.10	95528.0
96.10	6204.0
97.00	253.0
104.00	496.0
105.00	264.0
106.00	473.0
106.90	107.0
111.10	129.0
112.90	115.0
114.90	107.0
116.00	482.0
117.00	805.0
118.00	532.0
119.00	592.0
128.00	285.0
129.00	183.0
130.00	306.0
131.00	138.0
134.90	188.0
136.90	159.0
141.00	1133.0
141.90	116.0
143.00	1253.0
144.10	123.0
145.00	420.0
146.00	127.0
148.00	287.0
155.00	244.0
157.00	157.0
159.00	106.0
161.00	113.0
171.10	111.0
172.10	1018.0
174.10	68736.0
175.10	5289.0
176.10	66712.0
177.10	4335.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	890.0
37.00	5261.0
38.00	4691.0
39.00	1992.0
40.00	111.0
44.00	804.0
45.00	944.0
45.90	106.0
47.10	1130.0
47.90	542.0
49.00	4607.0
50.10	19016.0
51.10	5970.0
52.10	235.0
53.00	132.0
55.00	256.0
56.00	1540.0
57.00	2970.0
57.90	123.0
60.00	988.0
61.10	4981.0
62.10	4752.0
63.10	4129.0
64.00	558.0
65.10	673.0
67.00	363.0
68.10	10130.0
69.10	10012.0
70.00	825.0
72.00	606.0
73.10	4455.0
74.10	16784.0
75.10	48480.0
76.10	4134.0
77.00	532.0
77.90	393.0
79.00	4021.0
80.00	1232.0
81.00	4199.0
82.00	1090.0
87.00	3446.0
88.00	3704.0
90.90	433.0
92.00	2687.0
93.10	4097.0
94.10	10963.0
95.10	88208.0
96.10	5866.0
97.00	250.0
104.00	466.0
105.00	231.0
106.00	407.0
111.10	114.0
114.90	114.0
116.00	472.0
117.00	683.0
118.00	490.0
119.00	565.0
128.00	282.0
129.00	163.0
130.00	279.0
130.90	119.0
134.90	206.0
136.90	154.0
141.00	1055.0
141.90	118.0
143.00	1195.0
144.10	133.0
145.00	337.0
146.00	118.0
148.00	260.0
155.00	246.0
157.00	164.0
159.00	115.0
161.00	124.0
172.10	942.0
174.10	65792.0
175.10	4808.0
176.10	63584.0
177.10	3997.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
43.90	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28