




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055921.D
 Acq On : 27 Oct 2023 13:23
 Operator : MD/SY
 Sample : 05009-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4931

Manual IntegrationsAPPROVED

Quant Time: Oct 27 23:55:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 05:19:13 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

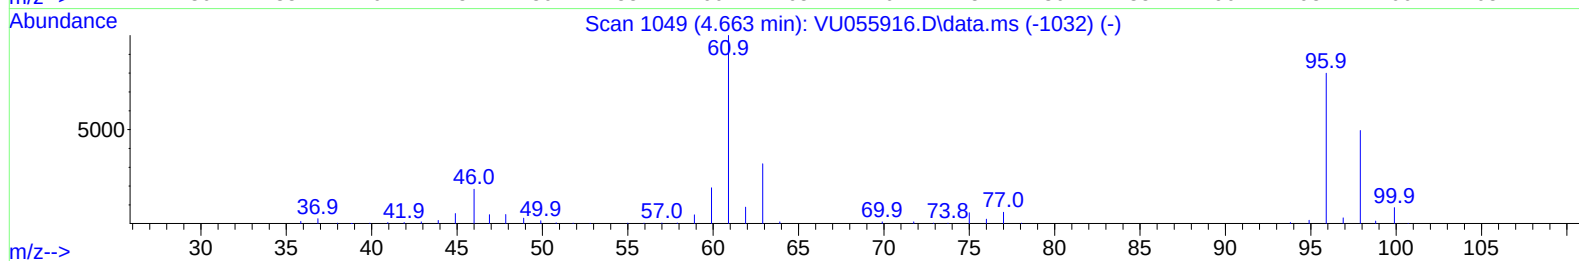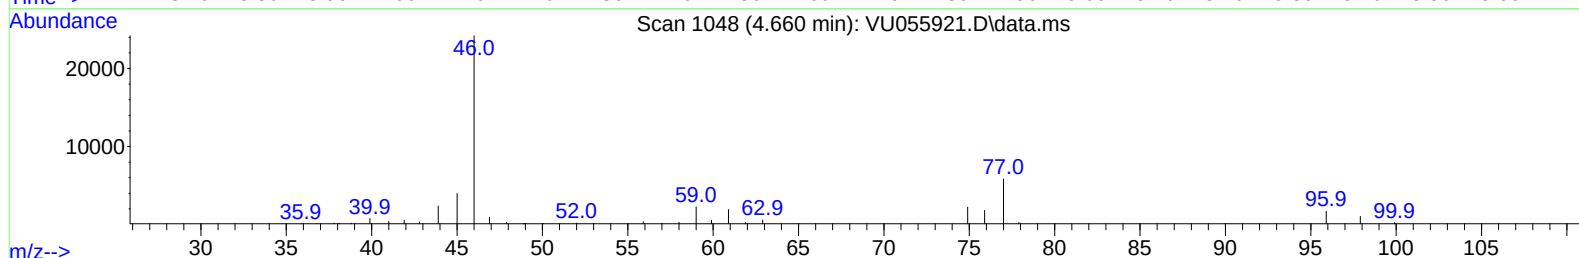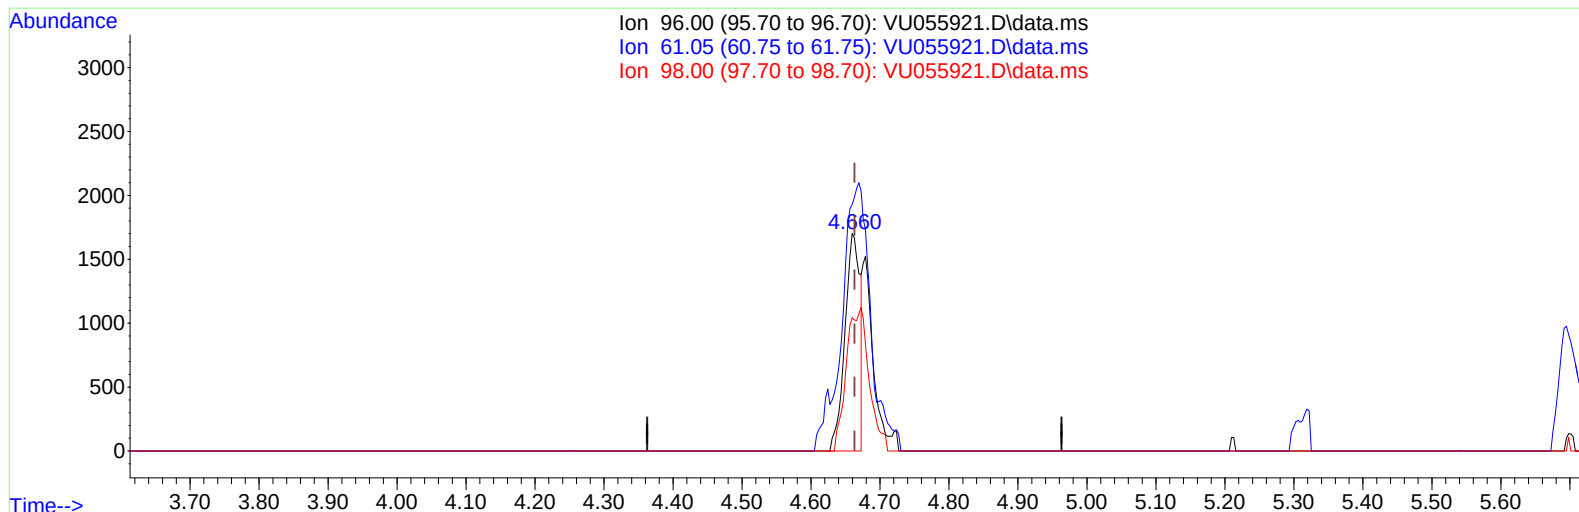

TIC: VU055921.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.660min (-0.003) 0.11 ug/L

response 2578

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	134.00	113.52
98.00	65.20	61.32
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055921.D
 Acq On : 27 Oct 2023 13:23
 Operator : MD/SY
 Sample : 05009-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4931

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

Quant Time: Oct 27 23:55:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 05:19:13 2023
 Response via : Initial Calibration

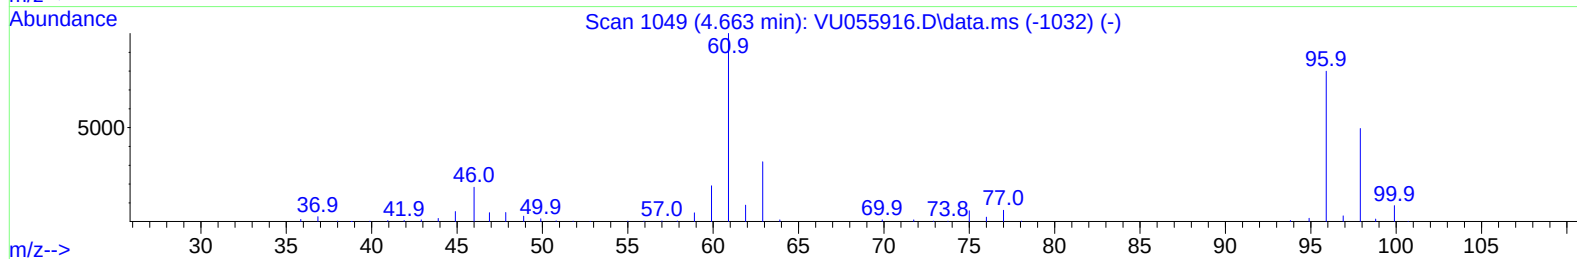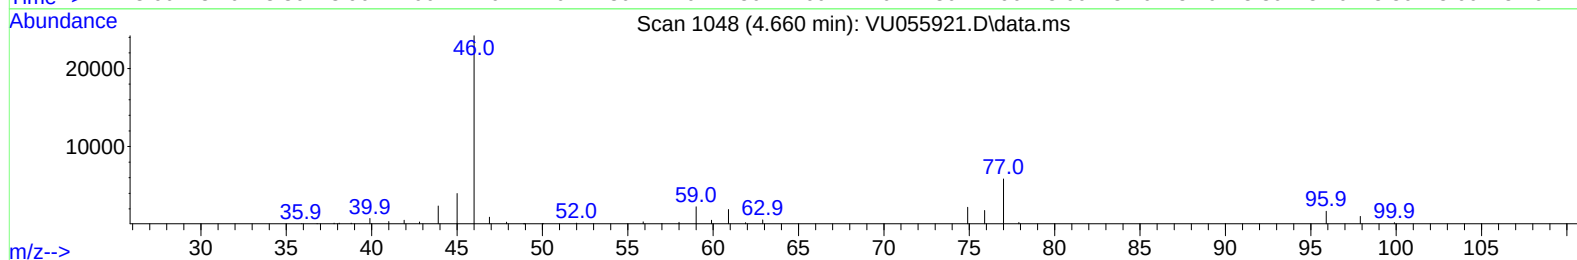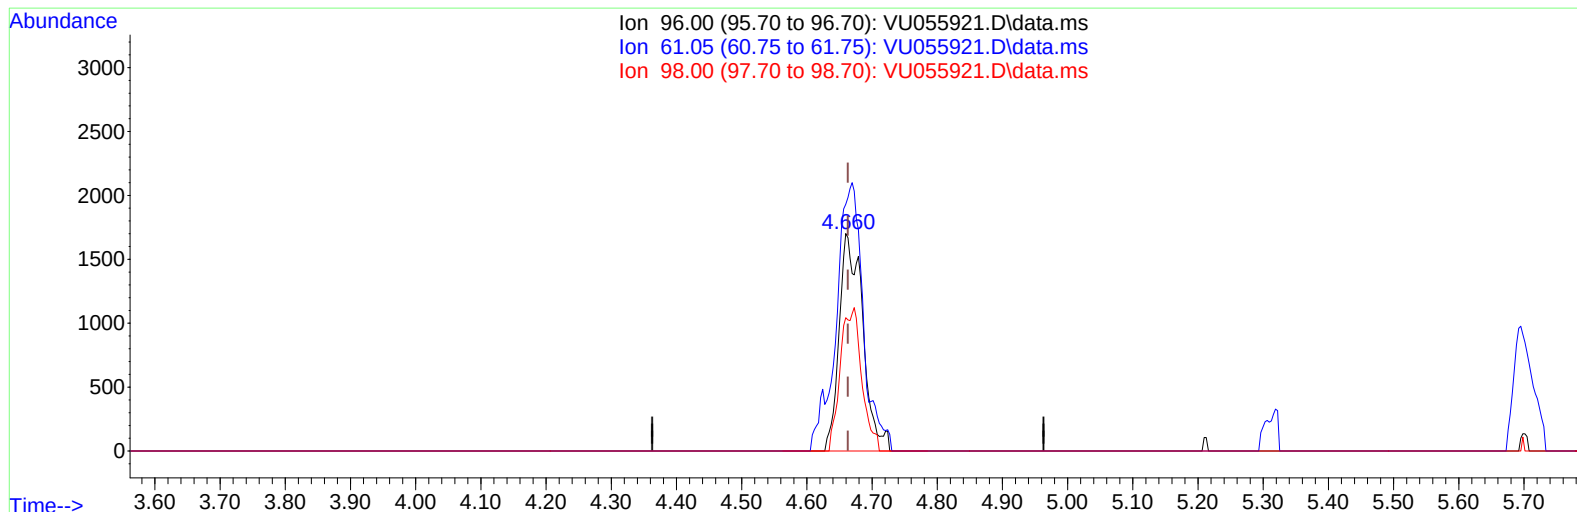

TIC: VU055921.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.660min (-0.003) 0.19 ug/L m

response 4273

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	134.00	113.52
98.00	65.20	61.32
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055921.D
 Acq On : 27 Oct 2023 13:23
 Operator : MD/SY
 Sample : 05009-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4931

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

Quant Time: Oct 27 23:55:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 05:19:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	385959	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	370357	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	178737	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	105074	3.441	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	68.800%		
7) Chloroethane-d5	1.914	69	91962	3.864	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	77.200%		
11) 1,1-Dichloroethene-d2	2.566	65	47302	3.649	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	73.000%		
20) 2-Butanone-d5	4.624	46	224214	41.165	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	82.320%		
24) Chloroform-d	5.058	84	229026	4.048	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	81.000%		
26) 1,2-Dichloroethane-d4	5.698	65	111623	4.050	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	81.000%		
32) Benzene-d6	5.724	84	463249	4.199	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	6.685	67	144707	4.425	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.400%		
41) Toluene-d8	7.894	98	402593	4.023	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	80.400%		
43) trans-1,3-Dichloroprop...	8.177	79	43282	3.384	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	67.600%		
46) 2-Hexanone-d5	8.631	63	194168	59.800	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	119.600%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	103524	4.347	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	87.000%		
66) 1,2-Dichlorobenzene-d4	12.190	152	144010	4.318	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	86.400%		
Target Compounds						
3) Chloromethane	1.518	50	3012	0.143	ug/L	100
22) cis-1,2-Dichloroethene	4.660	96	4273m	0.190	ug/L	
42) Toluene	7.968	91	39514	0.463	ug/L	92
53) m,p-Xylene	9.695	106	13337	0.369	ug/L	90
54) o-Xylene	10.100	106	5840	0.165	ug/L	89
63) 1,2,4-Trimethylbenzene	11.466	105	13695	0.203	ug/L	96
69) 1,3,5-Trichlorobenzene	13.222	180	7951	0.276	ug/L	97
70) 1,2,4-trichlorobenzene	13.843	180	10519	0.493	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055921.D
Acq On : 27 Oct 2023 13:23
Operator : MD/SY
Sample : 05009-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4931

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/30/2023
Supervised By :Mahesh Dadoda 10/31/2023

Quant Time: Oct 27 23:55:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 05:19:13 2023
Response via : Initial Calibration

