

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055918.D
 Acq On : 27 Oct 2023 11:24
 Operator : MD/SY
 Sample : 05053-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B14

Quant Time: Oct 27 12:53:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 05:19:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	412428	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	401989	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	184956	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	112610	3.452	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.000%
7) Chloroethane-d5	1.914	69	98397	3.869	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.400%
11) 1,1-Dichloroethene-d2	2.567	65	51027	3.684	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.600%
20) 2-Butanone-d5	4.628	46	260390	44.739	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.480%
24) Chloroform-d	5.062	84	250094	4.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
26) 1,2-Dichloroethane-d4	5.698	65	119123	4.044	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
32) Benzene-d6	5.724	84	496114	4.143	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	6.689	67	155472	4.380	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.898	98	439649	4.047	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	8.181	79	46442	3.345	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.000%
46) 2-Hexanone-d5	8.634	63	217109	61.604	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.200%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	111952	4.331	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	154204	4.469	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.400%
Target Compounds					Qvalue	
13) Acetone	2.644	43	42197	12.723	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055918.D
Acq On : 27 Oct 2023 11:24
Operator : MD/SY
Sample : 05053-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B14

Quant Time: Oct 27 12:53:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 05:19:13 2023
Response via : Initial Calibration

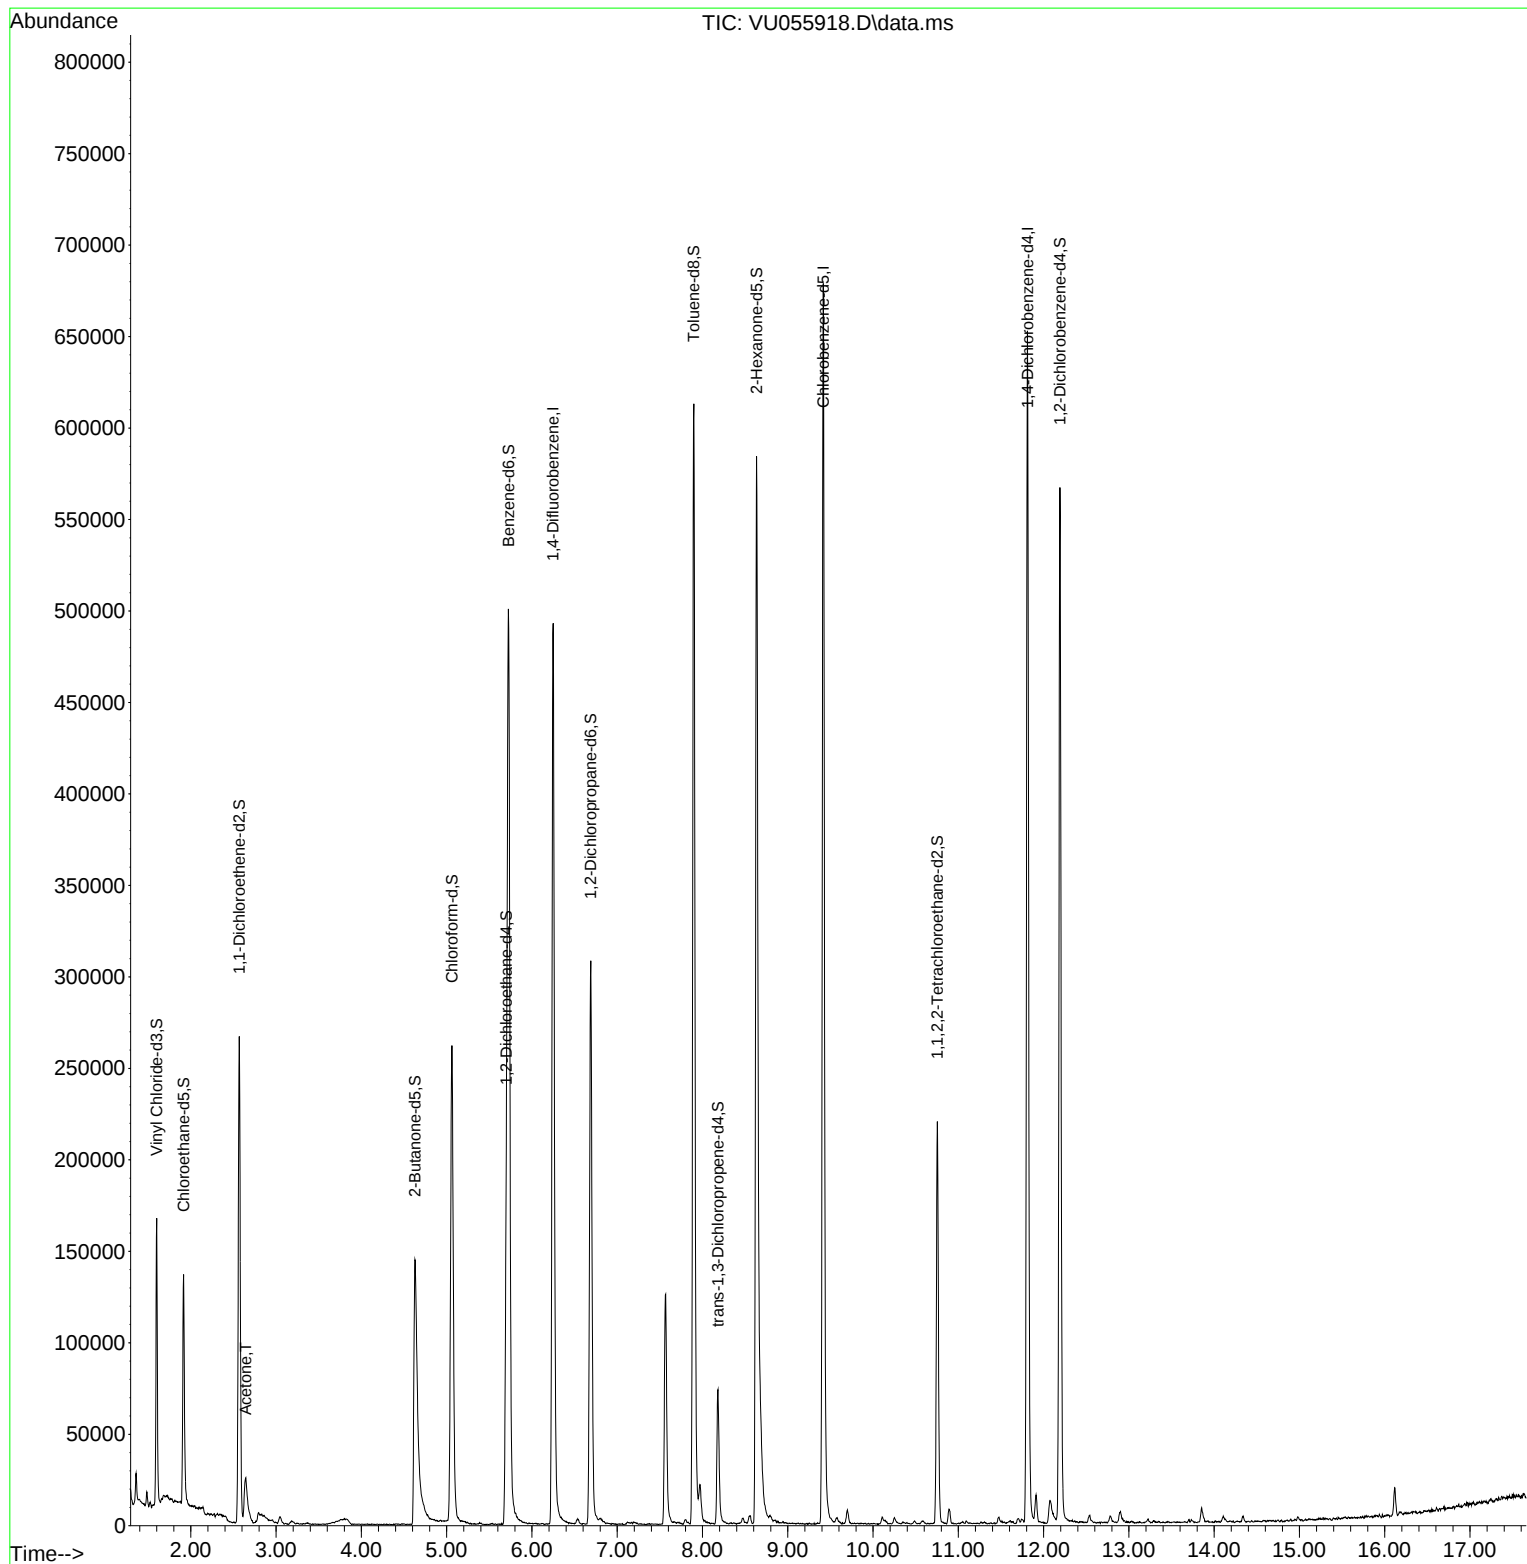

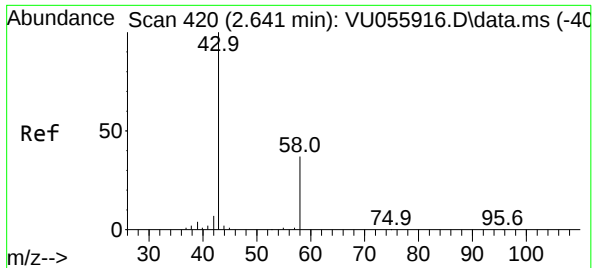

#13
 Acetone
 Concen: 12.723 ug/L
 RT: 2.644 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU055918.D
 Acq: 27 Oct 2023 11:24

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B14

Tgt Ion: 43 Resp: 42197
 Ion Ratio Lower Upper
 43 100
 58 35.9 0.0 69.0

