

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055919.D
 Acq On : 27 Oct 2023 11:48
 Operator : MD/SY
 Sample : 05053-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B19

Quant Time: Oct 27 12:53:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 05:19:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	404498	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	384249	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	180472	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	103989	3.250	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.000%
7) Chloroethane-d5	1.914	69	95854	3.843	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.800%
11) 1,1-Dichloroethene-d2	2.567	65	49497	3.644	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.800%
20) 2-Butanone-d5	4.628	46	237436	41.594	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.180%
24) Chloroform-d	5.062	84	235504	3.972	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.400%
26) 1,2-Dichloroethane-d4	5.698	65	114628	3.968	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
32) Benzene-d6	5.724	84	478138	4.177	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
36) 1,2-Dichloropropane-d6	6.685	67	147143	4.337	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.894	98	409434	3.943	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.800%
43) trans-1,3-Dichloroprop...	8.180	79	43990	3.315	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.200%
46) 2-Hexanone-d5	8.631	63	207888	61.711	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.420%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	106720	4.319	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	151122	4.488	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.800%
Target Compounds					Qvalue	
13) Acetone	2.640	43	41486	12.753	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055919.D
Acq On : 27 Oct 2023 11:48
Operator : MD/SY
Sample : 05053-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B19

Quant Time: Oct 27 12:53:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 05:19:13 2023
Response via : Initial Calibration

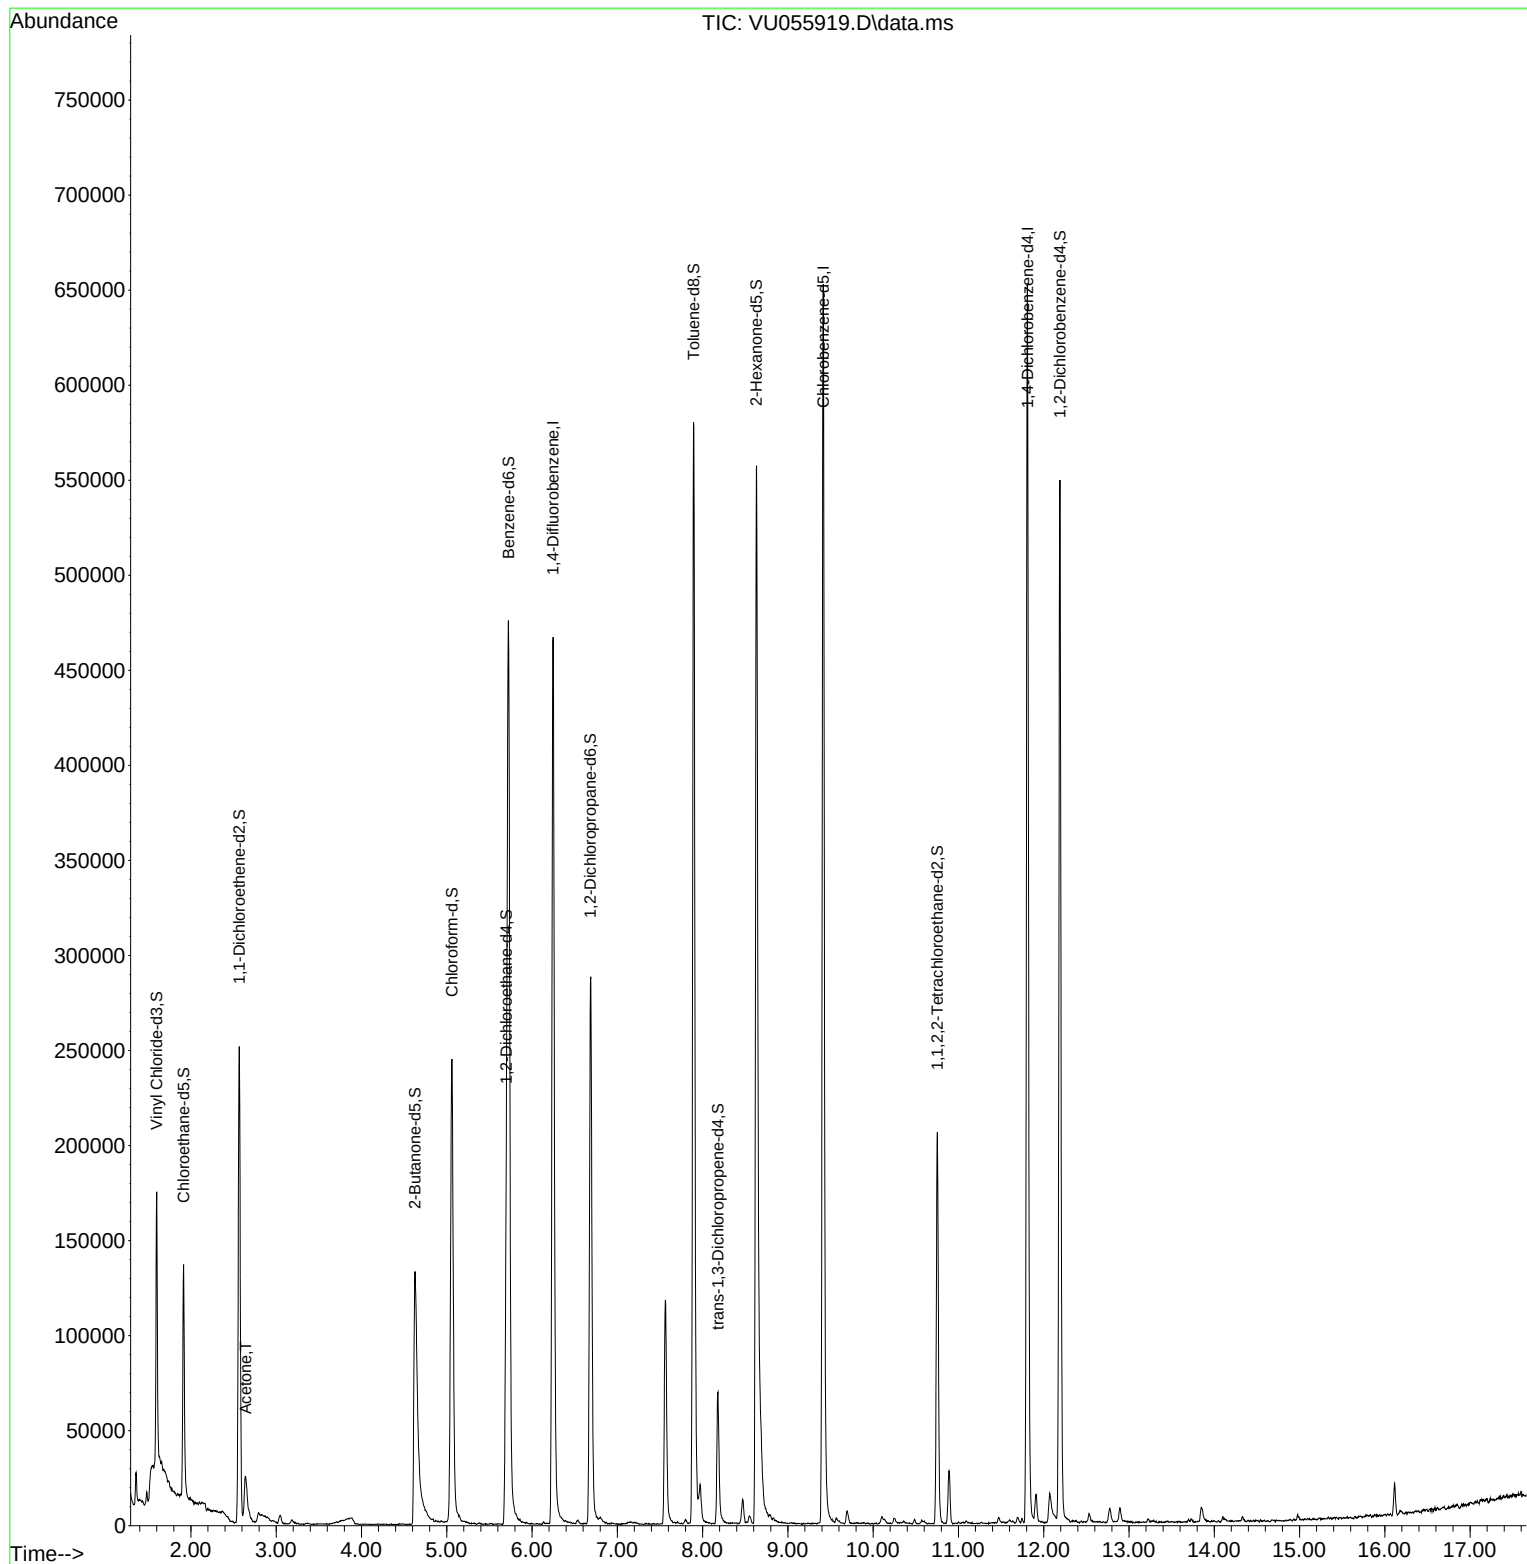

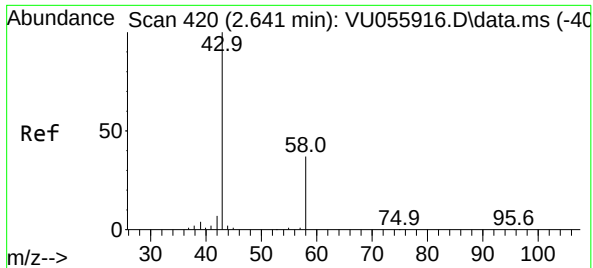

#13
 Acetone
 Concen: 12.753 ug/L
 RT: 2.640 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU055919.D
 Acq: 27 Oct 2023 11:48

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B19

Tgt Ion: 43 Resp: 41486
 Ion Ratio Lower Upper
 43 100
 58 35.6 0.0 69.0

