

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055919.D
 Acq On : 27 Oct 2023 11:48
 Operator : MD/SY
 Sample : 05053-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B19

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	15	21	29	rBV2	16883	19982	1.60%	0.183%
2	1.534	67	76	77	rBV6	16947	21650	1.73%	0.198%
3	1.599	89	96	105	rBV	142133	163147	13.07%	1.495%
4	1.914	186	194	213	rVB	123322	169691	13.59%	1.555%
5	2.567	385	397	410	rBV	250548	414559	33.20%	3.798%
6	2.637	410	419	439	rVB2	22383	56702	4.54%	0.520%
7	4.628	1025	1038	1096	rBV	132958	439911	35.23%	4.030%
8	5.062	1154	1173	1198	rBV	243352	554780	44.43%	5.083%
9	5.724	1358	1379	1405	rBV2	475426	1248693	100.00%	11.441%
10	6.248	1529	1542	1569	rBV	466263	929747	74.46%	8.518%
11	6.689	1663	1679	1700	rBV	287927	583291	46.71%	5.344%
12	7.563	1940	1951	1980	rBV2	117855	224300	17.96%	2.055%
13	7.894	2041	2054	2070	rBV	579011	1035496	82.93%	9.487%
14	7.971	2075	2078	2093	rVB2	19232	27667	2.22%	0.253%
15	8.180	2131	2143	2167	rBV	69416	130707	10.47%	1.198%
16	8.470	2220	2233	2244	rBV3	12832	23130	1.85%	0.212%
17	8.634	2272	2284	2316	rBV2	556502	1199345	96.05%	10.988%
18	9.415	2514	2527	2558	rBV	651527	1140588	91.34%	10.450%
19	9.695	2605	2614	2625	rBV4	6919	12597	1.01%	0.115%
20	10.753	2930	2943	2960	rBV	206052	348427	27.90%	3.192%
21	10.891	2975	2986	2999	rVB	27970	48174	3.86%	0.441%
22	11.807	3259	3271	3295	rBV	651879	1082781	86.71%	9.920%
23	11.910	3295	3303	3312	rVB7	14197	24004	1.92%	0.220%
24	12.071	3342	3353	3377	rBV4	15511	44612	3.57%	0.409%
25	12.190	3377	3390	3409	rVV	546585	911605	73.00%	8.352%
26	12.775	3560	3572	3585	rBV5	7596	16085	1.29%	0.147%
27	13.846	3899	3905	3922	rBV5	7306	15665	1.25%	0.144%
28	16.116	4601	4611	4621	rBV4	17330	27257	2.18%	0.250%




Sum of corrected areas: 10914593

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055919.D
Acq On : 27 Oct 2023 11:48
Operator : MD/SY
Sample : 05053-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

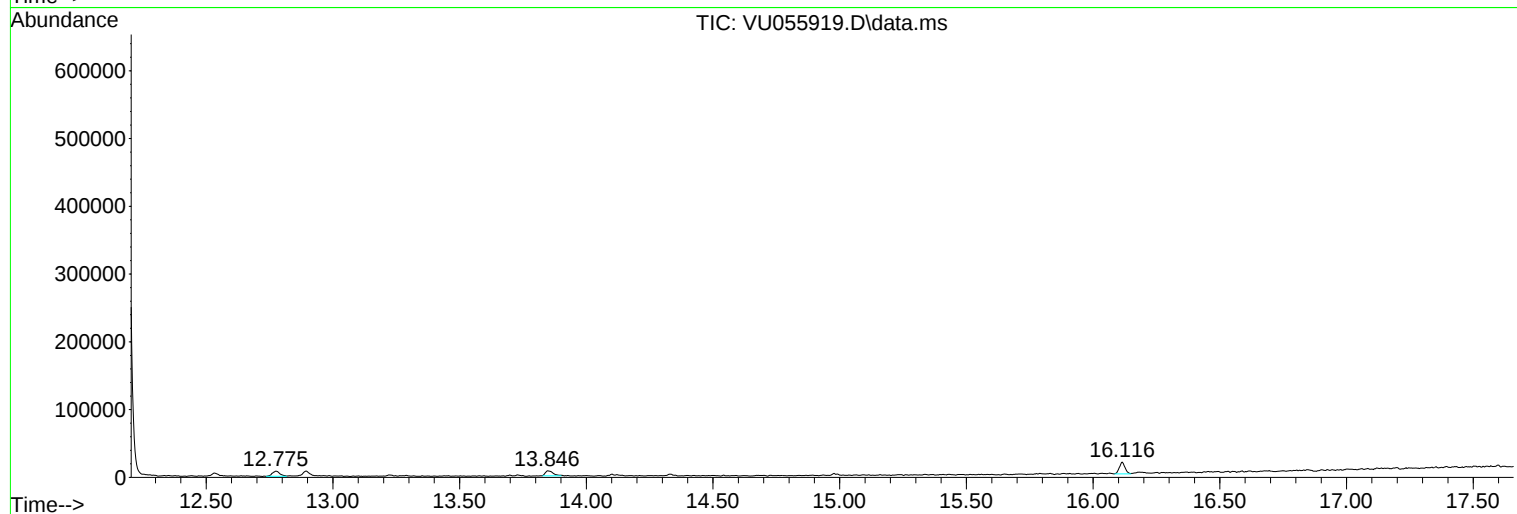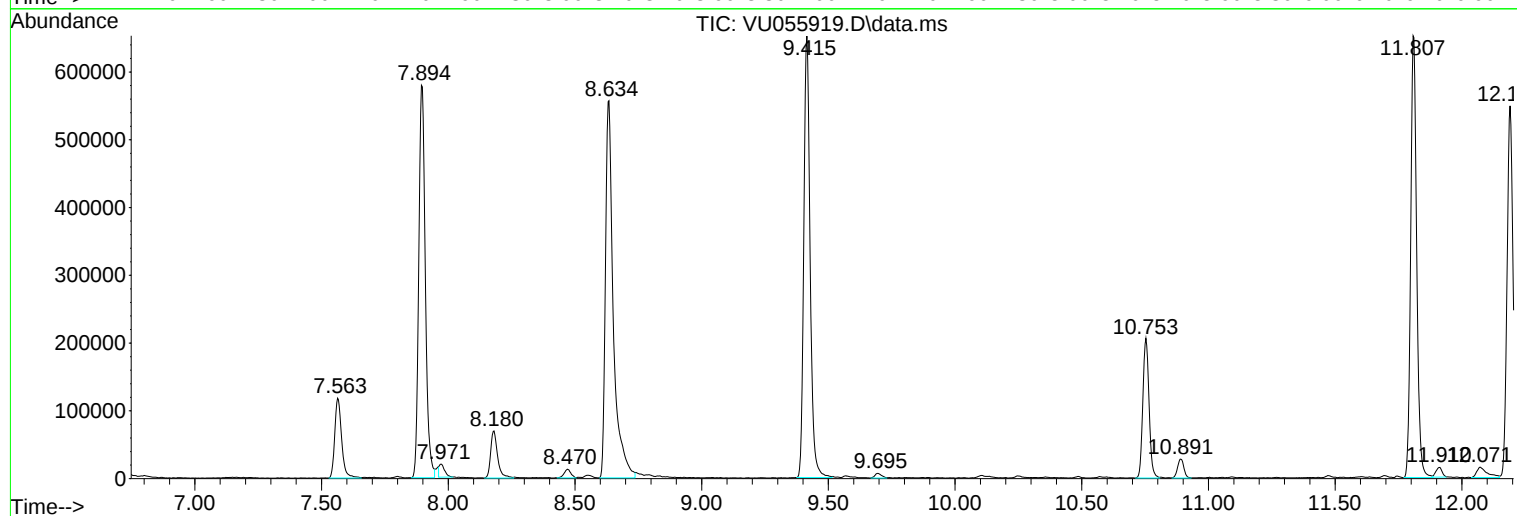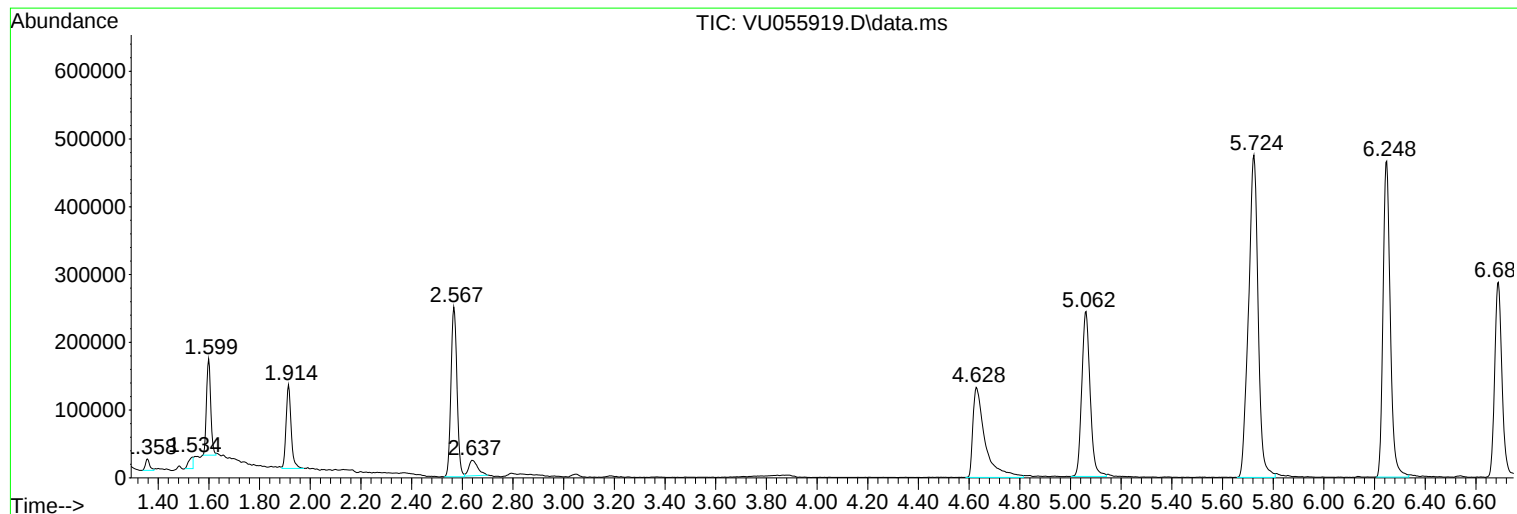

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055919.D
Acq On : 27 Oct 2023 11:48
Operator : MD/SY
Sample : 05053-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055919.D
Acq On : 27 Oct 2023 11:48
Operator : MD/SY
Sample : 05053-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc