

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055922.D
 Acq On : 27 Oct 2023 14:41
 Operator : MD/SY
 Sample : 05009-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A49A1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	79	rVB	15938	17667	1.42%	0.163%
2	1.599	88	96	107	rBV	145952	174027	14.00%	1.610%
3	1.914	186	194	209	rVB	118765	160320	12.90%	1.483%
4	2.567	383	397	411	rBV	248032	410803	33.05%	3.799%
5	4.628	1025	1038	1072	rBV	137313	412275	33.17%	3.813%
6	5.058	1157	1172	1194	rBV	237787	538995	43.36%	4.985%
7	5.721	1354	1378	1409	rBV2	472020	1243019	100.00%	11.497%
8	6.248	1528	1542	1568	rBV	477592	937526	75.42%	8.671%
9	6.537	1620	1632	1649	rVB7	7246	15924	1.28%	0.147%
10	6.689	1664	1679	1698	rBV	283830	572485	46.06%	5.295%
11	7.563	1940	1951	1977	rBV	117059	221143	17.79%	2.045%
12	7.798	2014	2024	2036	rBV4	8388	16373	1.32%	0.151%
13	7.898	2042	2055	2072	rBV	572966	1024147	82.39%	9.472%
14	8.180	2132	2143	2163	rBV	66102	124257	10.00%	1.149%
15	8.553	2249	2259	2272	rVB6	7298	13399	1.08%	0.124%
16	8.634	2272	2284	2332	rBV3	540420	1166983	93.88%	10.793%
17	9.415	2507	2527	2559	rBV	655398	1171764	94.27%	10.838%
18	9.695	2605	2614	2631	rBB2	10895	18980	1.53%	0.176%
19	10.753	2931	2943	2963	rBV	204437	340675	27.41%	3.151%
20	10.891	2975	2986	2998	rBV2	18557	30808	2.48%	0.285%
21	11.470	3155	3166	3176	rBV3	13013	20275	1.63%	0.188%
22	11.811	3260	3272	3296	rVV	657216	1101204	88.59%	10.185%
23	12.077	3344	3355	3370	rBV4	12423	33469	2.69%	0.310%
24	12.190	3377	3390	3412	rBV	538202	906914	72.96%	8.388%
25	13.222	3697	3711	3723	rBV5	24068	42834	3.45%	0.396%
26	13.843	3890	3904	3923	rBV2	33293	60803	4.89%	0.562%
27	14.331	4047	4056	4067	rBV4	21052	34970	2.81%	0.323%




Sum of corrected areas: 10812039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055922.D
Acq On : 27 Oct 2023 14:41
Operator : MD/SY
Sample : 05009-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

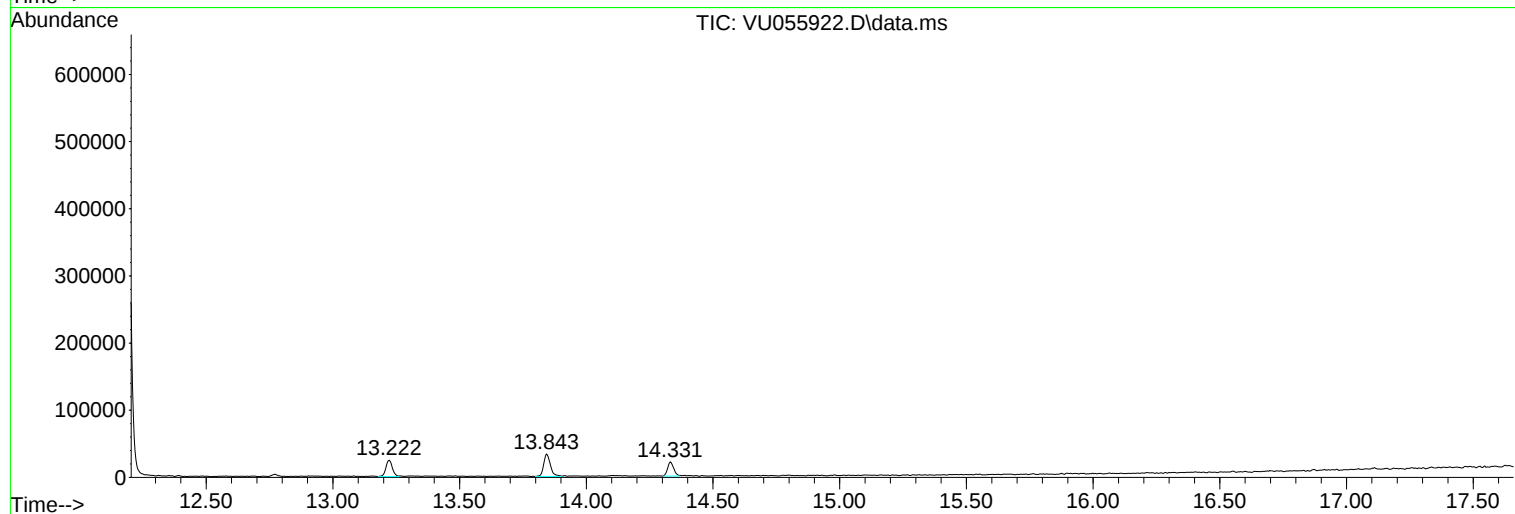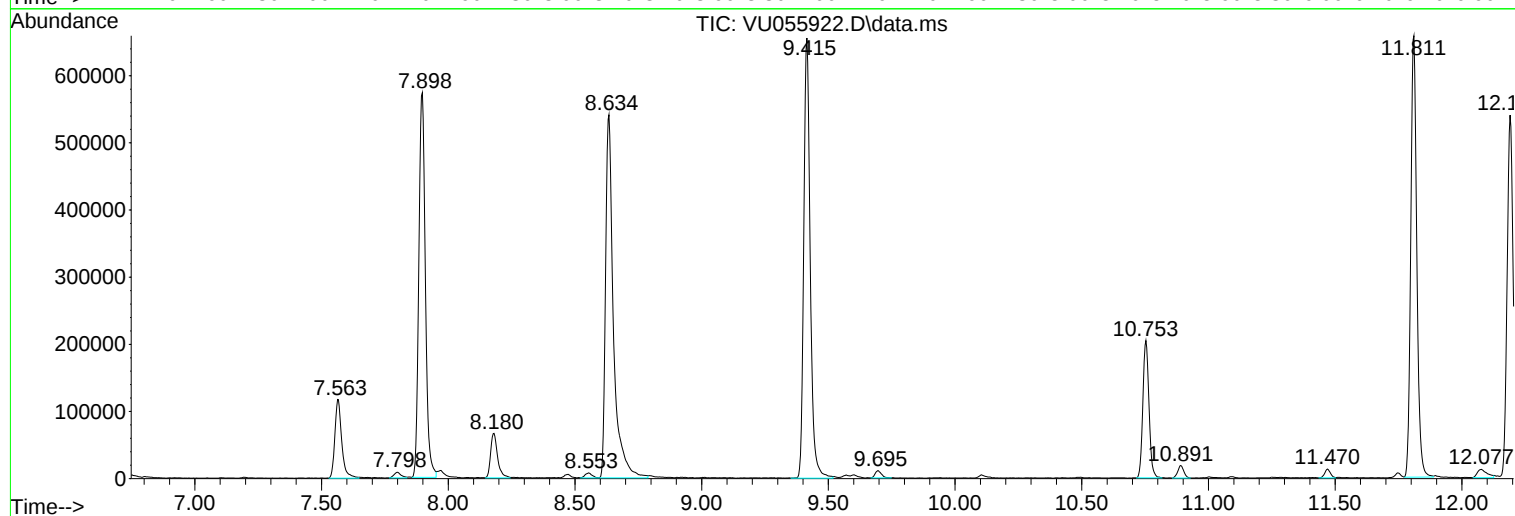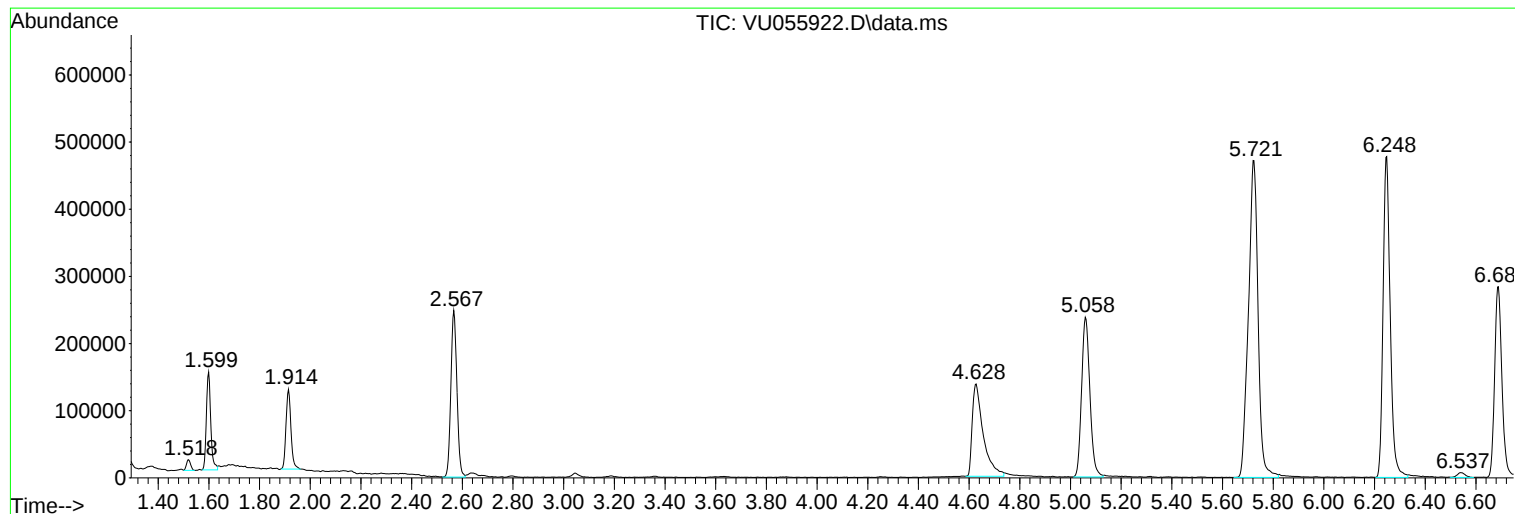

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055922.D
Acq On : 27 Oct 2023 14:41
Operator : MD/SY
Sample : 05009-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055922.D
Acq On : 27 Oct 2023 14:41
Operator : MD/SY
Sample : 05009-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49A1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc