

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055929.D
 Acq On : 27 Oct 2023 17:31
 Operator : MD/SY
 Sample : 05009-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A49J7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	65	71	84	rBV	30403	35534	2.91%	0.394%
2	1.599	89	96	107	rBV	92957	107205	8.79%	1.188%
3	1.914	186	194	210	rVB	83515	116032	9.52%	1.286%
4	2.567	383	397	411	rBV	162780	270763	22.21%	3.000%
5	4.624	1025	1037	1076	rBV	156408	455516	37.36%	5.047%
6	5.062	1157	1173	1197	rBV	191554	434148	35.61%	4.810%
7	5.724	1357	1379	1410	rBV2	344792	922177	75.64%	10.218%
8	6.248	1526	1542	1566	rBV	427456	851625	69.85%	9.436%
9	6.689	1665	1679	1705	rBV	226008	455654	37.37%	5.049%
10	7.566	1940	1952	1978	rBV	102390	195905	16.07%	2.171%
11	7.898	2041	2055	2072	rBV	385175	693796	56.91%	7.687%
12	8.180	2126	2143	2163	rBV2	60213	112511	9.23%	1.247%
13	8.631	2271	2283	2323	rBV2	563961	1219168	100.00%	13.508%
14	9.415	2514	2527	2551	rBV	588151	1047520	85.92%	11.607%
15	10.753	2931	2943	2962	rBV	194011	324733	26.64%	3.598%
16	10.891	2973	2986	2999	rBV3	8713	15584	1.28%	0.173%
17	11.811	3260	3272	3295	rBV	610224	1029071	84.41%	11.402%
18	12.081	3346	3356	3368	rBV8	7021	18110	1.49%	0.201%
19	12.190	3376	3390	3411	rBV	424615	720231	59.08%	7.980%




Sum of corrected areas: 9025283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055929.D
Acq On : 27 Oct 2023 17:31
Operator : MD/SY
Sample : 05009-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

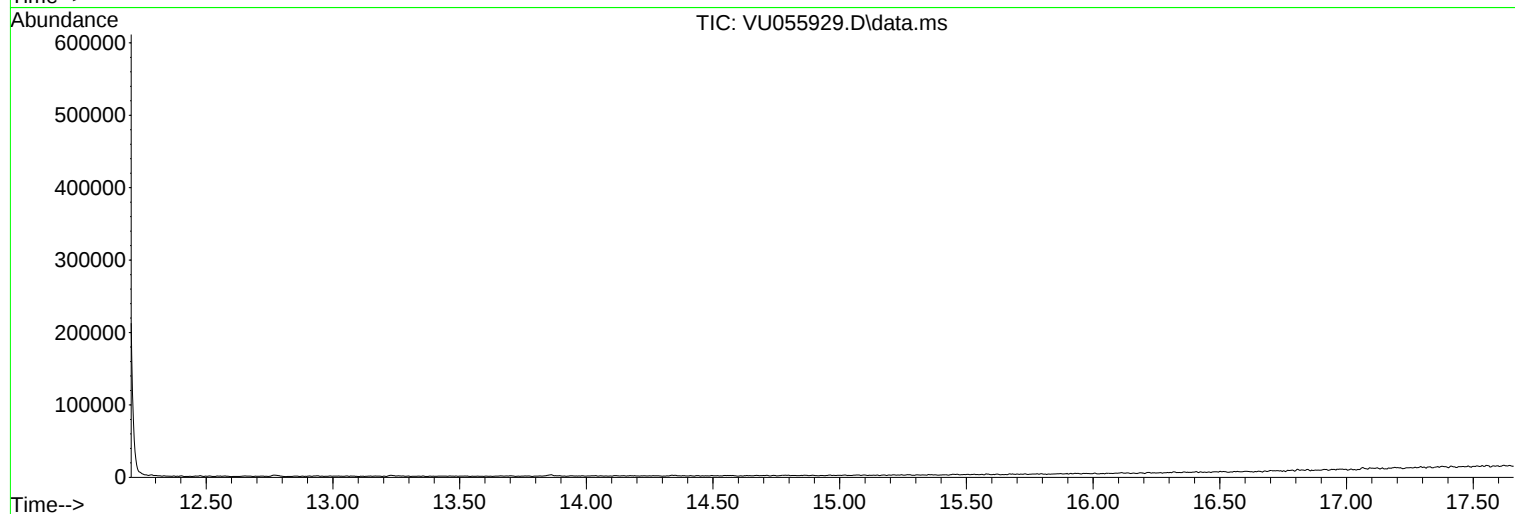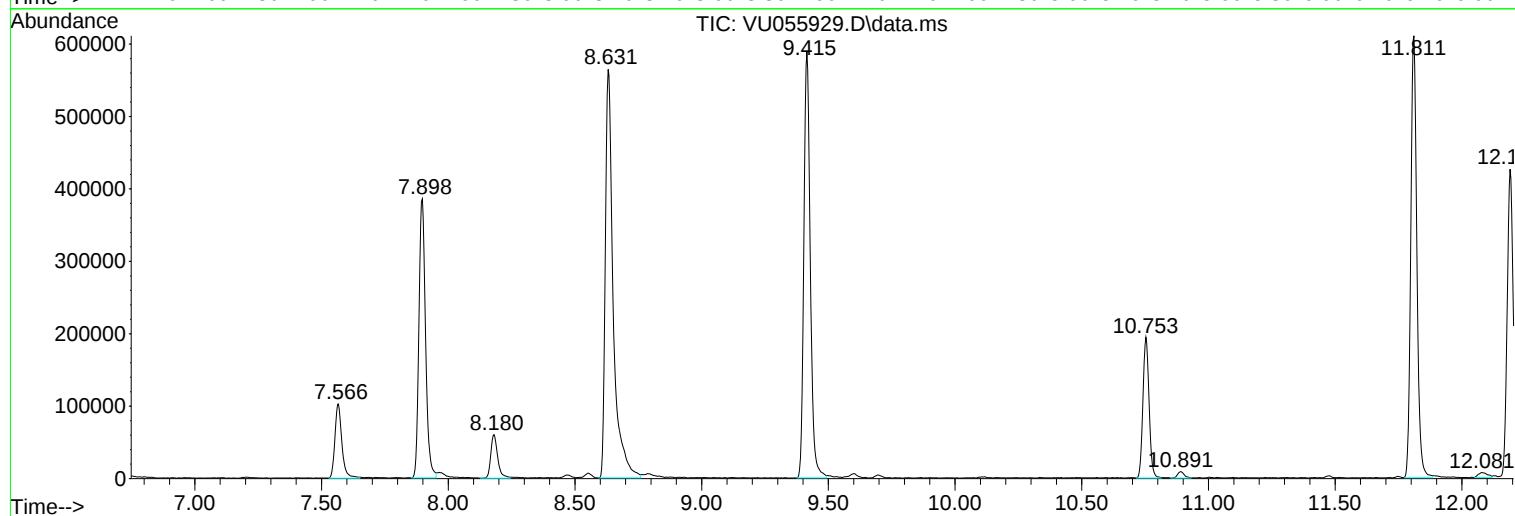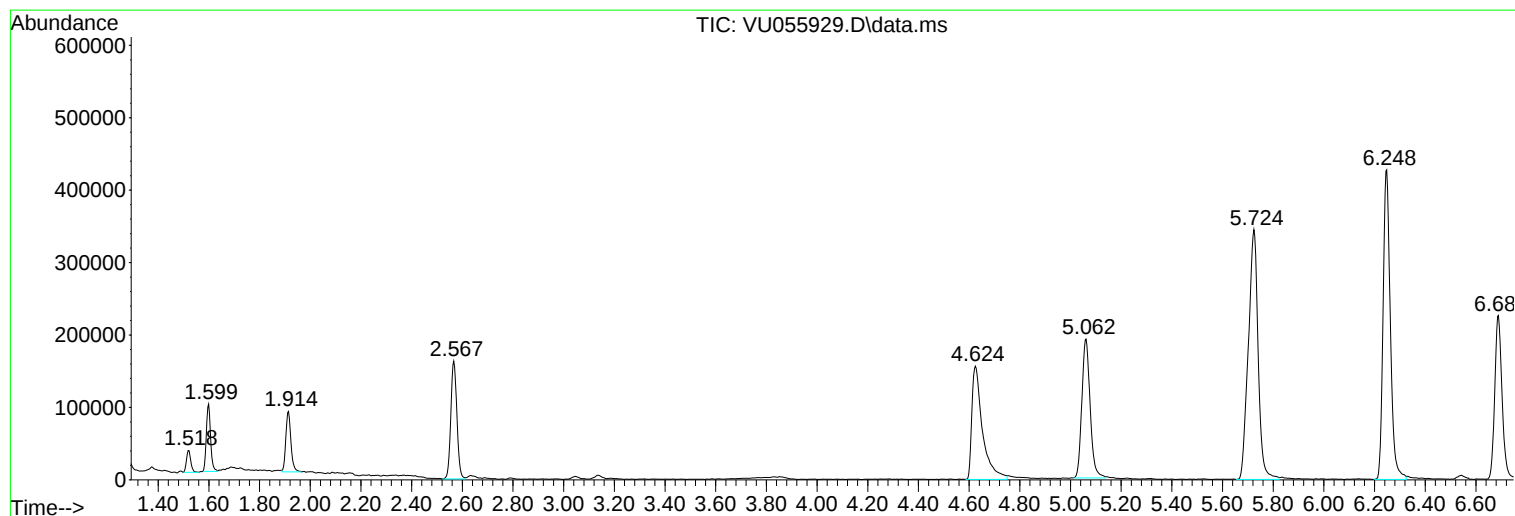

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055929.D
Acq On : 27 Oct 2023 17:31
Operator : MD/SY
Sample : 05009-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055929.D
Acq On : 27 Oct 2023 17:31
Operator : MD/SY
Sample : 05009-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc