

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU102723\  
 Data File : VU055936.D  
 Acq On : 27 Oct 2023 21:39  
 Operator : MD/SY  
 Sample : VU1027WBL02  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VBLK055

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055936.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.599       | 88            | 96          | 109          | rBV      | 151700         | 173696        | 14.31%          | 1.747%        |
| 2         | 1.914       | 186           | 194         | 212          | rVB      | 118506         | 166740        | 13.74%          | 1.677%        |
| 3         | 2.567       | 384           | 397         | 416          | rBV      | 266904         | 442220        | 36.43%          | 4.448%        |
| 4         | 4.628       | 1024          | 1038        | 1067         | rBV2     | 124075         | 363719        | 29.96%          | 3.658%        |
| 5         | 5.058       | 1157          | 1172        | 1196         | rBV      | 226305         | 515641        | 42.48%          | 5.186%        |
| 6         | 5.724       | 1358          | 1379        | 1409         | rBV2     | 468839         | 1213976       | 100.00%         | 12.210%       |
| 7         | 6.245       | 1528          | 1541        | 1566         | rBV      | 420542         | 839971        | 69.19%          | 8.448%        |
| 8         | 6.689       | 1664          | 1679        | 1705         | rBV      | 264819         | 550292        | 45.33%          | 5.535%        |
| 9         | 7.563       | 1939          | 1951        | 1976         | rBV      | 130333         | 247378        | 20.38%          | 2.488%        |
| 10        | 7.894       | 2041          | 2054        | 2087         | rBV      | 587325         | 1067687       | 87.95%          | 10.739%       |
| 11        | 8.177       | 2131          | 2142        | 2160         | rBV2     | 75009          | 137694        | 11.34%          | 1.385%        |
| 12        | 8.631       | 2272          | 2283        | 2324         | rBV2     | 468787         | 1026898       | 84.59%          | 10.328%       |
| 13        | 9.415       | 2514          | 2527        | 2552         | rBV      | 586715         | 1043474       | 85.96%          | 10.495%       |
| 14        | 10.753      | 2928          | 2943        | 2966         | rBV      | 187953         | 308493        | 25.41%          | 3.103%        |
| 15        | 11.811      | 3260          | 3272        | 3300         | rBV      | 579608         | 985520        | 81.18%          | 9.912%        |
| 16        | 12.190      | 3375          | 3390        | 3415         | rBV      | 502127         | 858999        | 70.76%          | 8.640%        |




Sum of corrected areas: 9942398

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU102723\  
Data File : VU055936.D  
Acq On : 27 Oct 2023 21:39  
Operator : MD/SY  
Sample : VU1027WBL02  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102423WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

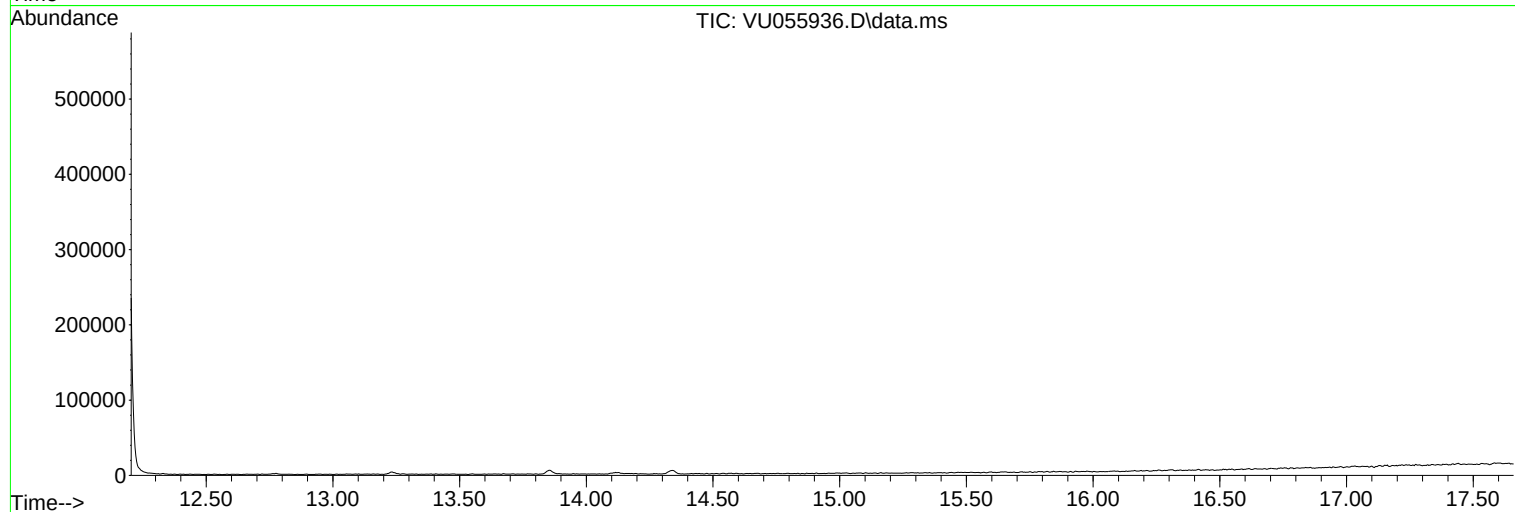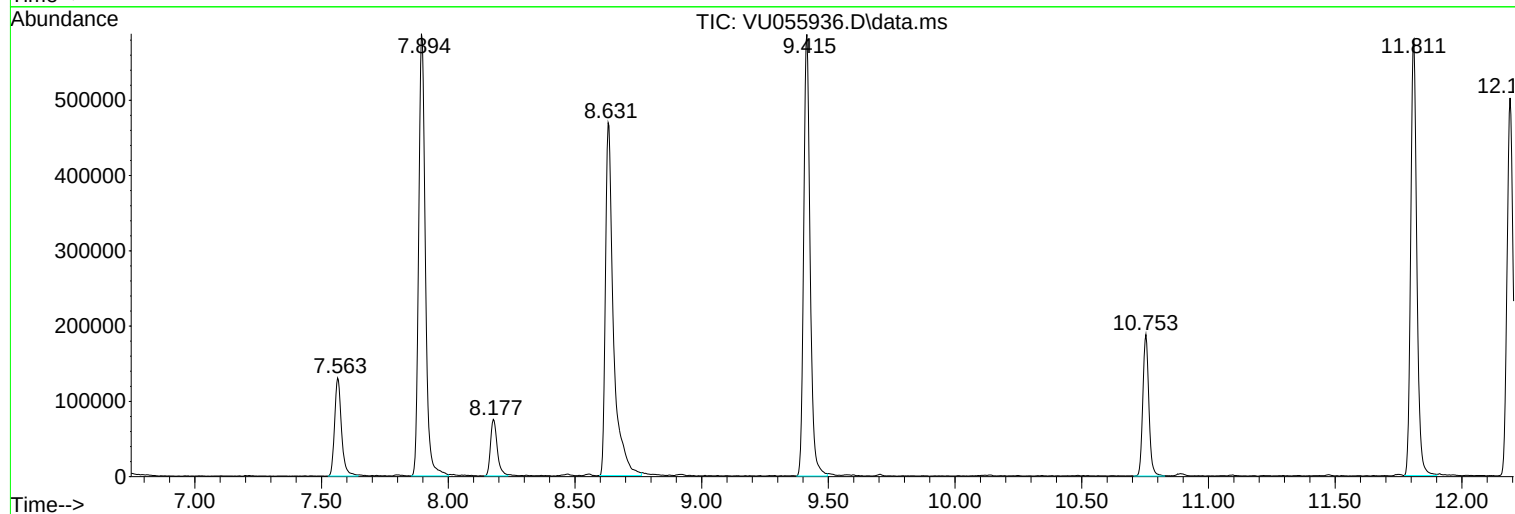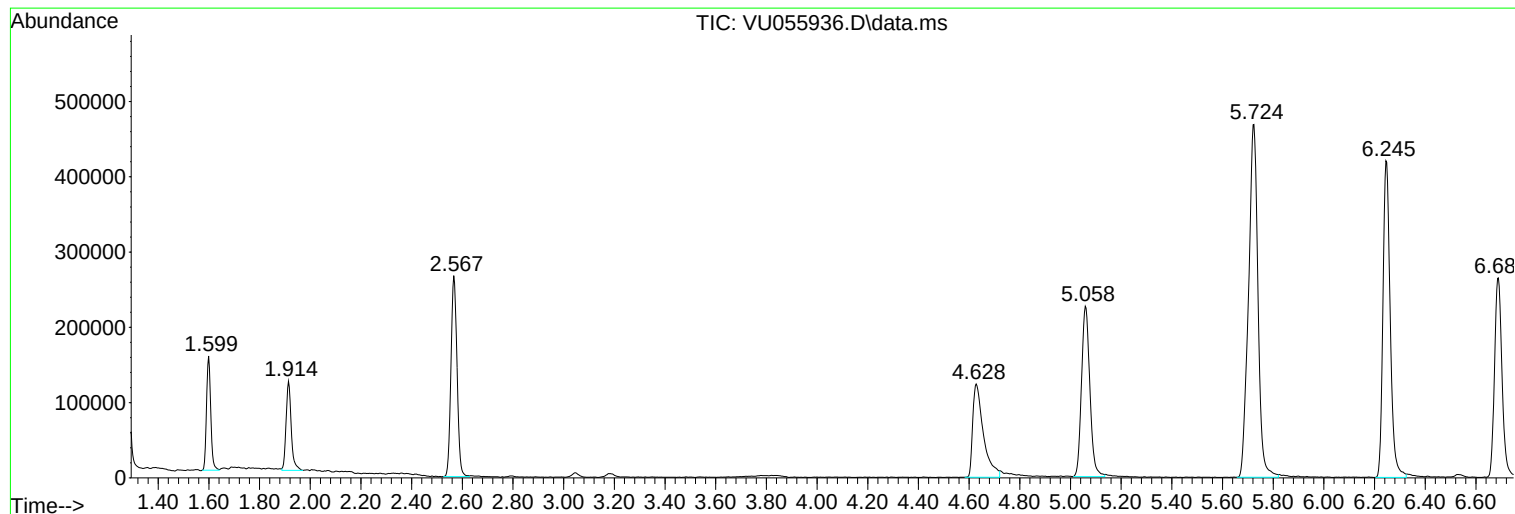

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU102723\  
Data File : VU055936.D  
Acq On : 27 Oct 2023 21:39  
Operator : MD/SY  
Sample : VU1027WBL02  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102423WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU102723\  
Data File : VU055936.D  
Acq On : 27 Oct 2023 21:39  
Operator : MD/SY  
Sample : VU1027WBL02  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102423WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|