

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055937.D
 Acq On : 27 Oct 2023 22:03
 Operator : MD/SY
 Sample : 04995-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A49C5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	110	rBV	96775	115051	8.99%	1.249%
2	1.914	186	194	209	rVB	87302	120248	9.39%	1.305%
3	2.566	385	397	411	rBV	164204	272851	21.32%	2.962%
4	3.181	577	588	600	rBV	7396	16595	1.30%	0.180%
5	4.627	1023	1038	1080	rBV	164834	512542	40.04%	5.564%
6	5.062	1156	1173	1203	rVB	198190	466616	36.46%	5.065%
7	5.724	1357	1379	1409	rBV2	354056	952264	74.40%	10.337%
8	6.248	1528	1542	1566	rBV	412029	825529	64.50%	8.961%
9	6.541	1623	1633	1647	rVB8	5939	13381	1.05%	0.145%
10	6.689	1664	1679	1700	rBV	230443	469038	36.65%	5.092%
11	7.563	1937	1951	1967	rBV	104312	193591	15.12%	2.101%
12	7.897	2041	2055	2072	rBV	387920	714679	55.84%	7.758%
13	7.965	2073	2076	2092	rVB	11521	20234	1.58%	0.220%
14	8.177	2131	2142	2164	rBV2	60554	114954	8.98%	1.248%
15	8.631	2272	2283	2325	rBV2	572077	1279946	100.00%	13.894%
16	9.415	2514	2527	2564	rBV	580044	1026379	80.19%	11.142%
17	10.753	2930	2943	2964	rBV	203814	337566	26.37%	3.664%
18	10.888	2975	2985	3000	rVB4	7527	14378	1.12%	0.156%
19	11.810	3260	3272	3289	rBV	576949	968817	75.69%	10.517%
20	12.077	3344	3355	3377	rBV4	12842	37796	2.95%	0.410%
21	12.190	3377	3390	3414	rVB	430297	739656	57.79%	8.029%




Sum of corrected areas: 9212111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055937.D
Acq On : 27 Oct 2023 22:03
Operator : MD/SY
Sample : 04995-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

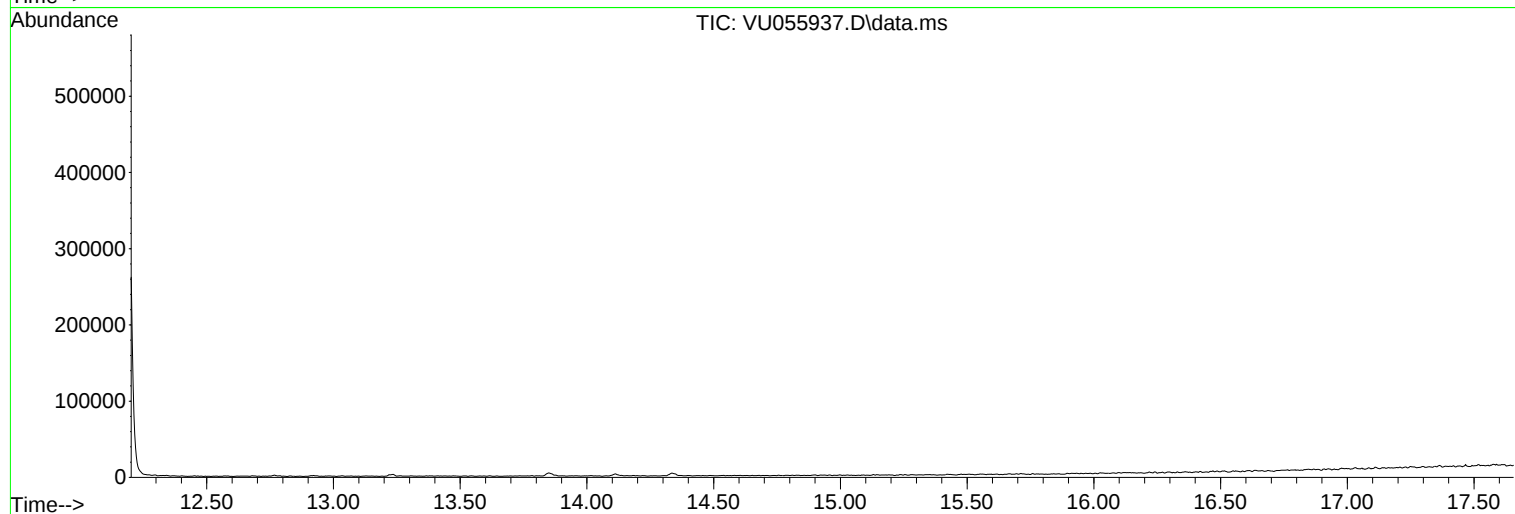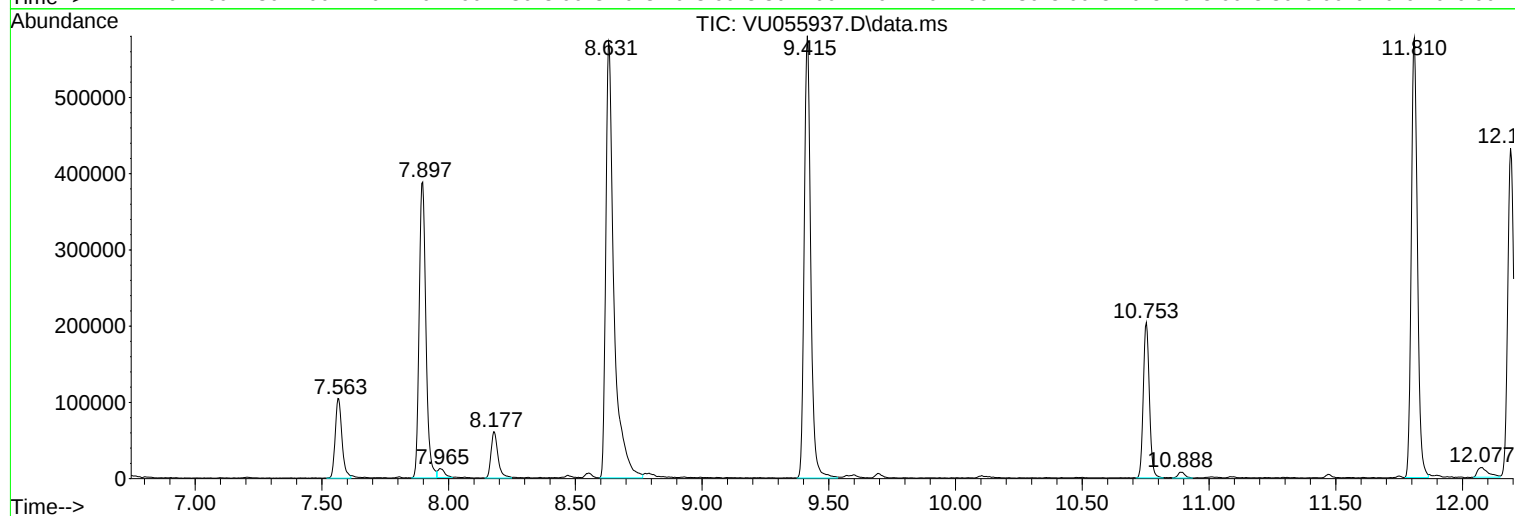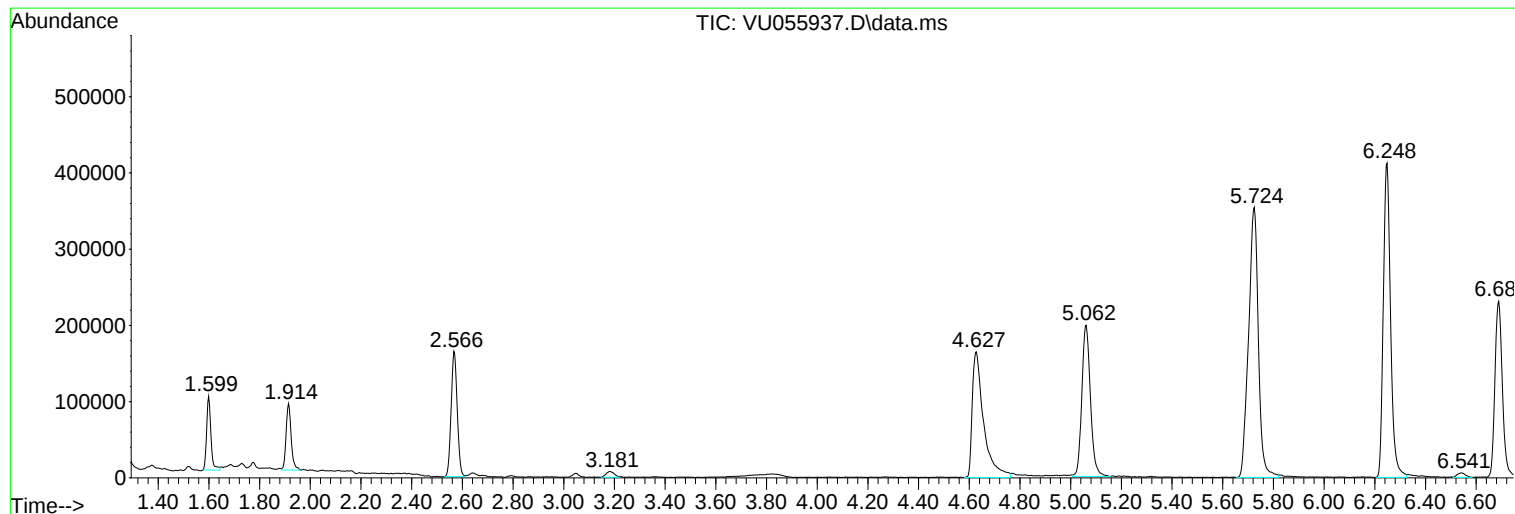

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055937.D
Acq On : 27 Oct 2023 22:03
Operator : MD/SY
Sample : 04995-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055937.D
Acq On : 27 Oct 2023 22:03
Operator : MD/SY
Sample : 04995-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc