

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055939.D
 Acq On : 27 Oct 2023 22:52
 Operator : MD/SY
 Sample : 05113-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B38

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	106	rBV	93165	109376	8.33%	1.203%
2	1.914	186	194	211	rVB	79127	111369	8.48%	1.225%
3	2.567	385	397	412	rBV	147311	245895	18.73%	2.705%
4	3.197	576	593	597	rBV2	17795	40500	3.09%	0.445%
5	4.628	1021	1038	1079	rBV	164868	524292	39.94%	5.767%
6	5.058	1155	1172	1201	rVB	188029	429967	32.76%	4.729%
7	5.724	1357	1379	1408	rBV2	336829	908419	69.21%	9.992%
8	6.245	1528	1541	1573	rBV	418373	845086	64.39%	9.295%
9	6.685	1663	1678	1698	rBV	227967	457714	34.87%	5.034%
10	7.563	1940	1951	1976	rBV	99993	189430	14.43%	2.084%
11	7.894	2042	2054	2073	rBV	365398	676425	51.54%	7.440%
12	8.181	2131	2143	2162	rBV2	58322	109727	8.36%	1.207%
13	8.634	2271	2284	2321	rBV2	585367	1312550	100.00%	14.437%
14	8.791	2326	2333	2349	rVB7	10164	21524	1.64%	0.237%
15	9.415	2512	2527	2553	rBV	601290	1052715	80.20%	11.579%
16	10.753	2925	2943	2964	rBV	202051	340381	25.93%	3.744%
17	11.811	3259	3272	3292	rBV	589661	994138	75.74%	10.935%
18	12.190	3378	3390	3413	rBV	414564	705312	53.74%	7.758%
19	12.897	3601	3610	3622	rBV6	8867	16803	1.28%	0.185%




Sum of corrected areas: 9091623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055939.D
Acq On : 27 Oct 2023 22:52
Operator : MD/SY
Sample : 05113-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

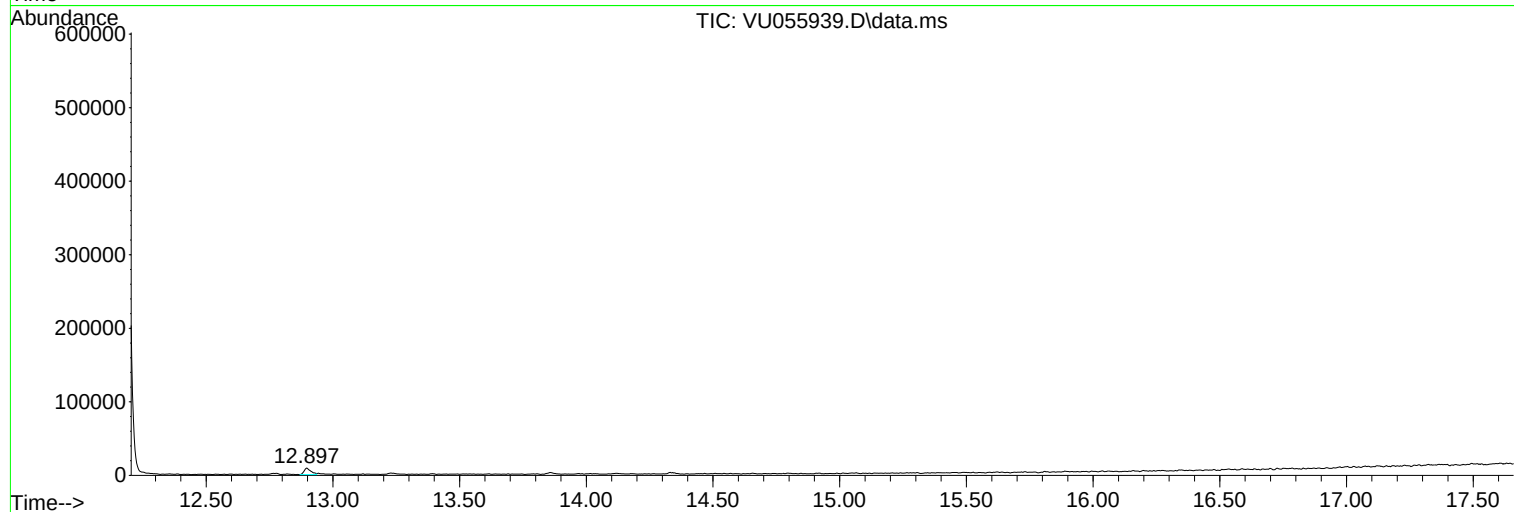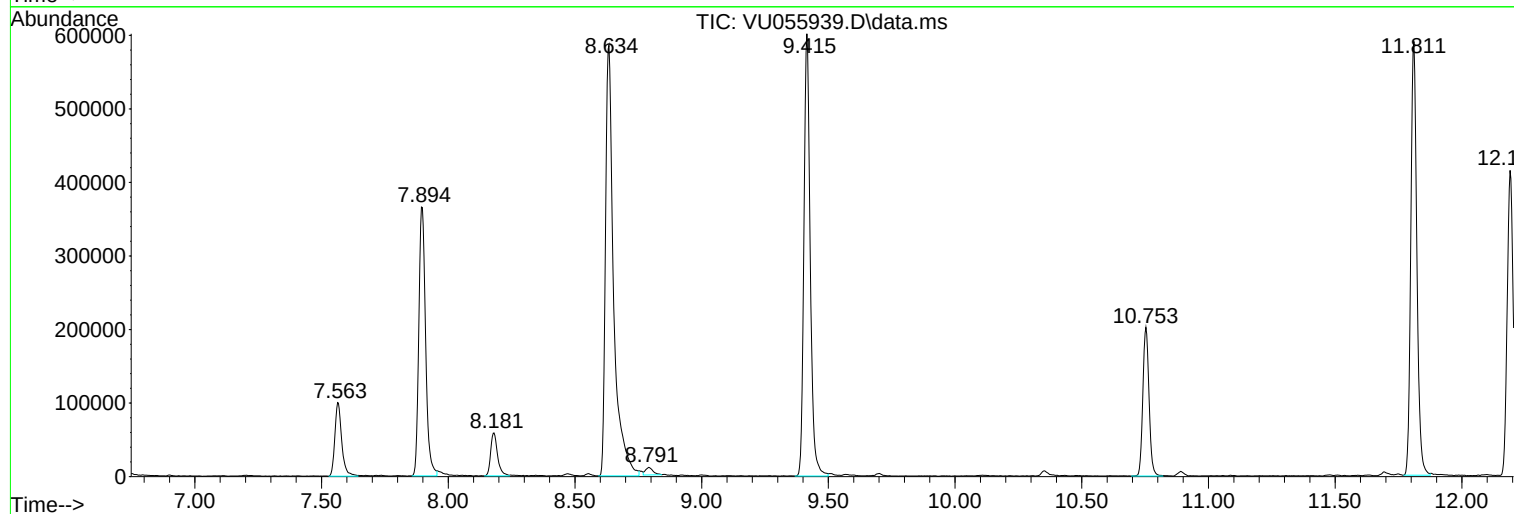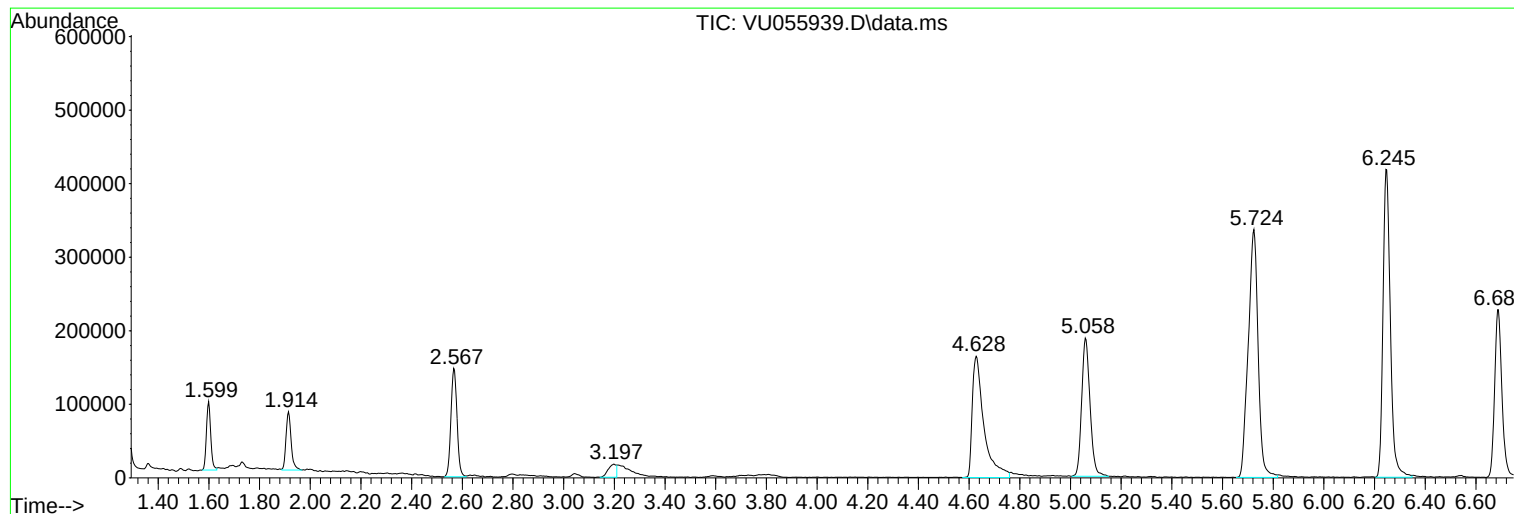

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055939.D
Acq On : 27 Oct 2023 22:52
Operator : MD/SY
Sample : 05113-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B38










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.563	1.12 ug/L	189430	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	33
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	28
3			3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	9
4			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
5			1,3-Cyclohexadiene	80	C6H8	000592-57-4	9

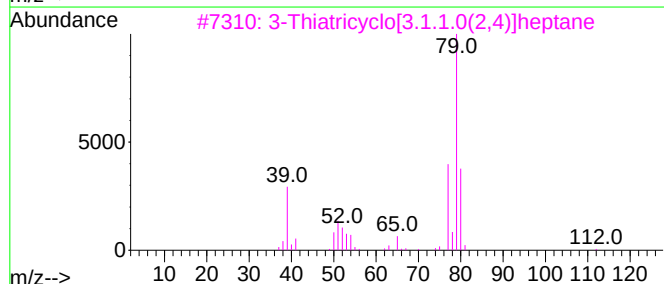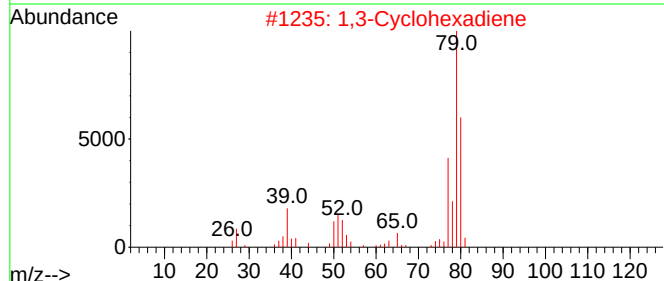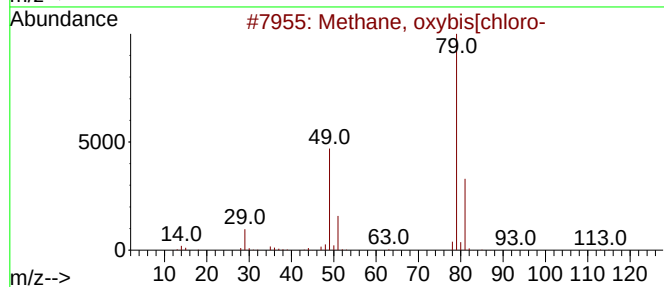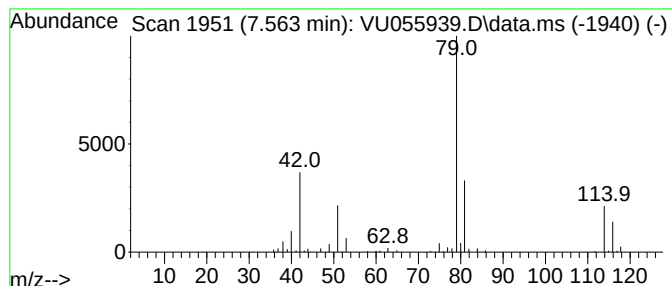

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055939.D
Acq On : 27 Oct 2023 22:52
Operator : MD/SY
Sample : 05113-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.563	1.1	ug/L	189430	1	6.248	845086	5.0