

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055948.D
 Acq On : 28 Oct 2023 02:29
 Operator : MD/SY
 Sample : 05113-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B54

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	32	rBV4	12686	15833	1.18%	0.165%
2	1.599	88	96	109	rVB	92649	109159	8.13%	1.140%
3	1.731	133	137	150	rVB2	11207	13855	1.03%	0.145%
4	1.914	186	194	209	rVB	88638	118977	8.86%	1.242%
5	2.567	381	397	412	rBV	156476	260581	19.40%	2.721%
6	2.801	456	470	476	rBV3	6391	14792	1.10%	0.154%
7	3.187	571	590	624	rBV3	37833	143612	10.69%	1.500%
8	4.628	1015	1038	1089	rBV2	202804	666249	49.60%	6.957%
9	5.062	1157	1173	1194	rBV	192065	437985	32.61%	4.573%
10	5.724	1359	1379	1414	rBV2	346526	951869	70.86%	9.939%
11	6.248	1526	1542	1573	rBV	426292	846297	63.00%	8.837%
12	6.689	1664	1679	1701	rBV	234568	475780	35.42%	4.968%
13	7.563	1939	1951	1987	rBV	101716	194383	14.47%	2.030%
14	7.897	2041	2055	2072	rBV	386554	703109	52.34%	7.342%
15	8.180	2130	2143	2161	rBV3	58146	108735	8.09%	1.135%
16	8.550	2248	2258	2272	rVB3	31154	53499	3.98%	0.559%
17	8.634	2272	2284	2328	rBV3	597126	1343305	100.00%	14.026%
18	9.415	2511	2527	2556	rBV	599211	1060601	78.95%	11.074%
19	10.753	2930	2943	2967	rVB	206567	343106	25.54%	3.583%
20	11.811	3259	3272	3294	rBV	586742	985162	73.34%	10.287%
21	12.190	3377	3390	3416	rBV	419253	730183	54.36%	7.624%




Sum of corrected areas: 9577072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055948.D
Acq On : 28 Oct 2023 02:29
Operator : MD/SY
Sample : 05113-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

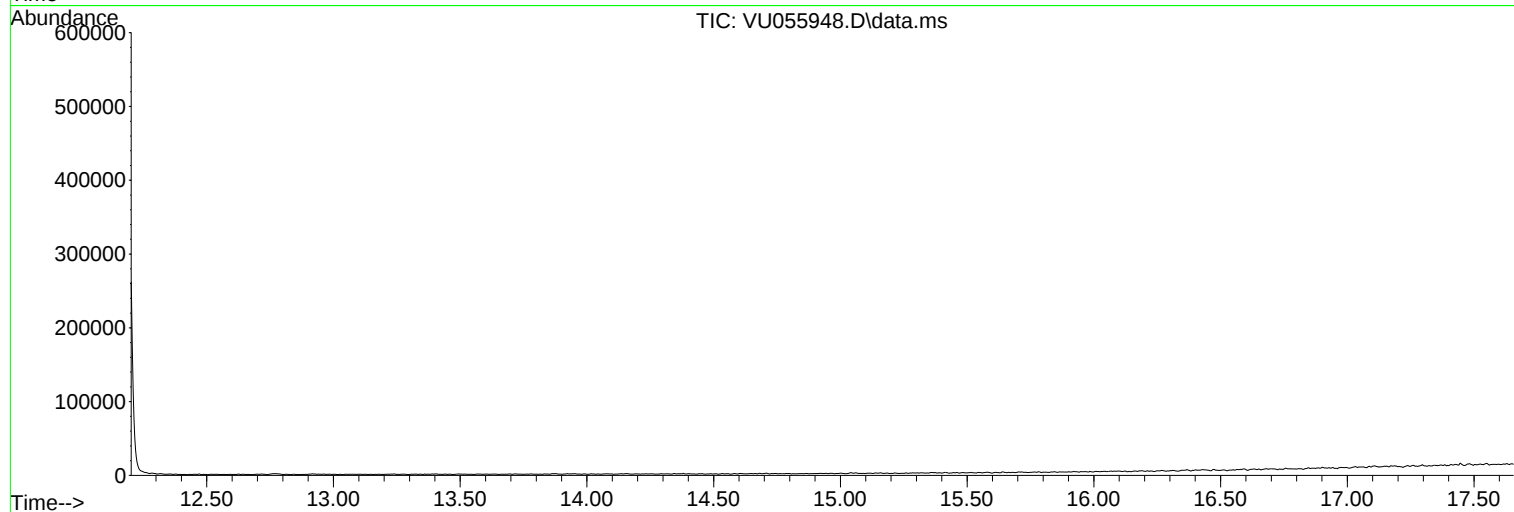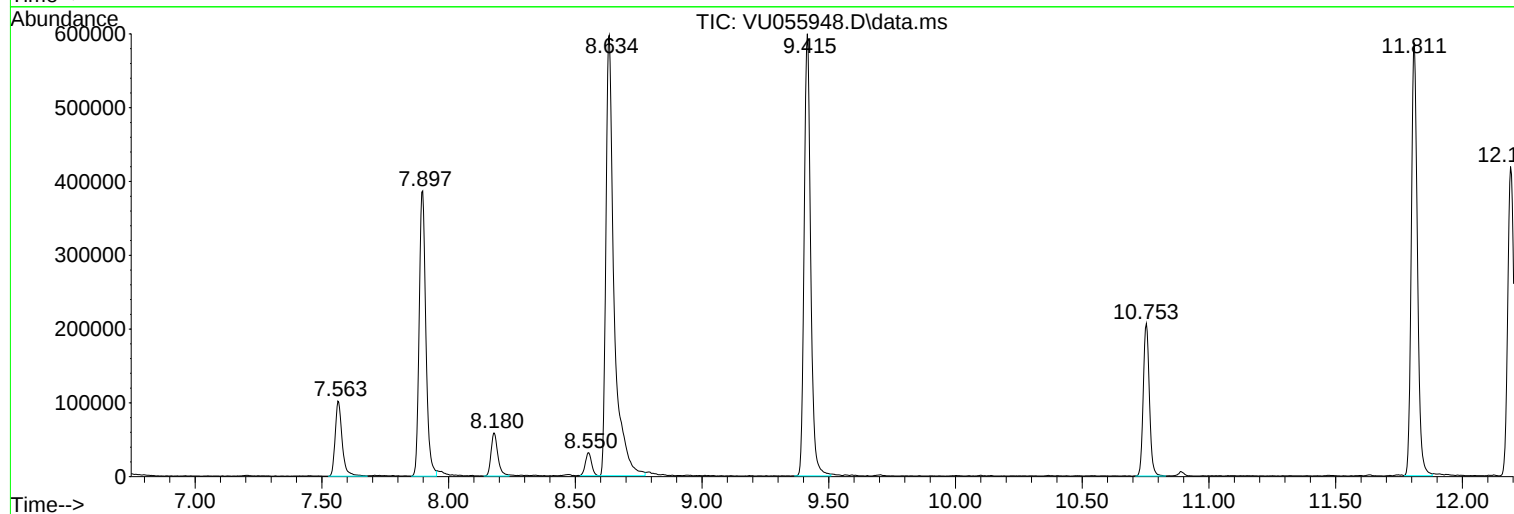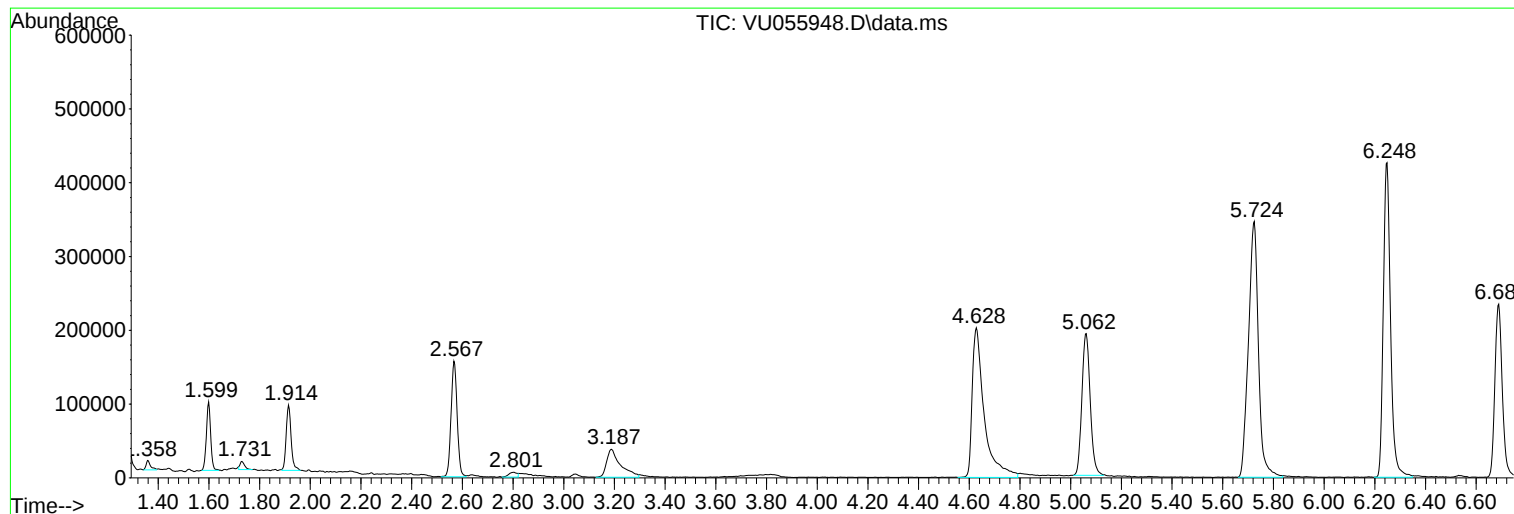

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055948.D
Acq On : 28 Oct 2023 02:29
Operator : MD/SY
Sample : 05113-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055948.D
Acq On : 28 Oct 2023 02:29
Operator : MD/SY
Sample : 05113-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc