

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
 Data File : VU055957.D
 Acq On : 28 Oct 2023 06:07
 Operator : MD/SY
 Sample : 05103-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A49Y7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	81	rVB	14347	16133	1.24%	0.180%
2	1.599	89	96	107	rBV	92271	101042	7.77%	1.125%
3	1.914	186	194	206	rBV	81224	110081	8.46%	1.226%
4	2.566	386	397	411	rBV	153594	251714	19.35%	2.804%
5	3.187	573	590	603	rBV	11700	26143	2.01%	0.291%
6	4.627	1024	1038	1082	rBV	166976	538950	41.43%	6.003%
7	5.058	1156	1172	1194	rBV	190611	434517	33.40%	4.840%
8	5.724	1353	1379	1406	rBV2	337439	918381	70.60%	10.229%
9	6.248	1528	1542	1566	rBV	402435	795217	61.13%	8.857%
10	6.688	1665	1679	1705	rBV	228110	460341	35.39%	5.127%
11	7.566	1939	1952	1972	rBV2	97678	182557	14.03%	2.033%
12	7.897	2042	2055	2072	rBV	375248	682769	52.49%	7.605%
13	8.180	2128	2143	2159	rBV	57547	105674	8.12%	1.177%
14	8.553	2250	2259	2271	rBV4	14179	25698	1.98%	0.286%
15	8.634	2271	2284	2325	rBV3	578730	1300793	100.00%	14.489%
16	9.415	2514	2527	2559	rBV	572546	998264	76.74%	11.119%
17	10.753	2931	2943	2966	rBV	202125	339498	26.10%	3.781%
18	11.810	3258	3272	3292	rBV	564506	935006	71.88%	10.414%
19	12.074	3343	3354	3366	rBV2	15103	37076	2.85%	0.413%
20	12.190	3378	3390	3418	rVB	421730	718212	55.21%	8.000%




Sum of corrected areas: 8978066

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055957.D
Acq On : 28 Oct 2023 06:07
Operator : MD/SY
Sample : 05103-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

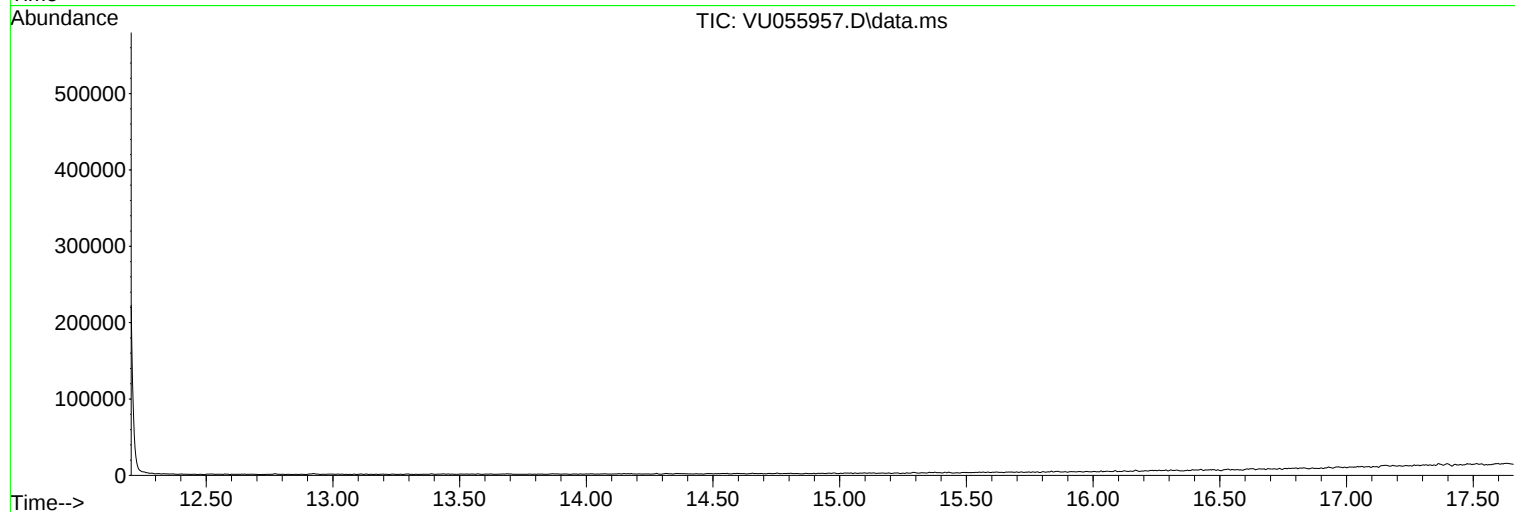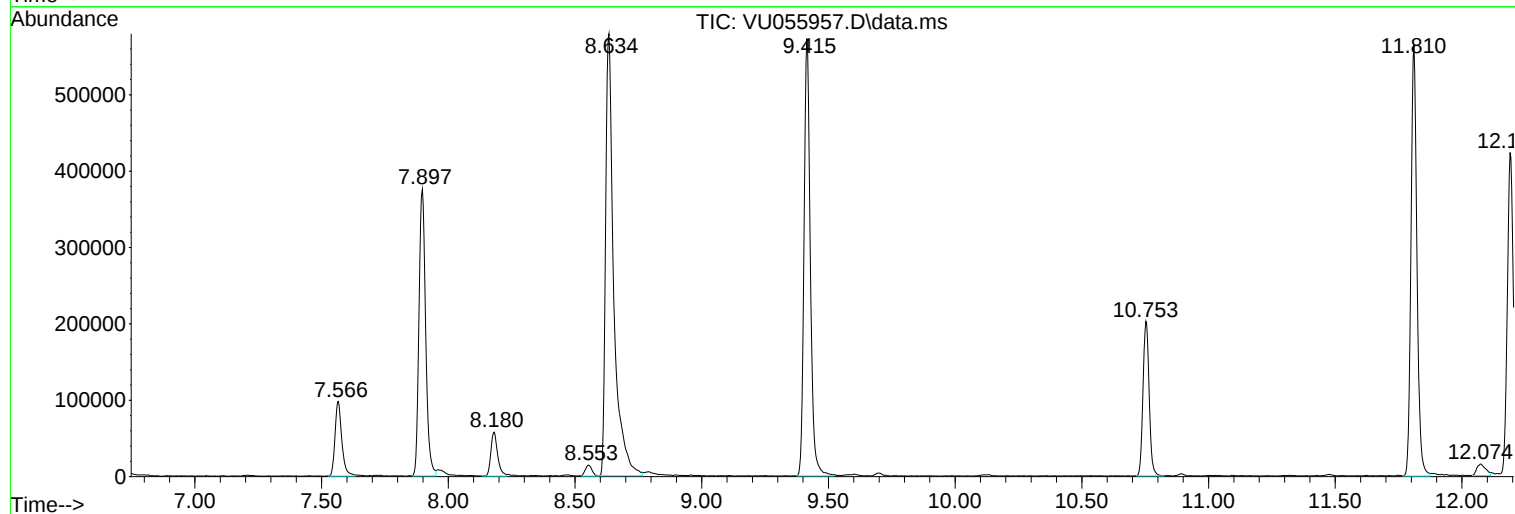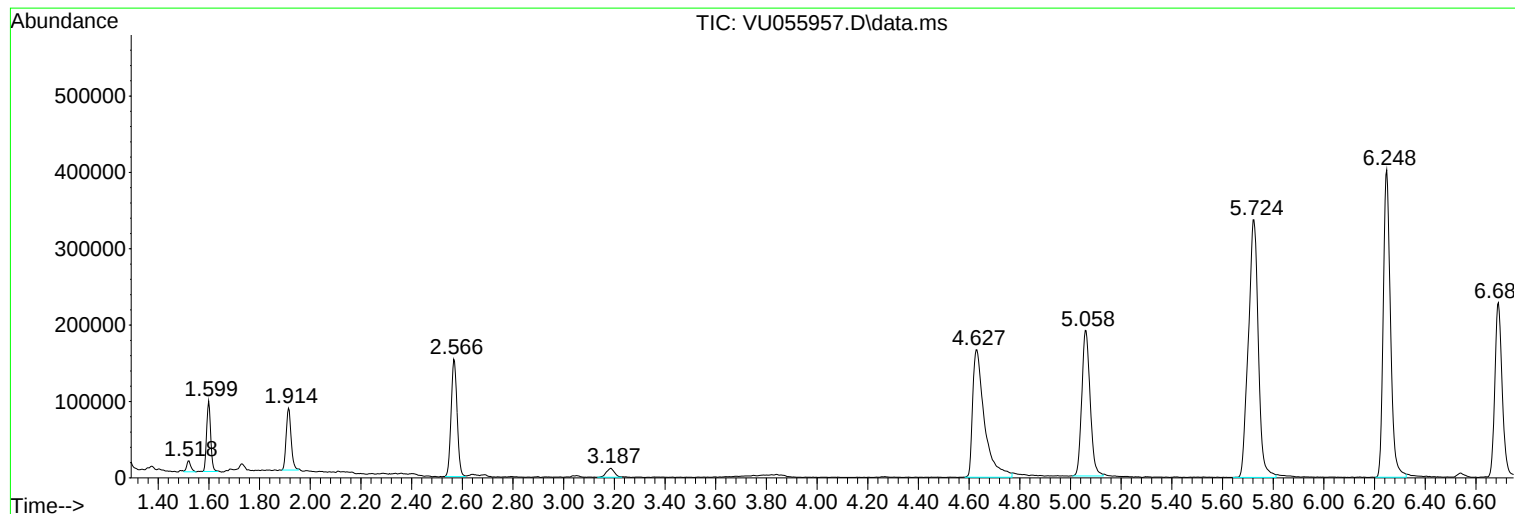

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055957.D
Acq On : 28 Oct 2023 06:07
Operator : MD/SY
Sample : 05103-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055957.D
Acq On : 28 Oct 2023 06:07
Operator : MD/SY
Sample : 05103-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A49Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
