


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102723\
Data File : VU055915.D
Acq On : 27 Oct 2023 08:34
Operator : MD/SY
Sample : BFB059
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB059

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 31 05:28:08 2023

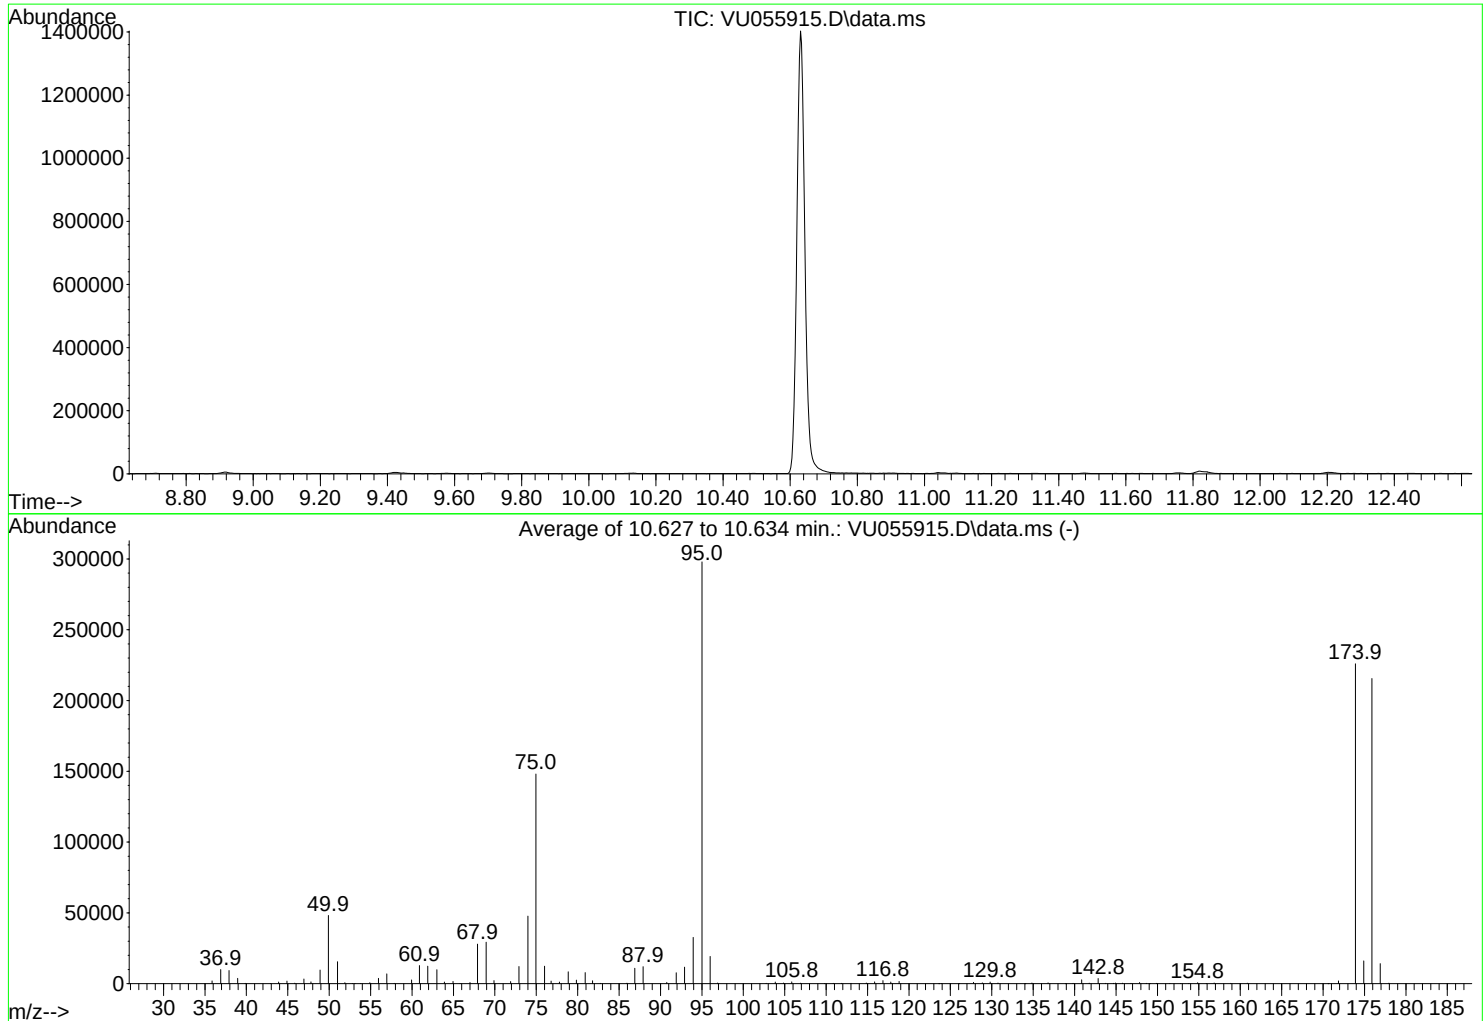

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	48173	PASS
75	95	30	80	49.7	148053	PASS
95	95	100	100	100.0	297984	PASS
96	95	5	9	6.4	19195	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.8	225984	PASS
175	174	5	9	7.1	16111	PASS
176	174	95	101	95.4	215616	PASS
177	176	5	9	6.6	14140	PASS

m/z	Abundance
39.80	359.0
43.90	727.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.80	1942.0
36.90	10052.0
37.90	8853.0
38.90	3697.0
39.90	603.0
42.80	186.0
43.90	1849.0
44.90	1813.0
45.80	213.0
46.90	3415.0
47.70	1184.0
48.90	9853.0
49.90	47288.0
51.00	14677.0
51.90	674.0
53.80	124.0
54.90	681.0
55.90	3502.0
57.00	6989.0
57.80	268.0
60.00	2700.0
60.90	12648.0
61.90	12337.0
63.00	9958.0
63.90	1102.0
64.90	1576.0
65.80	153.0
67.00	706.0
67.90	26792.0
68.90	28328.0
69.90	2079.0
71.90	1487.0
72.90	11555.0
74.00	46360.0
75.00	145280.0
76.00	12875.0
76.80	1878.0
77.80	1100.0
78.80	8105.0
79.90	2588.0
80.90	7491.0
81.80	1923.0
82.80	230.0
86.00	407.0
86.90	10551.0
87.90	11360.0
90.70	982.0
91.90	7458.0
92.90	11827.0
94.00	32016.0
95.00	289728.0
96.00	18368.0
96.90	374.0
102.80	205.0
103.80	1074.0
104.90	410.0
105.80	1114.0
106.90	321.0
109.80	154.0
110.80	239.0
111.80	230.0
113.00	195.0
114.80	441.0
115.90	1199.0
116.90	2196.0
117.80	994.0
118.80	1578.0
123.60	120.0
124.00	123.0
126.00	112.0
127.80	865.0
128.90	593.0
129.80	1068.0
130.80	398.0
134.90	519.0
136.80	561.0
139.80	189.0
140.90	2358.0
141.70	271.0
142.90	3521.0
143.70	183.0
144.70	572.0
145.90	342.0
146.80	292.0
147.80	820.0
148.60	177.0
149.00	130.0
149.90	270.0
151.50	115.0
152.70	129.0
153.80	125.0
154.90	732.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

155.90	112.0
156.80	506.0
158.90	247.0
160.90	309.0
171.90	1928.0
173.90	214080.0
174.90	15149.0
175.90	205952.0
176.90	13350.0
177.90	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.80	1971.0
36.90	10265.0
37.90	9544.0
38.90	3766.0
39.90	546.0
42.90	160.0
43.90	1937.0
44.90	1889.0
45.90	336.0
46.90	3436.0
47.80	1230.0
48.90	9961.0
49.90	49784.0
51.00	16064.0
51.90	713.0
52.80	128.0
53.10	122.0
53.80	125.0
54.90	693.0
55.90	3909.0
56.90	7044.0
57.80	256.0
59.90	2793.0
60.90	13128.0
61.90	12546.0
63.00	10042.0
63.90	1257.0
65.00	1687.0
65.80	164.0
67.00	816.0
67.90	28800.0
69.00	30336.0
69.90	2232.0
71.90	1572.0
72.90	12516.0
74.00	49328.0
75.00	152640.0
76.00	12628.0
76.80	1925.0
77.80	1203.0
78.80	8579.0
79.90	2610.0
80.90	7953.0
81.80	2119.0
82.80	257.0
86.00	409.0
86.90	11235.0
87.90	12558.0
90.80	980.0
91.90	7928.0
92.90	11891.0
94.00	33464.0
95.00	307072.0
96.00	19800.0
96.90	442.0
102.70	184.0
103.80	1141.0
104.80	396.0
105.80	1320.0
106.90	411.0
109.80	136.0
110.90	256.0
111.90	202.0
113.00	214.0
114.90	417.0
115.90	1213.0
116.80	2232.0
117.80	1222.0
118.80	1712.0
123.90	158.0
127.80	942.0
128.80	629.0
129.80	1195.0
130.70	434.0
134.80	501.0
136.80	639.0
139.80	209.0
140.80	2704.0
141.70	346.0
142.90	3729.0
143.80	235.0
144.90	614.0
145.80	351.0
146.80	249.0
147.90	766.0
148.70	193.0
149.90	270.0
151.50	117.0
152.80	152.0
153.80	157.0
154.90	755.0
155.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

156.90	562.0
158.80	247.0
160.80	321.0
171.90	2072.0
173.90	232704.0
174.90	16552.0
175.90	222336.0
176.90	14567.0
177.90	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	1750.0
36.90	9686.0
37.90	9422.0
39.00	3740.0
39.90	460.0
43.00	157.0
43.90	1774.0
44.90	1716.0
45.90	406.0
47.00	2916.0
47.90	1338.0
48.90	9121.0
49.90	47448.0
51.00	15620.0
51.90	617.0
52.80	136.0
53.10	130.0
54.90	693.0
56.00	3796.0
56.90	6616.0
57.90	228.0
59.90	2463.0
60.90	12633.0
61.90	12174.0
63.00	9459.0
63.90	1239.0
65.00	1653.0
65.80	160.0
67.00	834.0
67.90	28248.0
69.00	29168.0
69.90	2276.0
71.90	1515.0
72.90	12238.0
74.00	47592.0
74.90	146240.0
76.00	11335.0
76.80	1653.0
77.80	1084.0
78.90	8581.0
79.80	2375.0
80.90	7908.0
81.80	2063.0
82.70	211.0
85.90	366.0
86.90	10666.0
87.90	12219.0
90.80	871.0
91.90	7770.0
92.90	11180.0
93.90	32440.0
95.00	297152.0
96.00	19416.0
96.90	514.0
102.70	143.0
103.90	1107.0
104.80	419.0
105.90	1439.0
106.90	371.0
109.80	149.0
110.80	285.0
111.90	184.0
113.00	207.0
114.90	353.0
115.80	1193.0
116.80	2079.0
117.80	1284.0
118.80	1555.0
123.90	196.0
127.80	955.0
128.80	620.0
129.80	1189.0
130.70	413.0
134.00	102.0
134.80	427.0
136.80	603.0
138.90	126.0
139.80	193.0
140.80	3005.0
141.80	372.0
142.80	3570.0
143.80	264.0
145.00	594.0
145.70	307.0
146.80	195.0
147.90	690.0
148.70	240.0
149.90	286.0
152.90	205.0
153.80	153.0
154.80	689.0
156.90	501.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

158.80	224.0
160.80	279.0
170.60	137.0
171.80	1873.0
173.90	231168.0
174.90	16632.0
175.90	218560.0
176.90	14503.0
178.00	374.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059