


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102819\
 Data File : VU035527.D
 Acq On : 28 Oct 2019 09:14
 Operator : JC/SP
 Sample : BFB28
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB28

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102519WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 30 15:08:45 2019

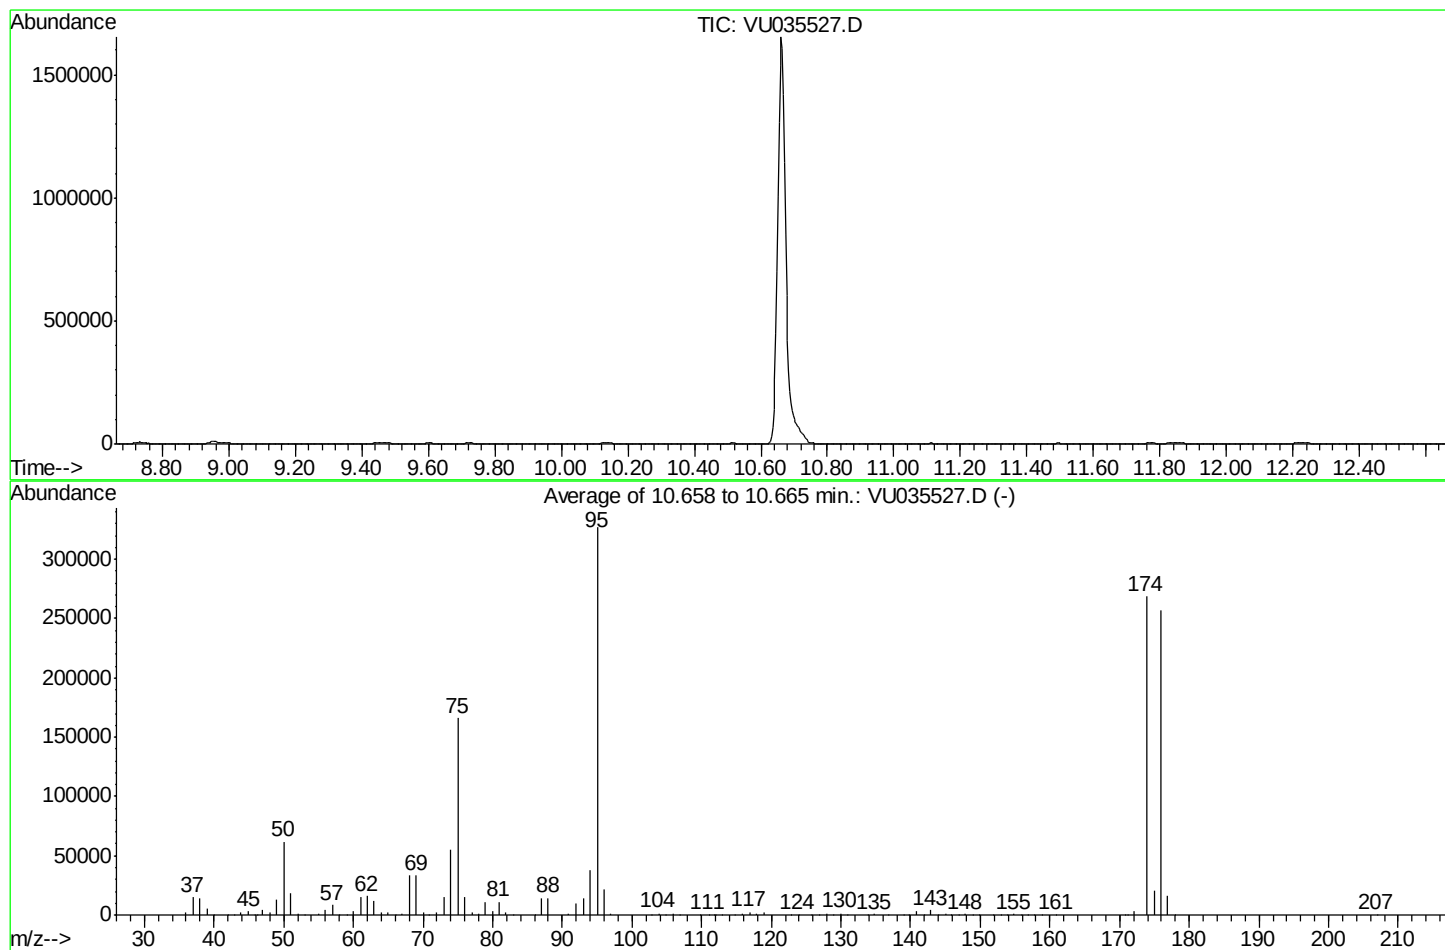

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	61578	PASS
75	95	30	80	50.8	166037	PASS
95	95	100	100	100.0	326976	PASS
96	95	5	9	6.8	22082	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.1	268394	PASS
175	174	5	9	7.5	20133	PASS
176	174	95	101	95.9	257386	PASS
177	176	5	9	6.4	16451	PASS

m/z	Abundance
36.00	2649.0
37.00	14978.0
38.00	13496.0
39.00	5480.0
39.90	416.0
43.10	222.0
43.90	2714.0
45.00	2956.0
45.90	309.0
46.20	287.0
47.00	4795.0
48.00	1979.0
49.00	12989.0
50.00	60312.0
51.00	18000.0
52.10	760.0
53.10	261.0
55.00	857.0
56.00	4765.0
57.00	8064.0
58.10	342.0
60.00	2976.0
61.00	14703.0
62.00	15967.0
63.00	12372.0
64.00	1976.0
65.00	2071.0
66.00	312.0
67.00	835.0
68.00	32504.0
69.00	32592.0
70.00	2334.0
72.00	1753.0
73.00	14600.0
74.00	53488.0
75.00	161152.0
76.00	14451.0
77.00	2269.0
77.90	1208.0
78.90	10359.0
80.00	3239.0
80.90	10601.0
81.90	2709.0
82.90	248.0
86.00	518.0
87.00	14019.0
88.00	14240.0
90.90	1079.0
92.00	9417.0
93.00	12889.0
94.00	36768.0
95.00	314496.0
96.00	21928.0
97.00	670.0
102.80	109.0
103.90	1731.0
104.80	420.0
105.90	1193.0
106.90	374.0
109.70	157.0
111.00	350.0
111.80	247.0
112.00	248.0
112.90	247.0
114.80	245.0
115.90	1161.0
116.90	2291.0
117.90	1305.0
118.90	1696.0
122.90	137.0
123.90	169.0
125.90	173.0
126.80	122.0
127.90	962.0
128.80	383.0
129.90	1063.0
130.80	369.0
133.80	105.0
134.80	567.0
136.80	415.0
138.90	185.0
140.90	3144.0
141.80	468.0
142.90	3812.0
143.90	335.0
145.00	982.0
145.80	367.0
146.90	147.0
147.90	764.0
148.90	207.0
149.80	222.0
151.80	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

152.90	218.0
153.80	301.0
154.80	661.0
155.80	182.0
156.90	560.0
157.80	121.0
158.80	339.0
160.90	387.0
171.10	302.0
172.00	2806.0
173.90	253248.0
174.90	19256.0
175.90	242560.0
176.90	16063.0
177.90	542.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	2712.0
37.00	15529.0
38.00	14149.0
39.00	5614.0
39.90	431.0
41.90	129.0
42.90	198.0
44.00	2835.0
45.00	2972.0
46.10	360.0
47.00	5069.0
48.00	1959.0
49.00	13317.0
50.00	63384.0
51.00	19096.0
52.10	672.0
53.00	223.0
55.00	959.0
56.00	4956.0
57.00	8506.0
58.00	333.0
59.00	103.0
60.00	3174.0
61.00	15688.0
62.00	16184.0
63.00	12657.0
64.00	1940.0
65.00	1984.0
66.00	309.0
67.00	838.0
68.00	34344.0
69.00	34472.0
70.00	2519.0
70.80	125.0
72.00	1812.0
73.00	15711.0
74.00	56608.0
75.00	171200.0
76.00	15428.0
77.00	2355.0
77.90	1246.0
78.90	11069.0
79.90	3244.0
80.90	11197.0
81.90	2765.0
82.90	328.0
86.00	628.0
87.00	15073.0
88.00	15126.0
90.90	1203.0
92.00	10127.0
93.00	13909.0
94.00	39400.0
95.00	337600.0
96.00	22848.0
97.00	806.0
102.80	119.0
103.90	1692.0
104.80	418.0
105.90	1325.0
106.90	436.0
109.70	163.0
111.00	338.0
111.70	236.0
112.00	223.0
112.90	241.0
114.80	300.0
115.90	1271.0
116.90	2479.0
117.80	1495.0
119.00	1774.0
122.90	134.0
123.90	212.0
125.80	164.0
126.80	107.0
127.90	1011.0
128.80	432.0
129.90	1211.0
130.80	393.0
133.90	139.0
134.80	700.0
136.80	394.0
138.90	147.0
140.90	3308.0
141.80	457.0
142.90	4041.0
143.90	343.0
145.00	949.0
145.90	509.0
146.80	178.0
147.90	830.0
148.90	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

149.70	230.0
151.80	176.0
152.90	235.0
153.80	295.0
154.90	806.0
155.90	243.0
156.90	581.0
157.80	101.0
158.90	368.0
160.90	393.0
170.80	320.0
172.00	2948.0
173.90	277824.0
175.00	20752.0
175.90	265280.0
176.90	16952.0
177.90	566.0
206.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	2577.0
37.00	14393.0
38.00	13646.0
39.00	5341.0
39.90	364.0
41.90	149.0
42.90	200.0
44.00	2759.0
45.00	2683.0
46.10	366.0
47.00	4716.0
48.00	1768.0
49.00	12635.0
50.00	61040.0
51.00	18416.0
52.00	561.0
52.90	184.0
55.00	942.0
56.00	4702.0
57.00	8093.0
57.90	398.0
59.00	111.0
60.00	3075.0
61.00	15242.0
62.00	15094.0
63.00	11732.0
64.00	1598.0
65.00	1739.0
66.00	226.0
67.00	773.0
68.00	32400.0
69.00	32960.0
70.00	2483.0
70.80	123.0
72.00	1801.0
73.00	15166.0
74.00	54224.0
75.00	165760.0
76.00	14955.0
77.00	2122.0
77.90	1265.0
78.90	10740.0
79.90	3064.0
80.90	10633.0
81.90	2685.0
82.90	352.0
86.10	579.0
87.00	14566.0
88.00	14477.0
90.90	1315.0
92.00	9972.0
93.00	13868.0
94.00	38248.0
95.00	328832.0
96.00	21472.0
97.00	731.0
102.80	104.0
103.90	1458.0
104.80	395.0
105.90	1400.0
106.90	401.0
109.80	152.0
111.00	298.0
111.70	224.0
112.90	241.0
114.80	287.0
115.90	1195.0
116.90	2341.0
117.80	1510.0
118.90	1617.0
122.90	109.0
123.90	218.0
125.70	126.0
127.90	992.0
128.90	481.0
129.90	1211.0
130.90	418.0
134.00	142.0
134.90	690.0
136.80	387.0
138.90	112.0
139.70	126.0
140.90	3132.0
141.90	386.0
142.90	3818.0
143.90	272.0
145.00	798.0
145.90	607.0
146.80	230.0
147.90	758.0
148.80	223.0
149.80	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

151.80	178.0
152.90	215.0
153.80	238.0
154.90	927.0
155.90	281.0
156.90	579.0
157.80	122.0
158.90	377.0
160.90	367.0
170.80	370.0
172.00	2578.0
173.90	274112.0
175.00	20392.0
175.90	264320.0
176.90	16340.0
177.90	517.0
206.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Scan 2883 (10.610 min): VU035527.D
BFB28

m/z	Abundance
40.10	175.0
43.00	123.0
43.90	1099.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28